

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030137.D
 Acq On : 03 Mar 2023 13:58
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	61	rBV2	4155	4577	1.06%	0.124%
2	1.281	69	75	94	rVB	56595	64715	14.93%	1.753%
3	1.535	147	154	171	rVB	61726	74463	17.18%	2.016%
4	2.063	307	318	335	rBV	116640	170177	39.26%	4.608%
5	2.455	429	440	453	rBV2	4734	7739	1.79%	0.210%
6	3.851	860	874	913	rBV2	25009	139478	32.18%	3.777%
7	4.265	985	1003	1030	rBV	80671	206802	47.71%	5.600%
8	4.969	1205	1222	1256	rBV3	170552	433449	100.00%	11.738%
9	5.545	1388	1401	1424	rBV	144472	299442	69.08%	8.109%
10	6.002	1527	1543	1570	rBV	101891	217860	50.26%	5.900%
11	6.924	1820	1830	1856	rBV2	40024	77495	17.88%	2.099%
12	7.252	1920	1932	1955	rBV	181370	331995	76.59%	8.991%
13	7.564	2019	2029	2051	rBV	24706	45407	10.48%	1.230%
14	8.040	2164	2177	2216	rBV	188621	389995	89.97%	10.561%
15	8.374	2268	2281	2294	rVB3	6120	10787	2.49%	0.292%
16	8.792	2399	2411	2437	rBV	220384	376353	86.83%	10.192%
17	10.162	2823	2837	2854	rBV	86355	138487	31.95%	3.750%
18	11.194	3147	3158	3181	rBV	240277	365031	84.22%	9.885%
19	11.570	3257	3275	3296	rBV	207281	325093	75.00%	8.804%
20	12.204	3463	3472	3484	rVB2	4459	7377	1.70%	0.200%
21	13.998	4015	4030	4039	rBV2	3307	5999	1.38%	0.162%




Sum of corrected areas: 3692721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030137.D
Acq On : 03 Mar 2023 13:58
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

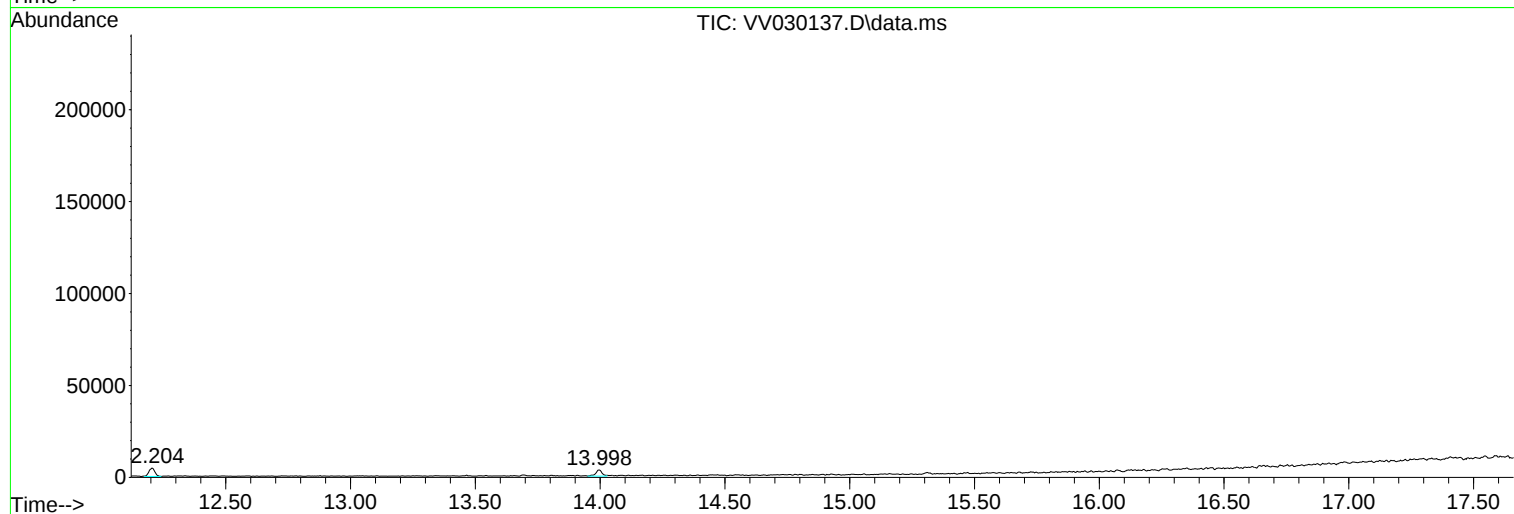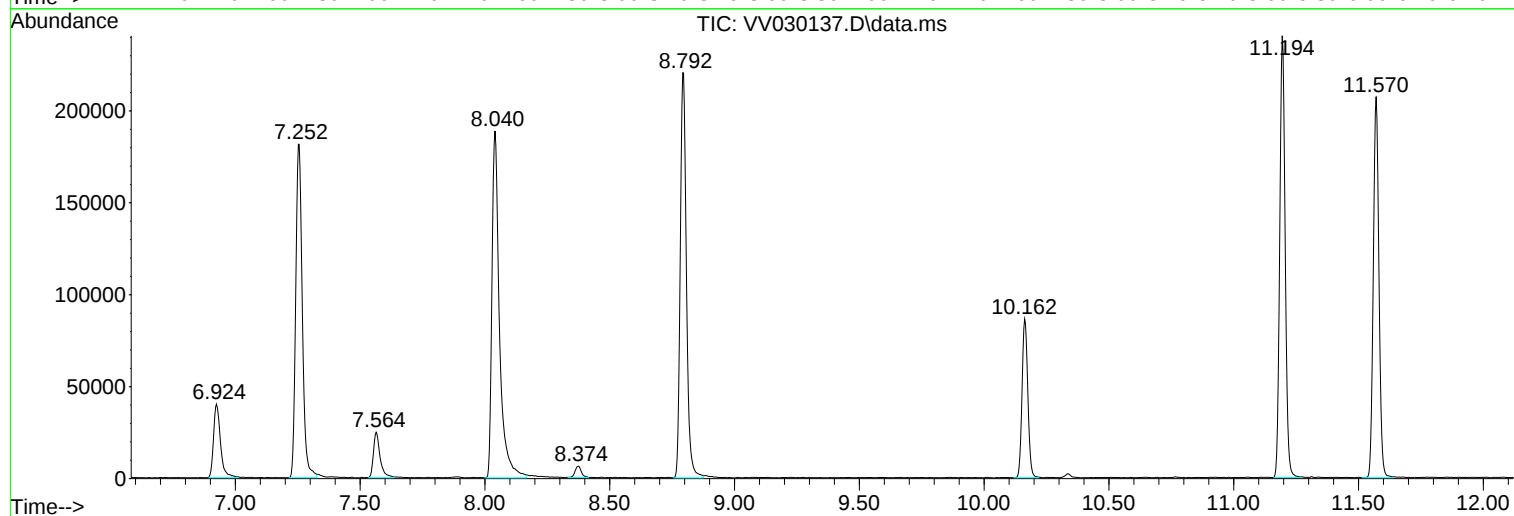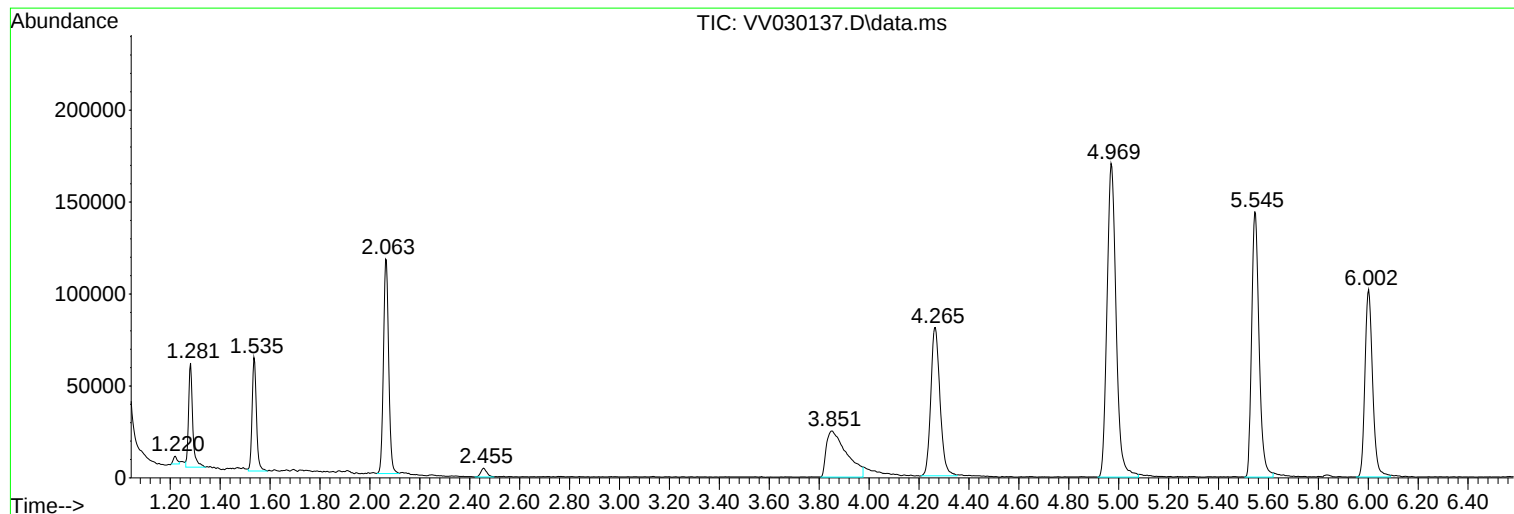

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030137.D
Acq On : 03 Mar 2023 13:58
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030137.D
Acq On : 03 Mar 2023 13:58
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------