

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
 Data File : VV030140.D
 Acq On : 03 Mar 2023 16:42
 Operator : SY/MD
 Sample : 01769-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	62	rBV2	5858	6530	1.55%	0.181%
2	1.282	68	75	95	rVB	55499	66979	15.87%	1.859%
3	1.536	146	154	169	rVB	63149	74368	17.62%	2.064%
4	2.063	308	318	334	rBV	116949	168667	39.95%	4.681%
5	2.455	430	440	455	rBV	10320	16972	4.02%	0.471%
6	2.976	589	602	614	rVB5	2846	5953	1.41%	0.165%
7	3.847	858	873	900	rBV2	21087	101460	24.03%	2.816%
8	4.259	984	1001	1030	rBV	78270	201890	47.82%	5.603%
9	4.970	1205	1222	1249	rBV3	164515	422157	100.00%	11.716%
10	5.542	1386	1400	1429	rBV	148656	310205	73.48%	8.609%
11	5.998	1528	1542	1565	rBV	100911	211661	50.14%	5.874%
12	6.921	1819	1829	1860	rVB	38554	75082	17.79%	2.084%
13	7.252	1919	1932	1956	rBV	184148	328259	77.76%	9.110%
14	7.564	2018	2029	2045	rBV	23092	42090	9.97%	1.168%
15	8.037	2166	2176	2208	rBV	171974	365784	86.65%	10.152%
16	8.793	2400	2411	2432	rBV	231000	381754	90.43%	10.595%
17	10.162	2826	2837	2856	rVB	84052	132964	31.50%	3.690%
18	11.194	3147	3158	3173	rBV	239082	367868	87.14%	10.210%
19	11.571	3264	3275	3292	rBV	198097	310720	73.60%	8.623%
20	12.204	3461	3472	3481	rBV2	5003	7465	1.77%	0.207%
21	13.995	4021	4029	4040	rVB	2899	4353	1.03%	0.121%




Sum of corrected areas: 3603181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030140.D
Acq On : 03 Mar 2023 16:42
Operator : SY/MD
Sample : 01769-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

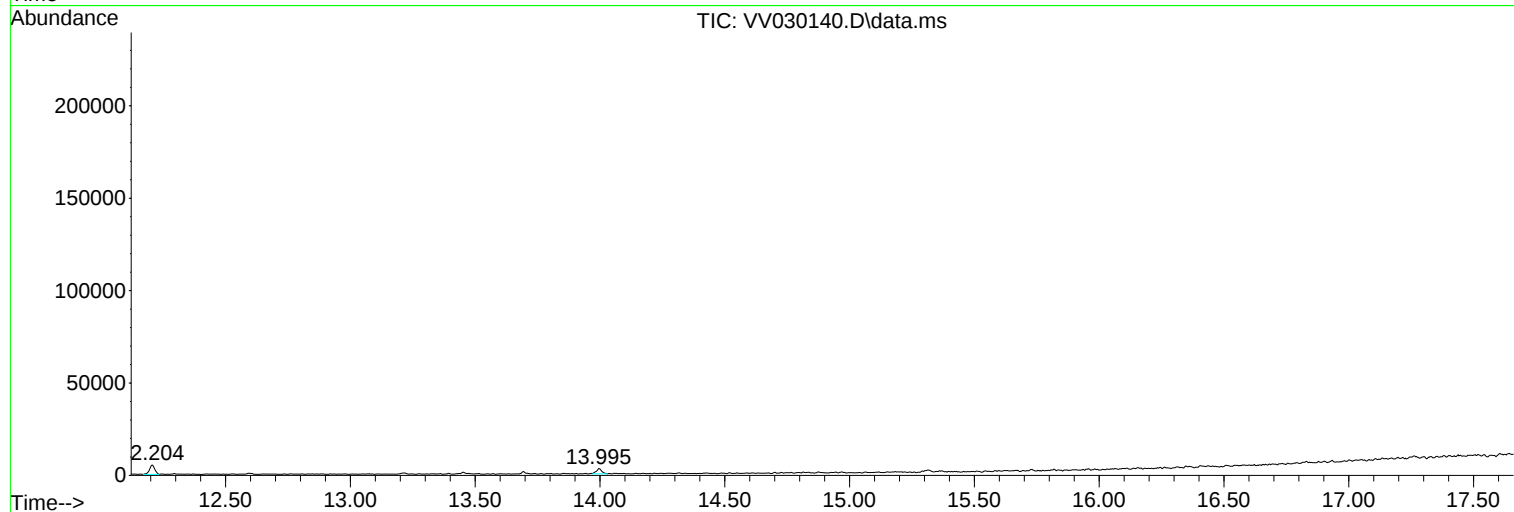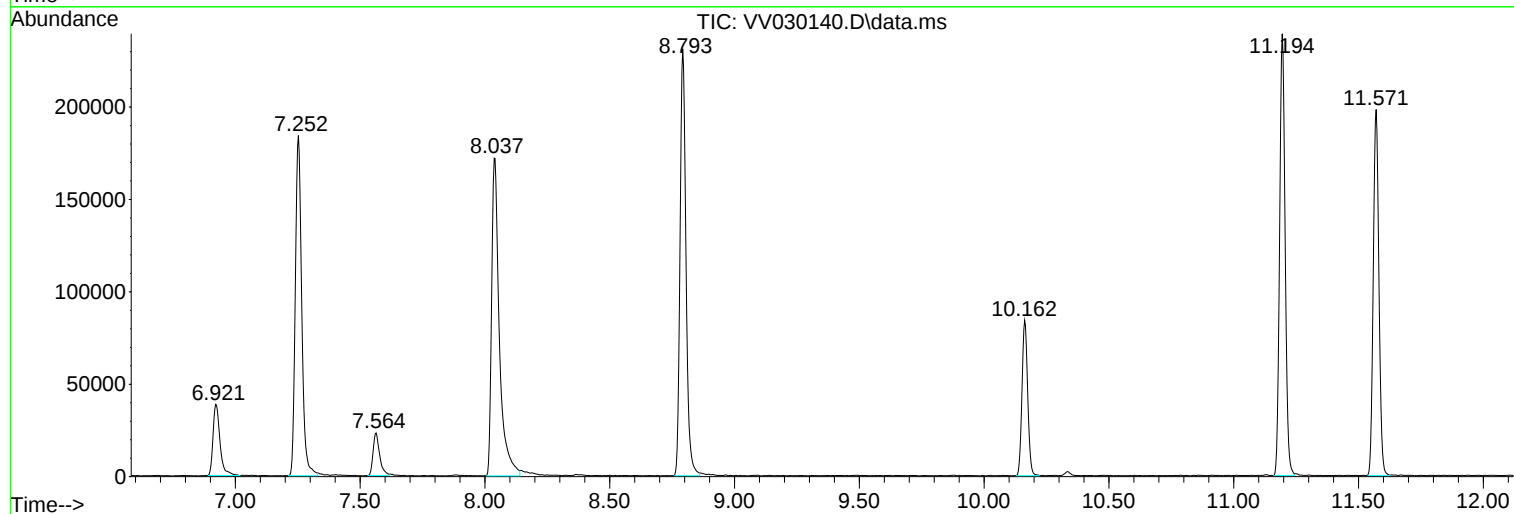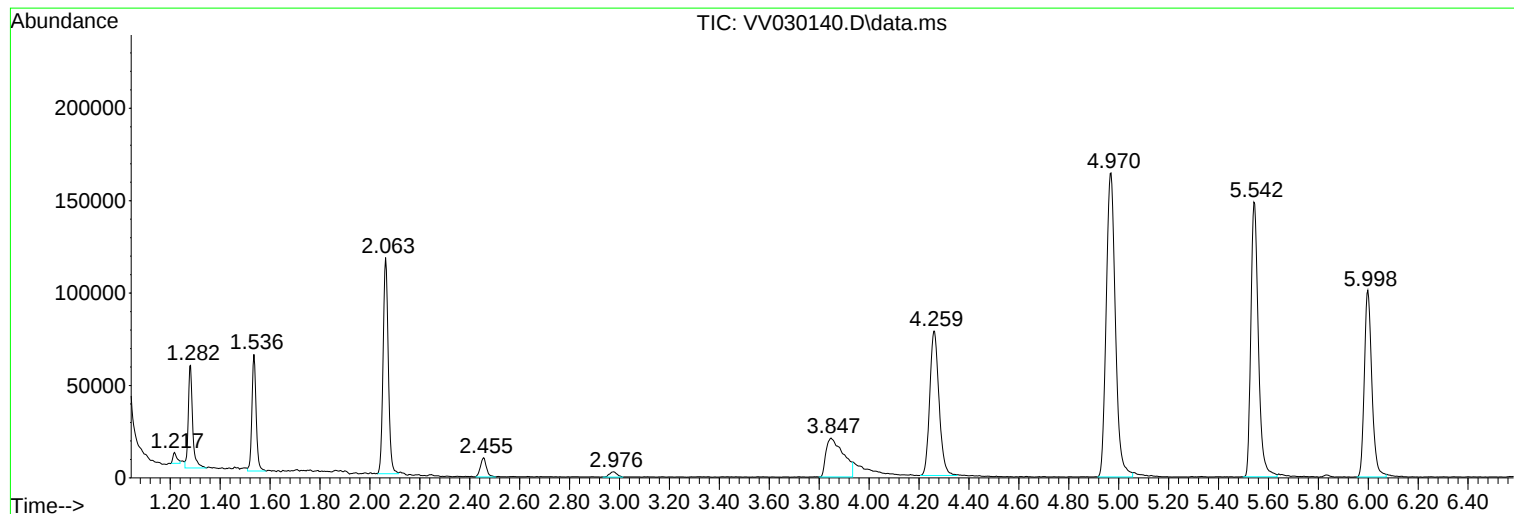

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030140.D
Acq On : 03 Mar 2023 16:42
Operator : SY/MD
Sample : 01769-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030323\
Data File : VV030140.D
Acq On : 03 Mar 2023 16:42
Operator : SY/MD
Sample : 01769-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc