


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030419\
Data File : VV009464.D
Acq On : 04 Mar 2019 10:09
Operator : SY/MD
Sample : BFB71
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022819WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Mar 02 00:06:51 2019

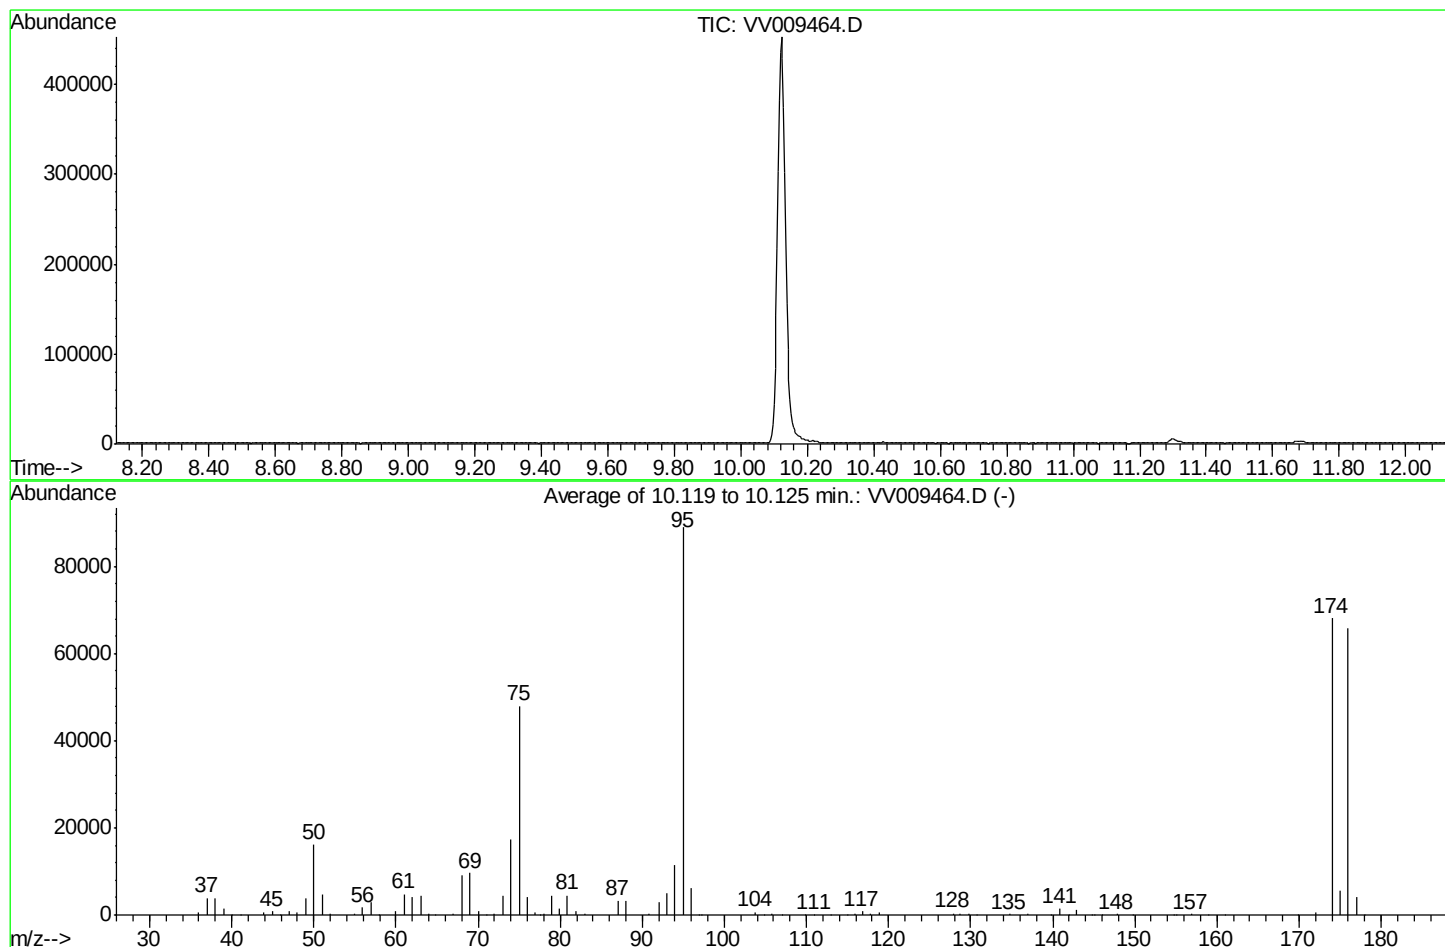

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	16062	PASS
75	95	30	80	53.9	47936	PASS
95	95	100	100	100.0	88949	PASS
96	95	5	9	6.9	6117	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.5	68016	PASS
175	174	5	9	8.0	5445	PASS
176	174	95	101	96.9	65941	PASS
177	176	5	9	6.1	4033	PASS

m/z	Abundance
36.00	631.0
37.00	3934.0
38.00	3901.0
39.00	1631.0
39.90	592.0
41.00	122.0
44.00	975.0
45.00	775.0
45.90	132.0
47.00	936.0
47.90	479.0
49.00	3801.0
50.00	15895.0
51.00	4711.0
52.10	312.0
54.90	251.0
55.90	1760.0
57.00	2995.0
57.90	120.0
60.00	878.0
61.00	4612.0
62.00	4205.0
63.00	4180.0
63.90	276.0
64.80	137.0
67.00	249.0
68.00	9207.0
69.00	10044.0
70.00	867.0
71.90	452.0
73.00	4619.0
74.00	17144.0
75.00	48000.0
76.00	3958.0
76.90	503.0
77.60	243.0
78.00	322.0
78.90	4362.0
79.90	1432.0
80.90	4458.0
81.90	891.0
83.00	143.0
87.00	3180.0
87.90	3134.0
90.80	424.0
92.00	2909.0
93.00	4676.0
94.00	11480.0
95.00	88904.0
96.00	6231.0
97.20	123.0
103.80	608.0
104.80	140.0
105.80	405.0
107.00	166.0
110.90	148.0
112.90	115.0
114.90	114.0
116.00	416.0
116.90	706.0
117.80	411.0
118.90	648.0
127.90	392.0
128.70	194.0
130.00	367.0
130.80	145.0
134.70	243.0
137.00	167.0
139.80	118.0
140.90	1255.0
141.90	101.0
143.00	1347.0
145.90	123.0
147.80	325.0
149.80	122.0
155.00	199.0
156.90	148.0
158.90	104.0
160.90	106.0
169.90	101.0
172.20	419.0
174.00	66184.0
175.00	5414.0
175.90	64744.0
177.00	3983.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	681.0
37.00	3991.0
38.00	3891.0
39.00	1700.0
39.90	639.0
44.00	891.0
44.90	836.0
45.90	111.0
47.00	875.0
47.90	496.0
49.00	3816.0
50.00	16584.0
51.00	4886.0
52.10	325.0
54.90	214.0
56.00	1733.0
57.00	3035.0
58.00	145.0
60.00	978.0
61.00	4957.0
62.00	4313.0
63.00	4429.0
63.90	300.0
64.80	166.0
67.00	234.0
68.00	9450.0
69.00	9953.0
70.00	837.0
71.90	448.0
73.00	4675.0
74.00	17872.0
75.00	49424.0
76.00	4294.0
77.00	566.0
78.00	325.0
78.90	4578.0
79.90	1419.0
80.90	4527.0
81.90	872.0
83.00	167.0
87.00	3494.0
87.90	3230.0
90.70	417.0
92.00	2964.0
93.00	4987.0
94.00	11622.0
95.00	91488.0
96.00	6286.0
96.90	158.0
97.10	156.0
103.80	623.0
104.80	169.0
105.80	438.0
107.00	131.0
110.90	166.0
113.00	143.0
116.00	448.0
116.80	811.0
117.80	431.0
118.80	688.0
127.90	420.0
128.70	219.0
129.80	336.0
130.80	142.0
134.70	228.0
137.00	185.0
139.80	116.0
140.90	1414.0
142.90	1375.0
145.00	113.0
146.00	120.0
147.80	288.0
149.80	157.0
154.70	128.0
155.10	142.0
156.90	183.0
158.90	131.0
161.00	100.0
172.10	480.0
174.00	70224.0
175.00	5625.0
175.90	67960.0
177.00	4107.0
178.00	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	642.0
37.00	3621.0
38.00	3540.0
39.00	1513.0
39.90	670.0
44.00	855.0
44.90	789.0
45.90	104.0
47.00	732.0
47.90	523.0
49.00	3468.0
50.00	15708.0
51.00	4758.0
52.00	271.0
55.00	219.0
56.00	1619.0
57.00	2785.0
58.00	158.0
60.00	931.0
61.00	4764.0
62.00	4063.0
63.00	4205.0
64.00	299.0
64.80	143.0
67.00	191.0
68.00	8856.0
69.00	9034.0
70.00	758.0
71.00	116.0
72.00	428.0
73.00	4233.0
74.00	16800.0
75.00	46384.0
76.00	4129.0
77.00	532.0
77.90	342.0
78.90	4366.0
79.90	1251.0
80.90	4256.0
81.90	840.0
83.00	174.0
87.00	3364.0
88.00	3061.0
90.80	464.0
92.00	2754.0
93.00	4964.0
94.00	10939.0
95.00	86456.0
96.00	5834.0
97.10	177.0
103.80	614.0
104.80	168.0
105.80	468.0
106.90	115.0
109.90	109.0
111.00	157.0
113.00	140.0
115.90	404.0
116.80	824.0
117.80	417.0
118.80	693.0
127.90	398.0
128.70	195.0
129.70	373.0
130.80	106.0
134.80	211.0
137.00	196.0
140.90	1349.0
141.90	135.0
142.90	1268.0
144.70	119.0
146.00	129.0
147.80	254.0
149.80	154.0
154.70	123.0
155.10	111.0
156.90	171.0
158.90	116.0
172.00	500.0
174.00	67640.0
175.00	5298.0
176.00	65120.0
177.00	4009.0
177.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
39.90	509.0
43.90	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71