

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030420\
 Data File : VV014732.D
 Acq On : 04 Mar 2020 14:16
 Operator : SY/MD
 Sample : L1677-24
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CD9

Quant Time: Mar 05 06:51:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 05 06:28:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	252562	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	243833	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	117941	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77449	3.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.40%
7) Chloroethane-d5	1.58	69	68403	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.40%
11) 1,1-Dichloroethene-d2	2.13	63	106568	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	3.97	46	191142	46.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.54%
24) Chloroform-d	4.40	84	159963	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.08	65	85697	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	5.10	84	330066	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.12	67	104848	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.36	98	293556	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.66	79	38509	4.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.00%
46) 2-Hexanone-d5	8.14	63	140237	40.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.04%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	73843	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	106194	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%

Target Compounds


					Ovalue
3) Chloromethane	1.25	50	5444	0.213 ug/L	98
25) Chloroform	4.42	83	5888	0.159 ug/L	82
42) Toluene	7.43	91	18175	0.214 ug/L	97
53) m,p-xylene	9.18	106	4059	0.115 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030420\
Data File : VV014732.D
Acq On : 04 Mar 2020 14:16
Operator : SY/MD
Sample : L1677-24
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CD9

Quant Time: Mar 05 06:51:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 05 06:28:00 2020
Response via : Initial Calibration

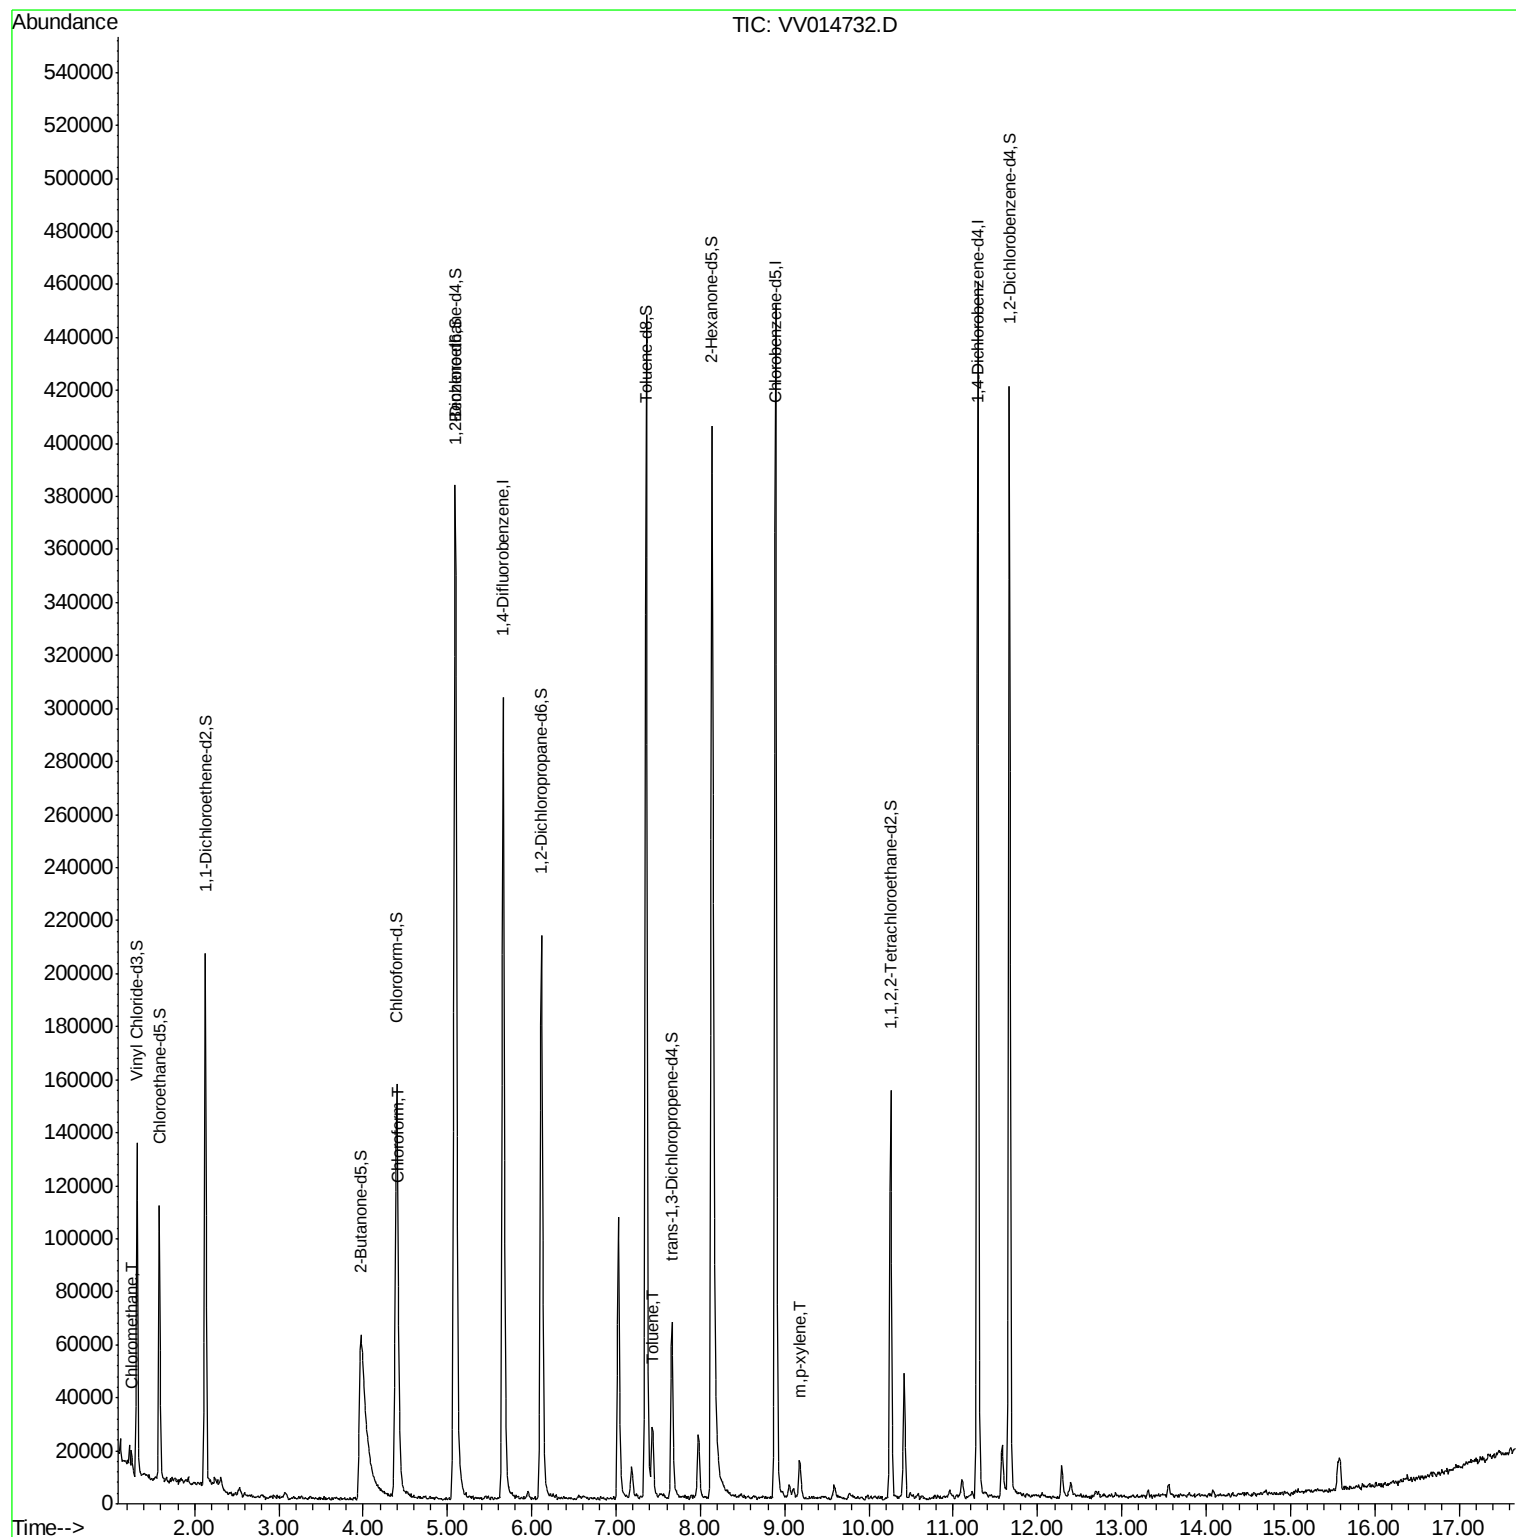

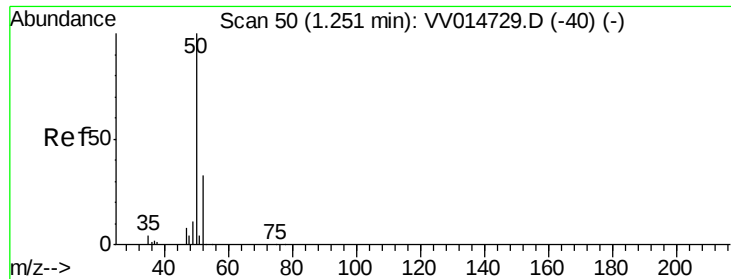

#3

Chloromethane

Concen: 0.213 ug/L

RT: 1.25 min Scan# 51

Delta R.T. 0.00 min

Lab File: VV014732.D

Acq: 04 Mar 2020 14:16

Instrument :

MSVOA_V

ClientSampleId :





C0CD9

Tot Ion: 50 Resp: 5444

Ion Ratio Lower Upper

50 100

52 31.4 22.9 42.5

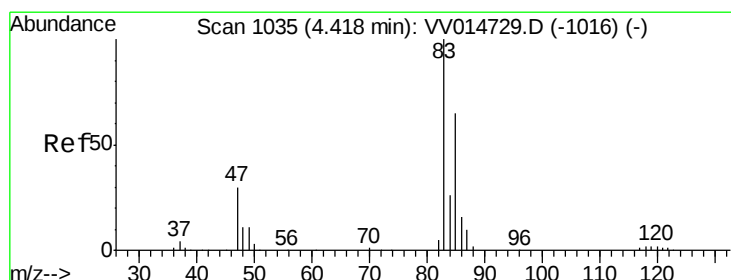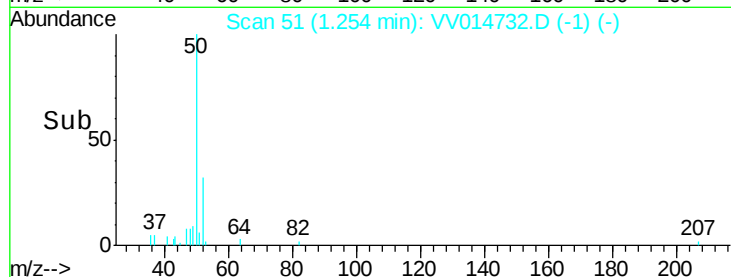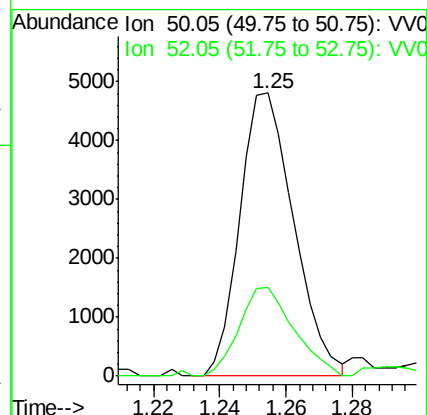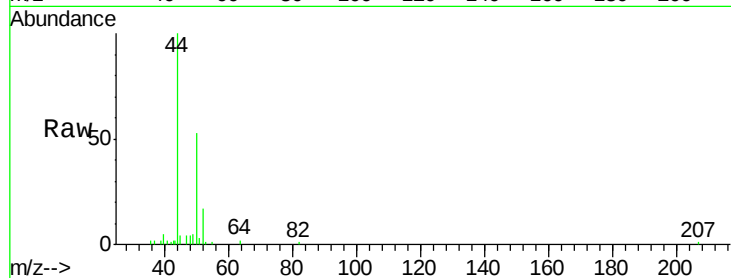

#25

Chloroform

Concen: 0.159 ug/L

RT: 4.42 min Scan# 1037

Delta R.T. 0.01 min

Lab File: VV014732.D




Acq: 04 Mar 2020 14:16


Tgt Ion: 83 Resp: 5888

Ion Ratio Lower Upper

83 100

85 78.3 44.7 83.1

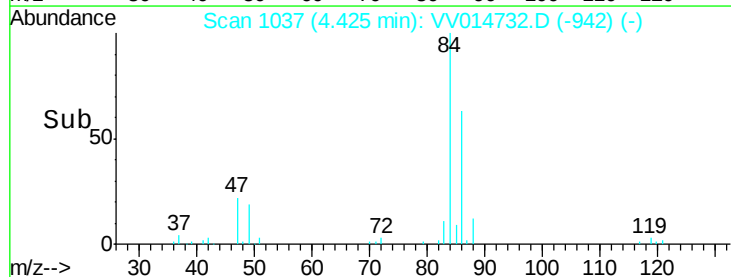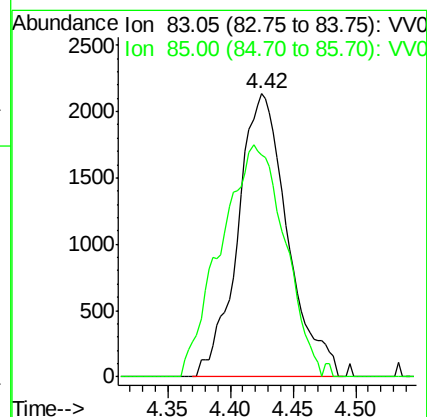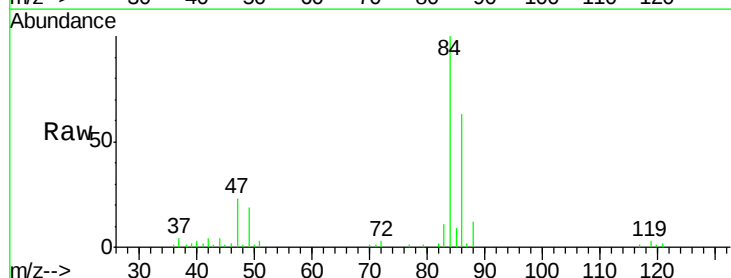

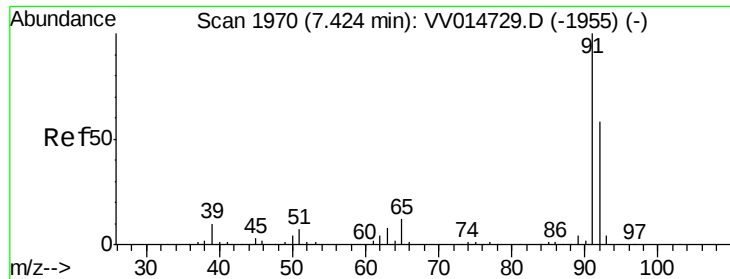

#42

Toluene

Concen: 0.214 ug/L

RT: 7.43 min Scan# 1973

Delta R.T. 0.01 min

Lab File: VV014732.D

Acq: 04 Mar 2020 14:16

Instrument :

MSVOA_V

ClientSampled :


C0CD9

Tot Ion: 91 Resp: 18175

Ion Ratio Lower Upper




91 100

92 60.1 40.3 74.9

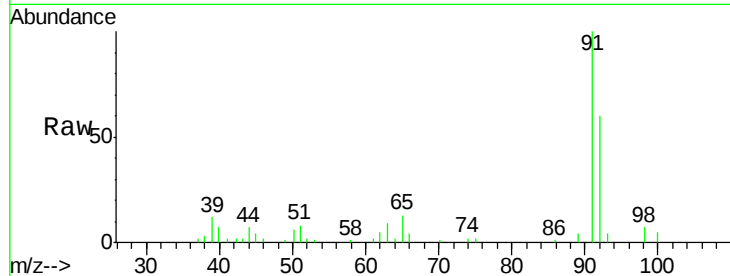

Abundance Ion 91.15 (90.85 to 91.85): VV014729.D (-1955) (-)

Ion 92.15 (91.85 to 92.85): VV014729.D (-1955) (-)

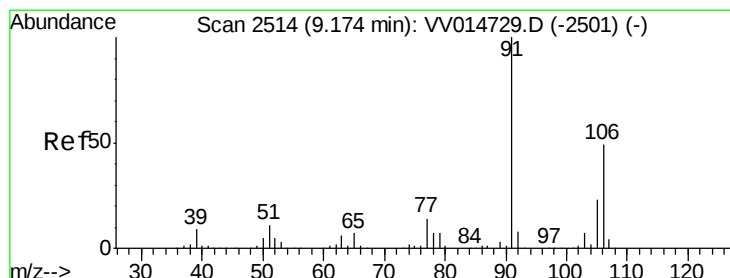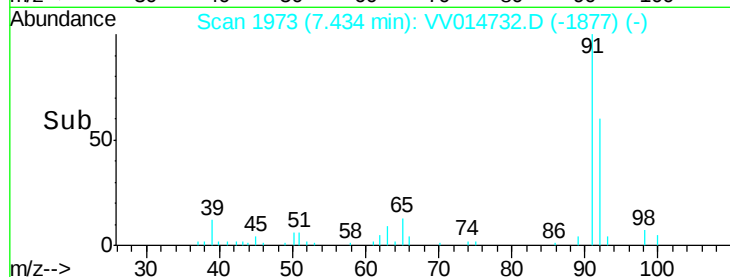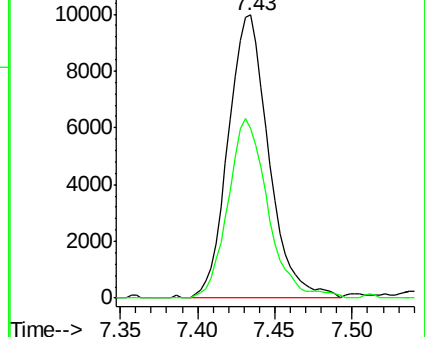

#53

m,p-xylene

Concen: 0.115 ug/L

RT: 9.18 min Scan# 2515

Delta R.T. 0.00 min

Lab File: VV014732.D


Acq: 04 Mar 2020 14:16

Tgt Ion: 106 Resp: 4059

Ion Ratio Lower Upper

106 100

91 208.9 142.5 264.6

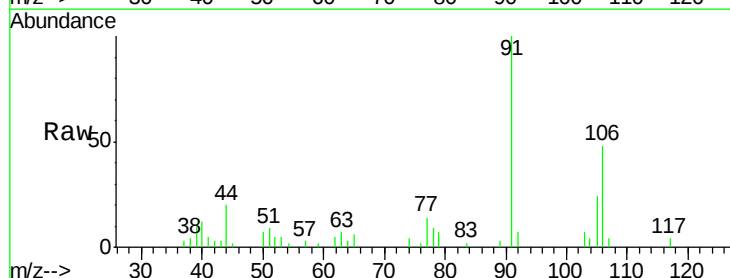

Abundance Ion 106.15 (105.85 to 106.85): VV014729.D (-2501) (-)

Ion 91.15 (90.85 to 91.85): VV014729.D (-2501) (-)

