

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030420\
 Data File : VV014734.D
 Acq On : 04 Mar 2020 15:04
 Operator : SY/MD
 Sample : L1708-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C98

Quant Time: Mar 05 11:30:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 05 06:28:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	249611	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	238198	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	118312	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	78112	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.59	69	63483	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.00%
11) 1,1-Dichloroethene-d2	2.13	63	100169	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	3.96	46	218713	54.15	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.30%
24) Chloroform-d	4.40	84	155733	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	5.08	65	87286	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	321470	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.12	67	104570	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	280983	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	7.66	79	36896	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.14	63	148681	43.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.96%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	77435	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	108061	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.23	43	9754	3.588 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030420\
Data File : VV014734.D
Acq On : 04 Mar 2020 15:04
Operator : SY/MD
Sample : L1708-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C98

Quant Time: Mar 05 11:30:52 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 05 06:28:00 2020
Response via : Initial Calibration

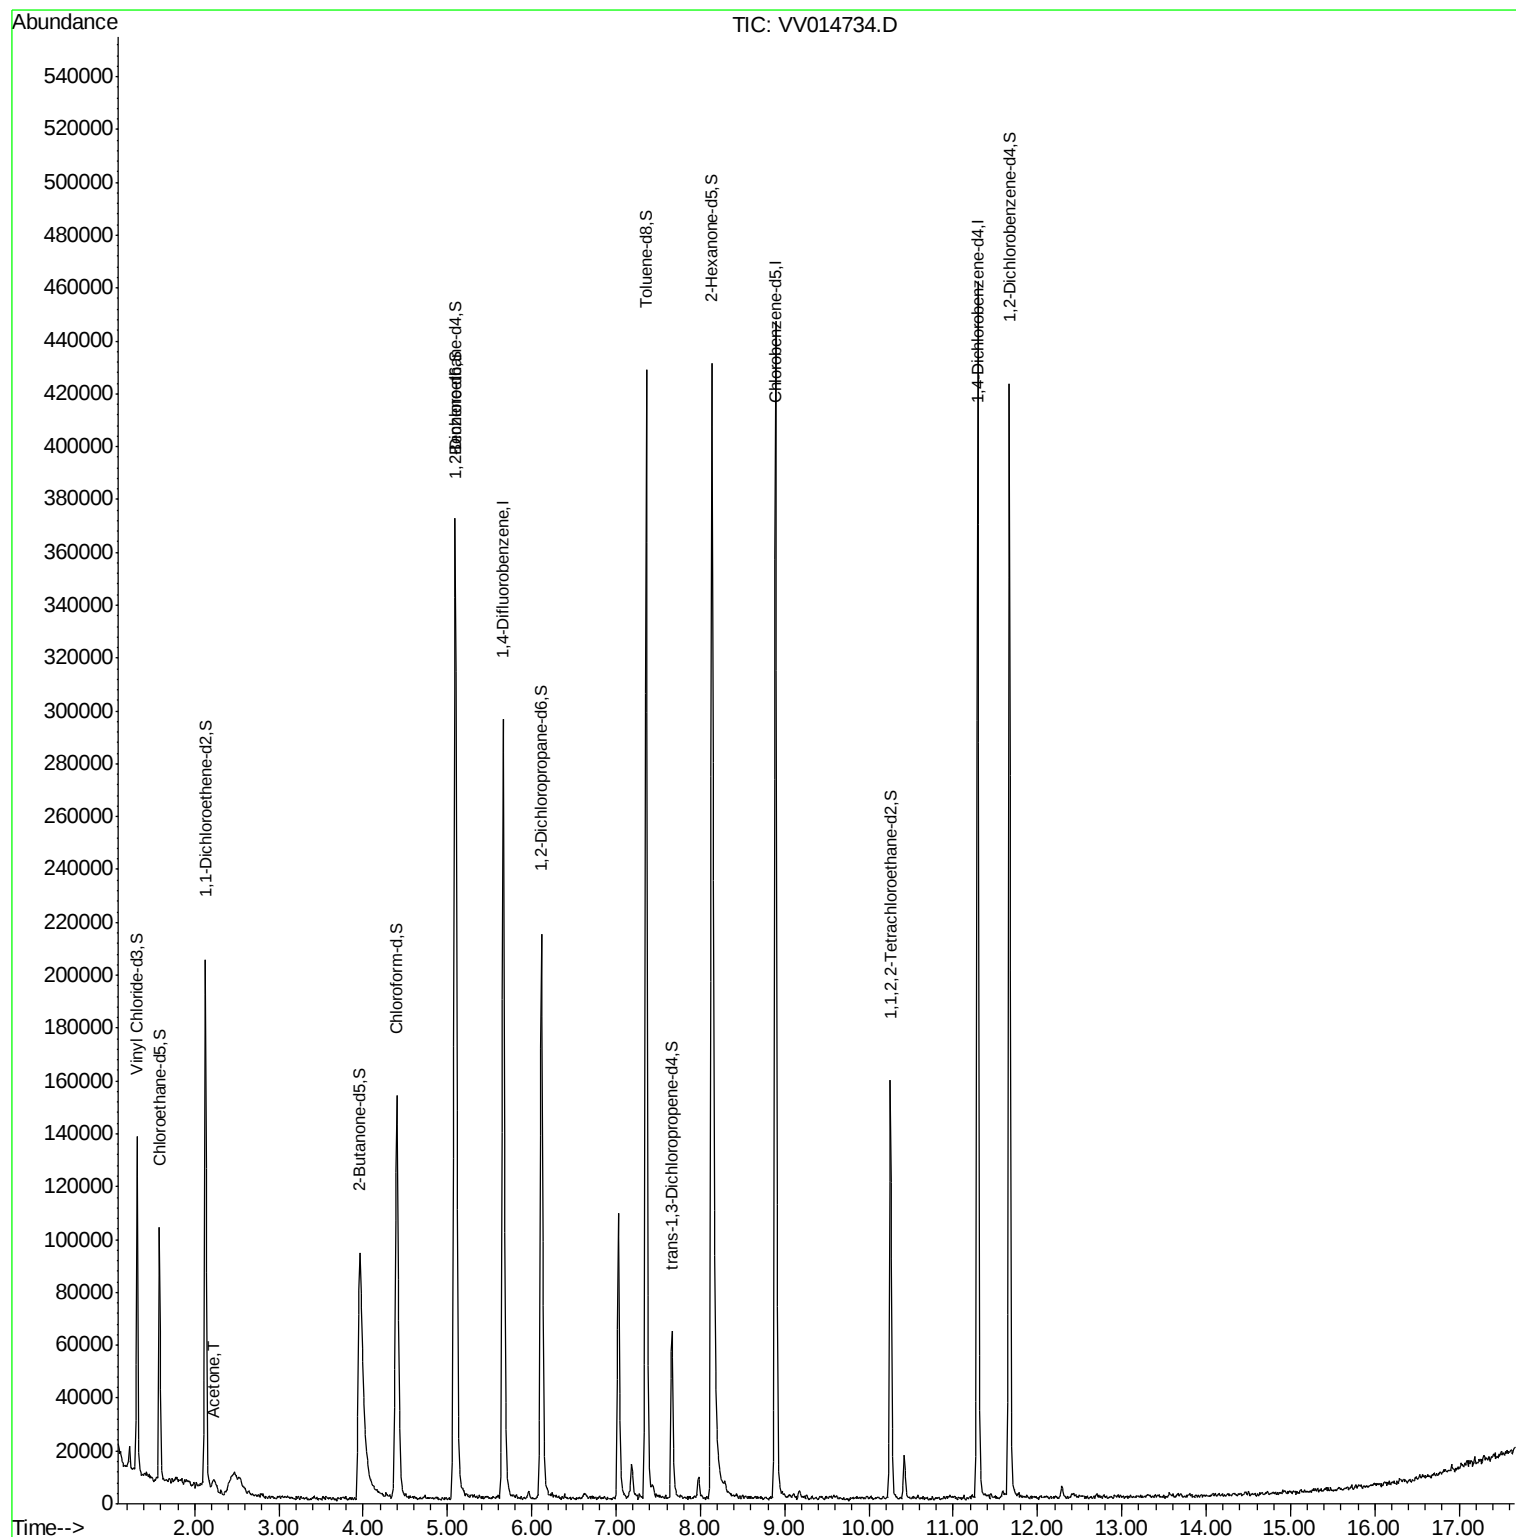

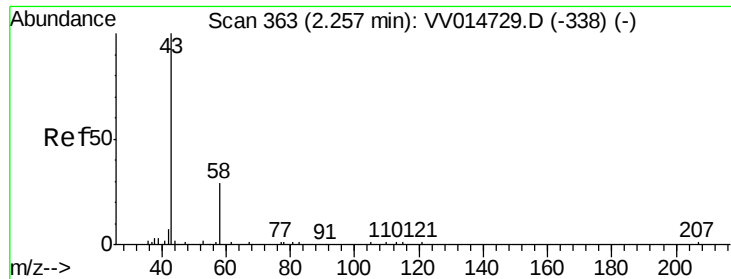

#13

Acetone

Concen: 3.588 ug/L

RT: 2.23 min Scan# 355

Delta R.T. -0.03 min

Lab File: VV014734.D

Acq: 04 Mar 2020 15:04

Instrument :

MSVOA_V

ClientSampleId :

C0C98

Tot Ion: 43 Resp: 9754

Ion Ratio Lower Upper

43 100

58 19.4 0.0 20.0

