

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030420\
 Data File : VV014737.D
 Acq On : 04 Mar 2020 16:14
 Operator : SY/MD
 Sample : L1708-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE2

Quant Time: Mar 05 11:32:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 05 06:28:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	245243	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	236075	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	114065	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76183	3.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.40%
7) Chloroethane-d5	1.59	69	64974	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.60%
11) 1,1-Dichloroethene-d2	2.13	63	99171	3.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.80%
20) 2-Butanone-d5	3.96	46	192314	48.46	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.92%
24) Chloroform-d	4.40	84	154773	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.08	65	82611	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.10	84	322186	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.12	67	102539	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.36	98	283220	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	7.66	79	34994	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.14	63	120429	35.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.88%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	71101	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	105993	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Ovalue
13) Acetone	2.22	43	9664	3.618 ug/L	87
42) Toluene	7.43	91	10689	0.130 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030420\
Data File : VV014737.D
Acq On : 04 Mar 2020 16:14
Operator : SY/MD
Sample : L1708-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE2

Quant Time: Mar 05 11:32:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 05 06:28:00 2020
Response via : Initial Calibration

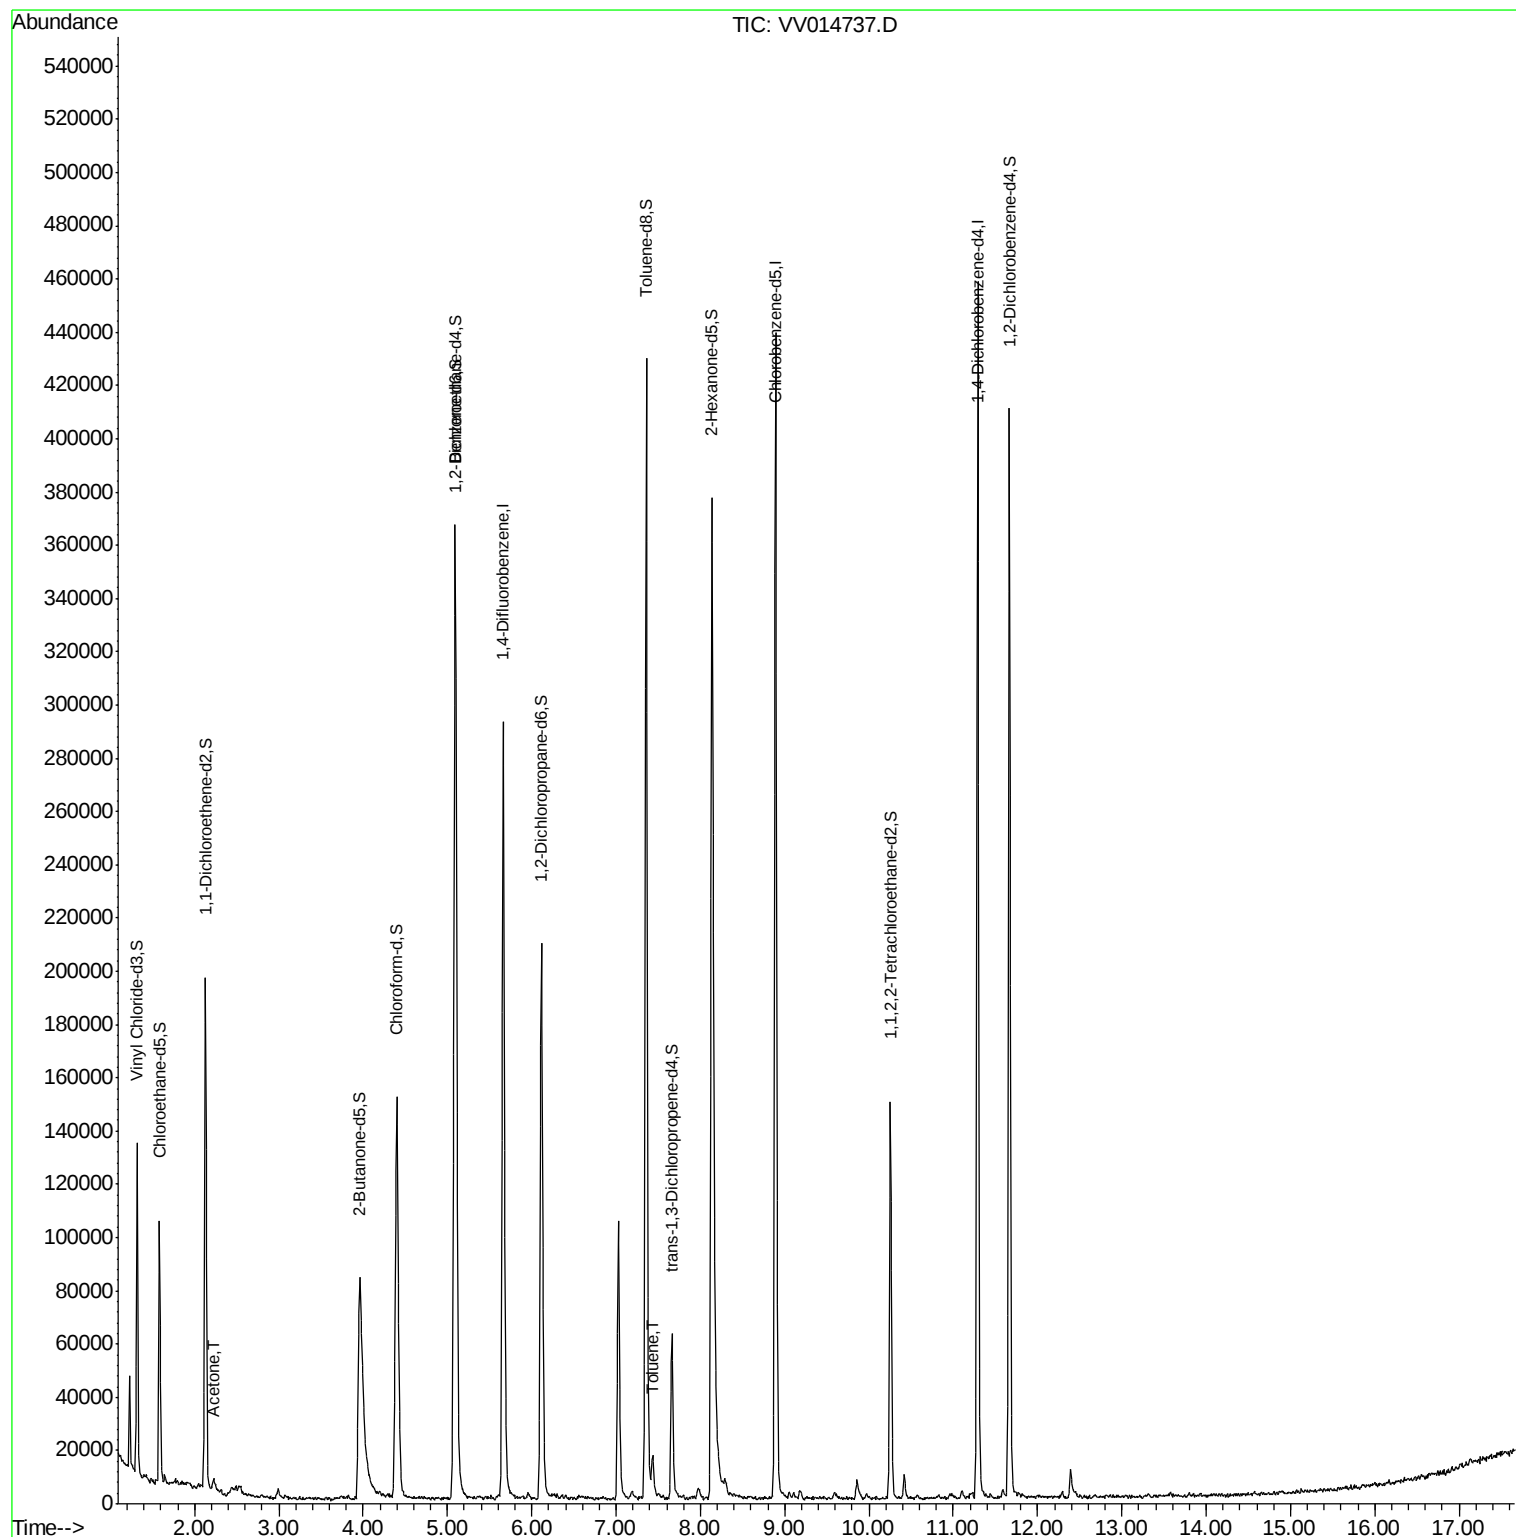

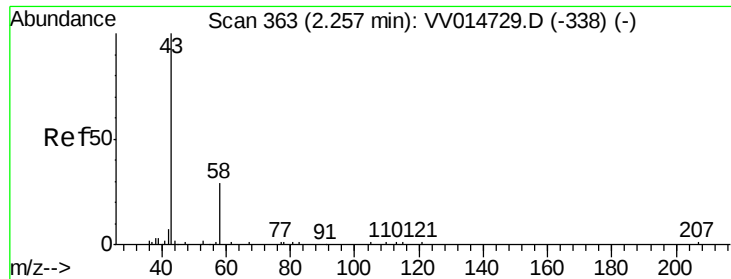

#13

Acetone

Concen: 3.618 ug/L

RT: 2.22 min Scan# 352

Delta R.T. -0.04 min

Lab File: VV014737.D

Acq: 04 Mar 2020 16:14

Instrument :

MSVOA_V

ClientSampleId :





C0CE2

Tot Ion: 43 Resp: 9664

Ion Ratio Lower Upper

43 100

58 15.0 0.0 20.0

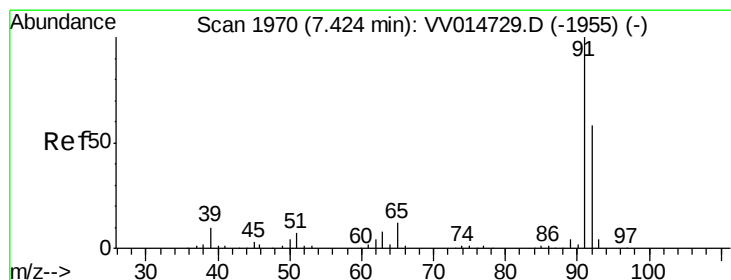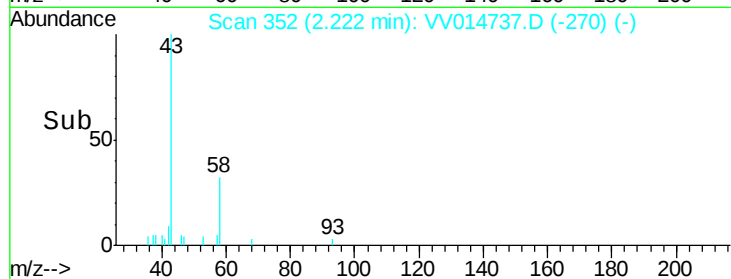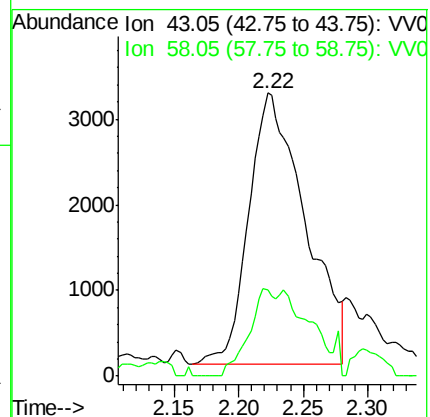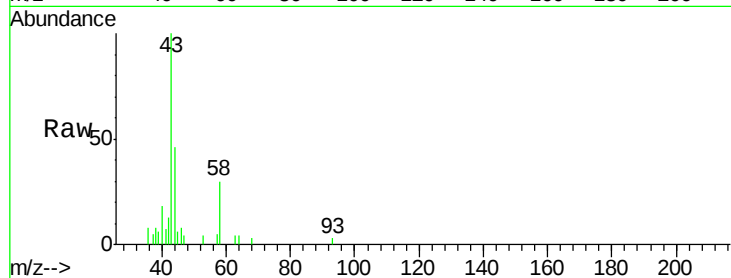

#42

Toluene

Concen: 0.130 ug/L

RT: 7.43 min Scan# 1972

Delta R.T. 0.01 min

Lab File: VV014737.D

Acq: 04 Mar 2020 16:14

Tgt Ion: 91 Resp: 10689

Ion Ratio Lower Upper

91 100

92 46.3 40.3 74.9

