

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV030420\
 Data File : VV014738.D
 Acq On : 04 Mar 2020 16:37
 Operator : SY/MD
 Sample : L1677-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CD6

Quant Time: Mar 05 11:32:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Mar 05 06:28:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	246483	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	235041	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	115865	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	75392	3.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.20%
7) Chloroethane-d5	1.58	69	65955	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.13	63	100274	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.96	46	192914	48.37	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.74%
24) Chloroform-d	4.40	84	155629	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
26) 1,2-Dichloroethane-d4	5.08	65	84540	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.10	84	321874	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.11	67	103403	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	7.36	98	280916	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
43) trans-1,3-Dichloropropene-	7.66	79	34610	4.20	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.00%
46) 2-Hexanone-d5	8.13	63	129302	38.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.52%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	73642	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	106503	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	3937	0.158 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV030420\
Data File : VV014738.D
Acq On : 04 Mar 2020 16:37
Operator : SY/MD
Sample : L1677-18
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CD6

Quant Time: Mar 05 11:32:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 05 06:28:00 2020
Response via : Initial Calibration

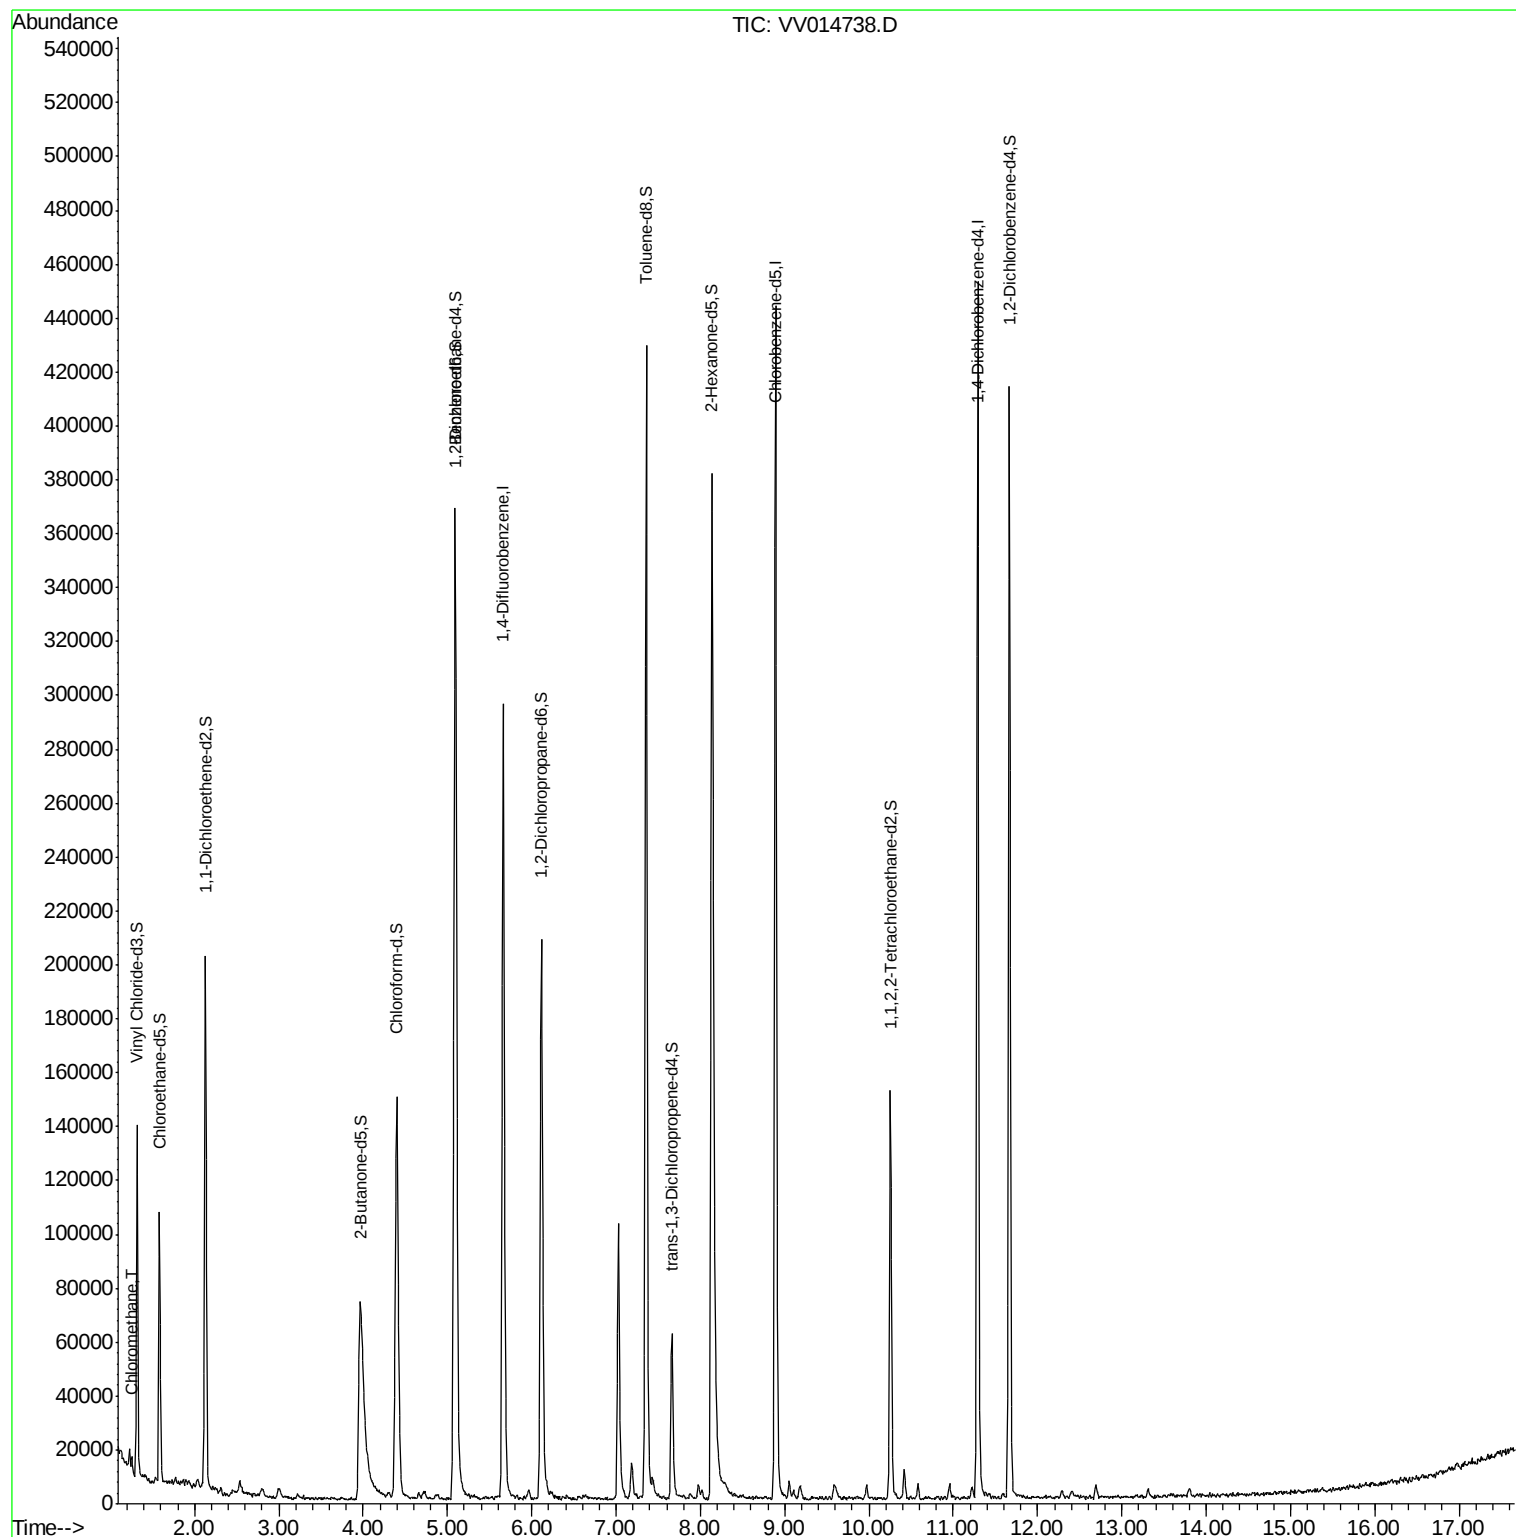

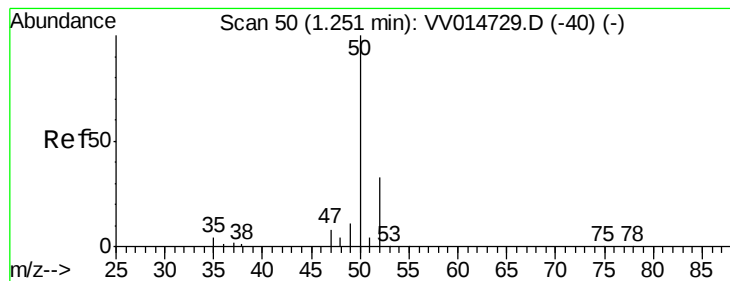

#3

Chloromethane

Concen: 0.158 ug/L

RT: 1.25 min Scan# 51

Delta R.T. 0.00 min

Lab File: VV014738.D

Acq: 04 Mar 2020 16:37

Instrument :
MSVOA_V
ClientSampleId :
C0CD6

Tot Ion: 50 Resp: 3937

Ion Ratio Lower Upper

50 100

52 33.8 22.9 42.5

