


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030420\
Data File : VV014728.D
Acq On : 04 Mar 2020 09:25
Operator : SY/MD
Sample : BFB41
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Mar 05 06:28:00 2020

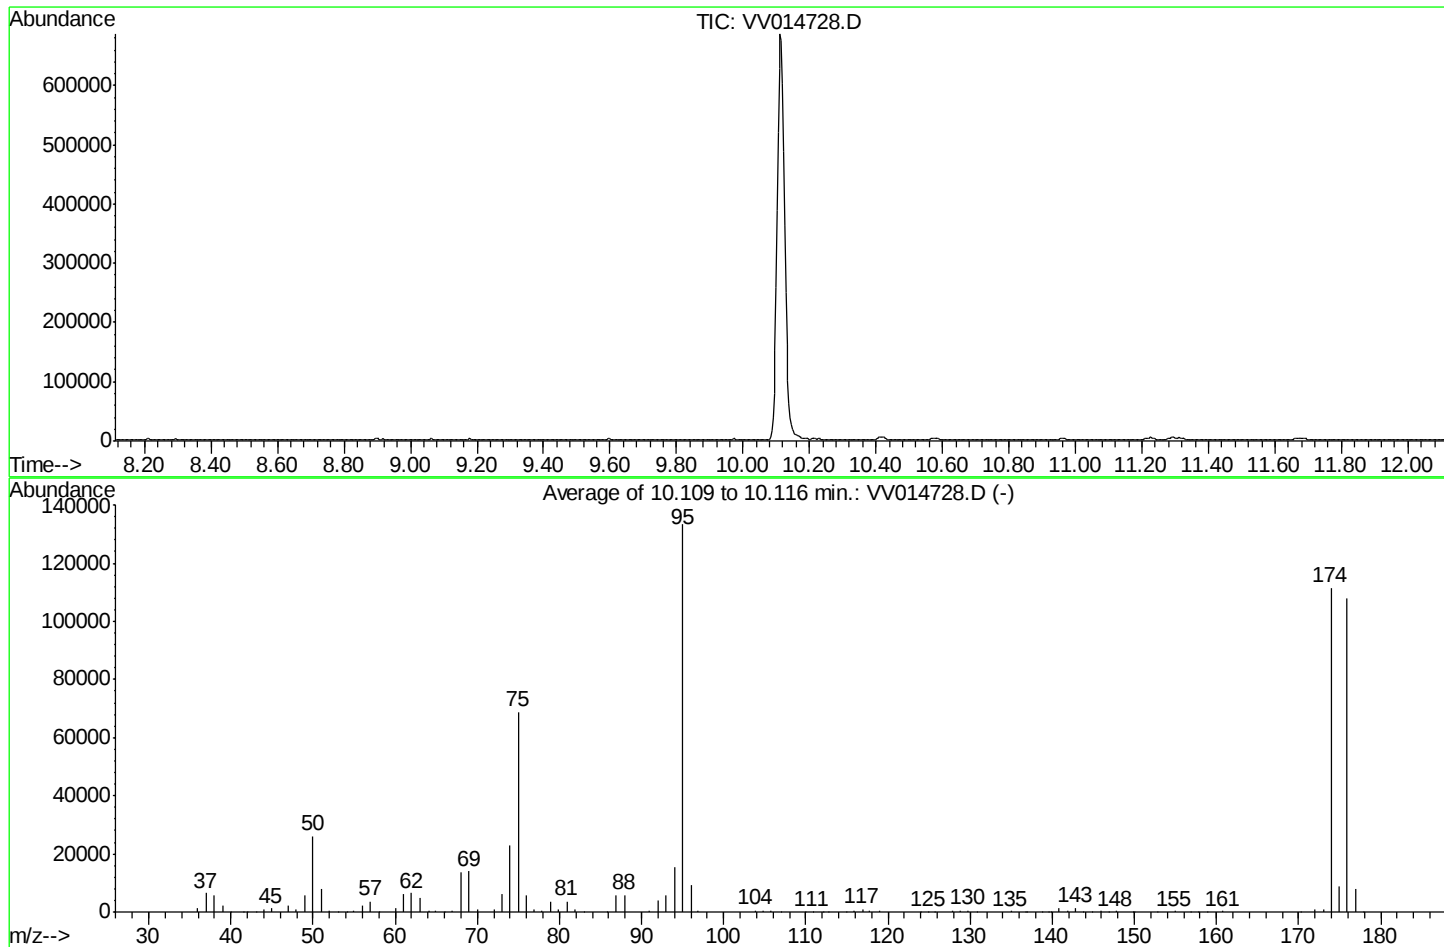

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	26013	PASS
75	95	30	80	51.6	68866	PASS
95	95	100	100	100.0	133376	PASS
96	95	5	9	7.0	9334	PASS
173	174	0.00	2	0.7	815	PASS
174	95	50	120	83.6	111498	PASS
175	174	5	9	7.7	8622	PASS
176	174	95	101	96.8	107973	PASS
177	176	5	9	7.2	7741	PASS

m/z	Abundance
36.00	1130.0
37.00	6461.0
38.00	5357.0
39.00	2266.0
39.90	513.0
41.50	109.0
42.00	120.0
43.10	152.0
44.00	1469.0
44.90	1158.0
47.00	2166.0
47.90	899.0
49.00	5261.0
50.00	25904.0
51.00	8113.0
52.00	301.0
53.00	158.0
55.00	358.0
56.00	1986.0
57.00	3487.0
58.20	161.0
60.00	1414.0
61.00	6077.0
62.00	6023.0
63.10	4602.0
64.00	568.0
64.90	571.0
65.90	105.0
67.00	312.0
68.00	12782.0
69.00	13209.0
70.00	983.0
72.00	765.0
73.00	5730.0
74.00	21992.0
75.00	65216.0
76.00	5654.0
76.90	1022.0
77.90	489.0
78.90	3218.0
79.90	1014.0
80.90	3673.0
81.90	930.0
82.90	117.0
85.80	196.0
86.90	5649.0
87.90	5912.0
91.00	522.0
92.00	3580.0
93.00	5430.0
94.00	14732.0
95.00	125760.0
96.00	8888.0
96.90	296.0
103.90	626.0
104.90	318.0
105.80	640.0
106.90	170.0
110.00	123.0
110.90	132.0
112.10	104.0
112.90	143.0
115.70	355.0
116.90	834.0
117.70	428.0
118.90	606.0
123.90	106.0
127.90	412.0
128.70	338.0
129.80	514.0
130.80	199.0
134.90	316.0
136.90	183.0
138.80	123.0
140.00	149.0
140.80	1020.0
141.80	291.0
142.90	1548.0
143.80	136.0
145.00	178.0
146.00	277.0
146.90	110.0
147.80	306.0
149.80	151.0
152.70	125.0
154.90	316.0
156.90	216.0
158.80	193.0
160.80	357.0
170.30	110.0
171.90	872.0
173.00	1150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

173.90	104264.0
174.90	8495.0
175.90	100296.0
176.90	7404.0
177.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
35.90	1154.0
37.00	6129.0
38.00	5795.0
39.00	2504.0
39.90	520.0
41.80	139.0
43.00	202.0
44.00	1441.0
45.00	1161.0
47.00	2079.0
47.90	817.0
49.00	5597.0
50.00	25208.0
51.00	7544.0
51.90	385.0
53.00	157.0
54.10	111.0
55.00	305.0
56.00	2281.0
57.00	3557.0
58.00	256.0
60.00	1520.0
61.00	6263.0
62.00	6698.0
63.00	4720.0
64.10	644.0
65.00	613.0
66.00	168.0
66.90	347.0
68.00	13843.0
69.00	14268.0
70.00	972.0
72.00	795.0
73.00	6407.0
74.00	23056.0
75.00	70248.0
76.00	5775.0
77.00	943.0
77.90	610.0
79.00	3516.0
79.90	1111.0
80.90	3668.0
81.90	788.0
82.90	145.0
85.80	183.0
86.90	5515.0
87.90	5591.0
90.90	537.0
92.00	4167.0
93.00	6061.0
94.00	15950.0
95.00	136448.0
96.00	9503.0
96.90	208.0
103.90	646.0
104.80	253.0
105.80	641.0
107.10	141.0
110.80	195.0
112.10	128.0
112.70	151.0
114.90	127.0
115.90	462.0
116.90	924.0
117.90	612.0
118.90	706.0
124.90	166.0
125.70	142.0
127.90	459.0
128.90	190.0
129.70	610.0
130.80	211.0
135.00	285.0
136.70	151.0
136.90	142.0
139.60	106.0
140.90	1345.0
141.80	201.0
142.80	1458.0
144.80	154.0
145.90	220.0
146.90	150.0
147.80	333.0
150.00	140.0
152.80	126.0
155.00	389.0
156.90	207.0
157.80	124.0
158.80	109.0
160.70	185.0
172.00	1001.0
173.90	114960.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

174.90	8430.0
175.90	111832.0
176.90	7711.0
177.80	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	1190.0
37.00	6676.0
38.00	5953.0
39.00	2465.0
39.90	536.0
41.50	104.0
42.10	120.0
43.00	185.0
44.00	1545.0
44.90	1215.0
47.00	2220.0
47.90	873.0
49.00	5819.0
50.00	26928.0
51.00	8265.0
51.90	342.0
53.00	163.0
55.00	325.0
56.00	2315.0
57.00	3747.0
58.00	215.0
60.00	1637.0
61.00	6480.0
62.00	6673.0
63.00	4801.0
64.10	592.0
64.90	627.0
65.90	162.0
67.00	359.0
68.00	14208.0
69.00	14592.0
70.00	1048.0
72.00	814.0
73.00	6356.0
74.00	23568.0
75.00	71136.0
76.00	5944.0
77.00	1019.0
77.90	555.0
78.90	3426.0
79.90	1122.0
80.90	3836.0
81.90	893.0
82.90	138.0
85.80	218.0
86.90	5914.0
87.90	6073.0
91.00	558.0
92.00	4039.0
93.00	6129.0
94.00	15981.0
95.00	137920.0
96.00	9611.0
96.90	257.0
103.90	721.0
104.80	298.0
105.80	660.0
107.00	147.0
110.90	152.0
112.10	126.0
112.80	158.0
115.80	423.0
116.90	935.0
117.80	505.0
118.90	708.0
123.90	104.0
124.90	141.0
127.90	455.0
128.80	233.0
129.80	566.0
130.80	224.0
134.90	316.0
137.00	168.0
139.80	114.0
140.90	1162.0
141.80	238.0
142.80	1645.0
143.70	116.0
144.80	175.0
146.00	272.0
146.90	147.0
147.80	311.0
150.00	140.0
152.80	131.0
155.00	368.0
156.80	212.0
158.80	141.0
160.70	289.0
170.30	105.0
171.90	951.0
173.00	1297.0
173.90	115272.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

174.90	8941.0
175.90	111792.0
176.90	8108.0
177.80	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
37.70	104.0
38.40	116.0
39.90	511.0
41.00	109.0
41.80	111.0
44.00	775.0
47.80	107.0
67.80	147.0
77.90	157.0
207.00	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41