

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020460.D
 Acq On : 04 Mar 2021 10:41
 Operator : SY/MD
 Sample : VV0304WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Quant Time: Mar 04 12:34:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 04 00:36:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	504447	50.00	ug/L	# 0.00
28) Chlorobenzene-d5	8.857	117	502201	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	250326	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	157622	42.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.72%
7) Chloroethane-d5	1.571	69	139121	46.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.108	63	223010	32.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.16%
21) 2-Butanone-d5	3.895	46	216452	105.34	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.34%
24) Chloroform-d	4.352	84	323876	49.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.98%
26) 1,2-Dichloroethane-d4	5.037	65	213560	51.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.94%
32) Benzene-d6	5.053	84	648105	49.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.62%
36) 1,2-Dichloropropane-d6	6.072	67	200240	51.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.10%
41) Toluene-d8	7.320	98	595429	48.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.40%
43) trans-1,3-Dichloroprop...	7.625	79	89283	45.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.18%
47) 2-Hexanone-d5	8.091	63	137715	85.22	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.22%
57) 1,1,2,2-Tetrachloroeth...	10.220	84	255984	45.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.78%
64) 1,2-Dichlorobenzene-d4	11.631	152	273516	57.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.50%
Target Compounds						
25) Chloroform	4.384	83	12300	1.99	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020460.D
Acq On : 04 Mar 2021 10:41
Operator : SY/MD
Sample : VV0304WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK67

Quant Time: Mar 04 12:34:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 04 00:36:40 2021
Response via : Initial Calibration

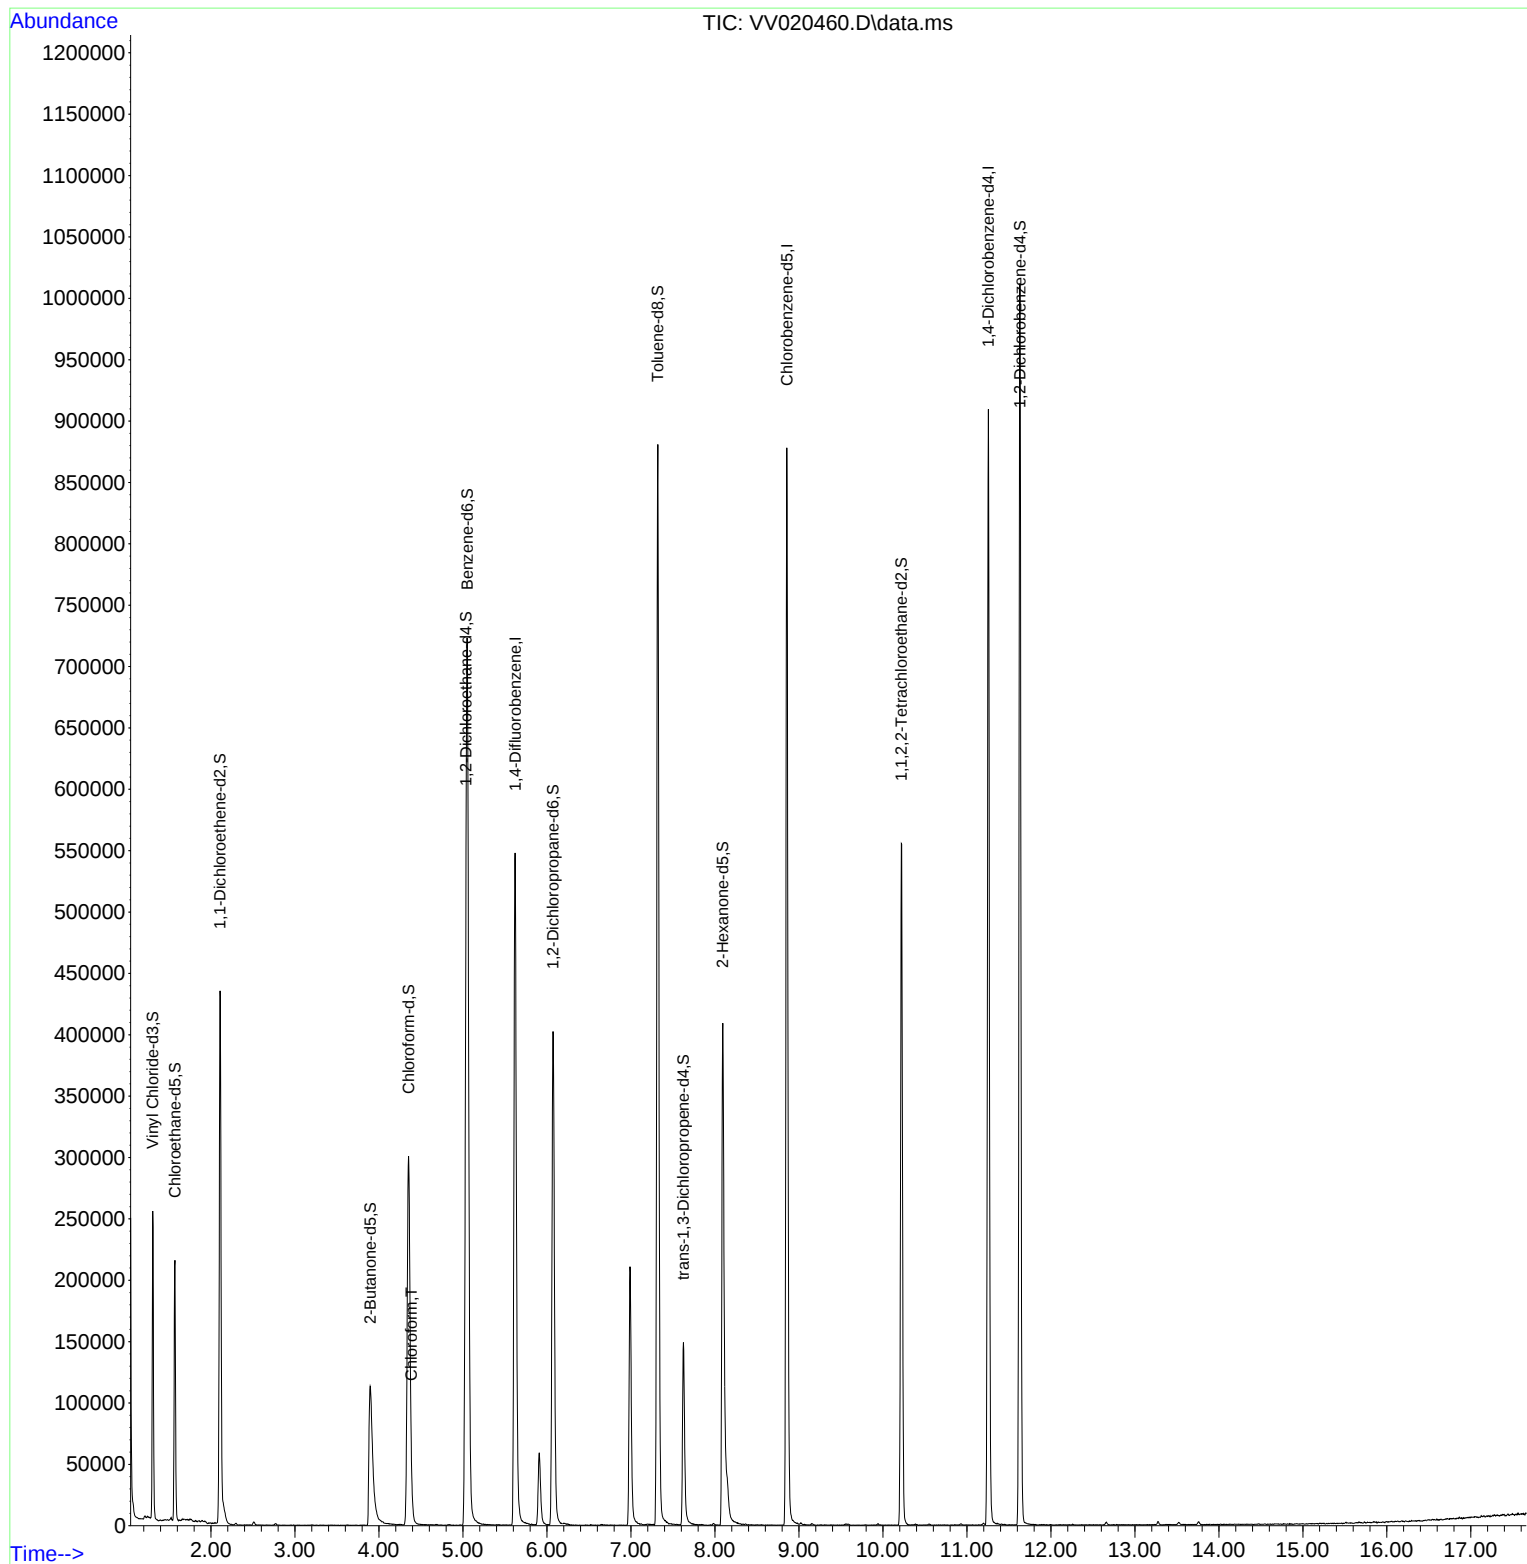

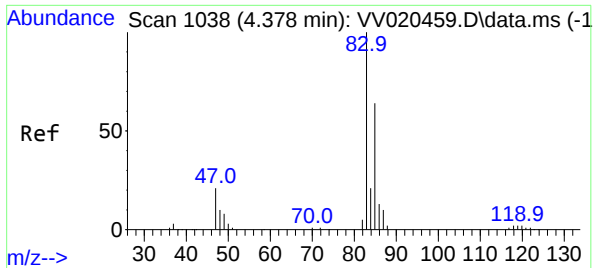

#25
 Chloroform
 Concen: 1.99 ug/L
 RT: 4.384 min Scan# 1040
 Delta R.T. 0.009 min
 Lab File: VV020460.D
 Acq: 04 Mar 2021 10:41

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK67

Tgt Ion: 83 Resp: 12300
 Ion Ratio Lower Upper
 83 100
 85 66.7 44.2 82.2

