

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020463.D
 Acq On : 04 Mar 2021 12:09
 Operator : SY/MD
 Sample : M1546-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Mar 04 12:35:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 04 00:36:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	502166	50.00	ug/L	# 0.00
28) Chlorobenzene-d5	8.857	117	505037	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	256088	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	151004	41.24	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.48%	
7) Chloroethane-d5	1.568	69	136150	45.33	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	90.66%	
11) 1,1-Dichloroethene-d2	2.108	63	214295	30.96	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	61.92%	
21) 2-Butanone-d5	3.892	46	207206	101.30	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.30%	
24) Chloroform-d	4.349	84	314555	48.28	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.56%	
26) 1,2-Dichloroethane-d4	5.034	65	207106	50.14	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.28%	
32) Benzene-d6	5.050	84	638720	48.81	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.62%	
36) 1,2-Dichloropropane-d6	6.072	67	198472	50.81	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.62%	
41) Toluene-d8	7.320	98	592547	48.19	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.38%	
43) trans-1,3-Dichloroprop...	7.622	79	88930	44.66	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.32%	
47) 2-Hexanone-d5	8.091	63	130463	80.28	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	80.28%	
57) 1,1,2,2-Tetrachloroeth...	10.223	84	245884	43.84	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.68%	
64) 1,2-Dichlorobenzene-d4	11.632	152	275315	56.82	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	113.64%	
Target Compounds						
25) Chloroform	4.381	83	12189	1.98	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020463.D
Acq On : 04 Mar 2021 12:09
Operator : SY/MD
Sample : M1546-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Mar 04 12:35:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 04 00:36:40 2021
Response via : Initial Calibration

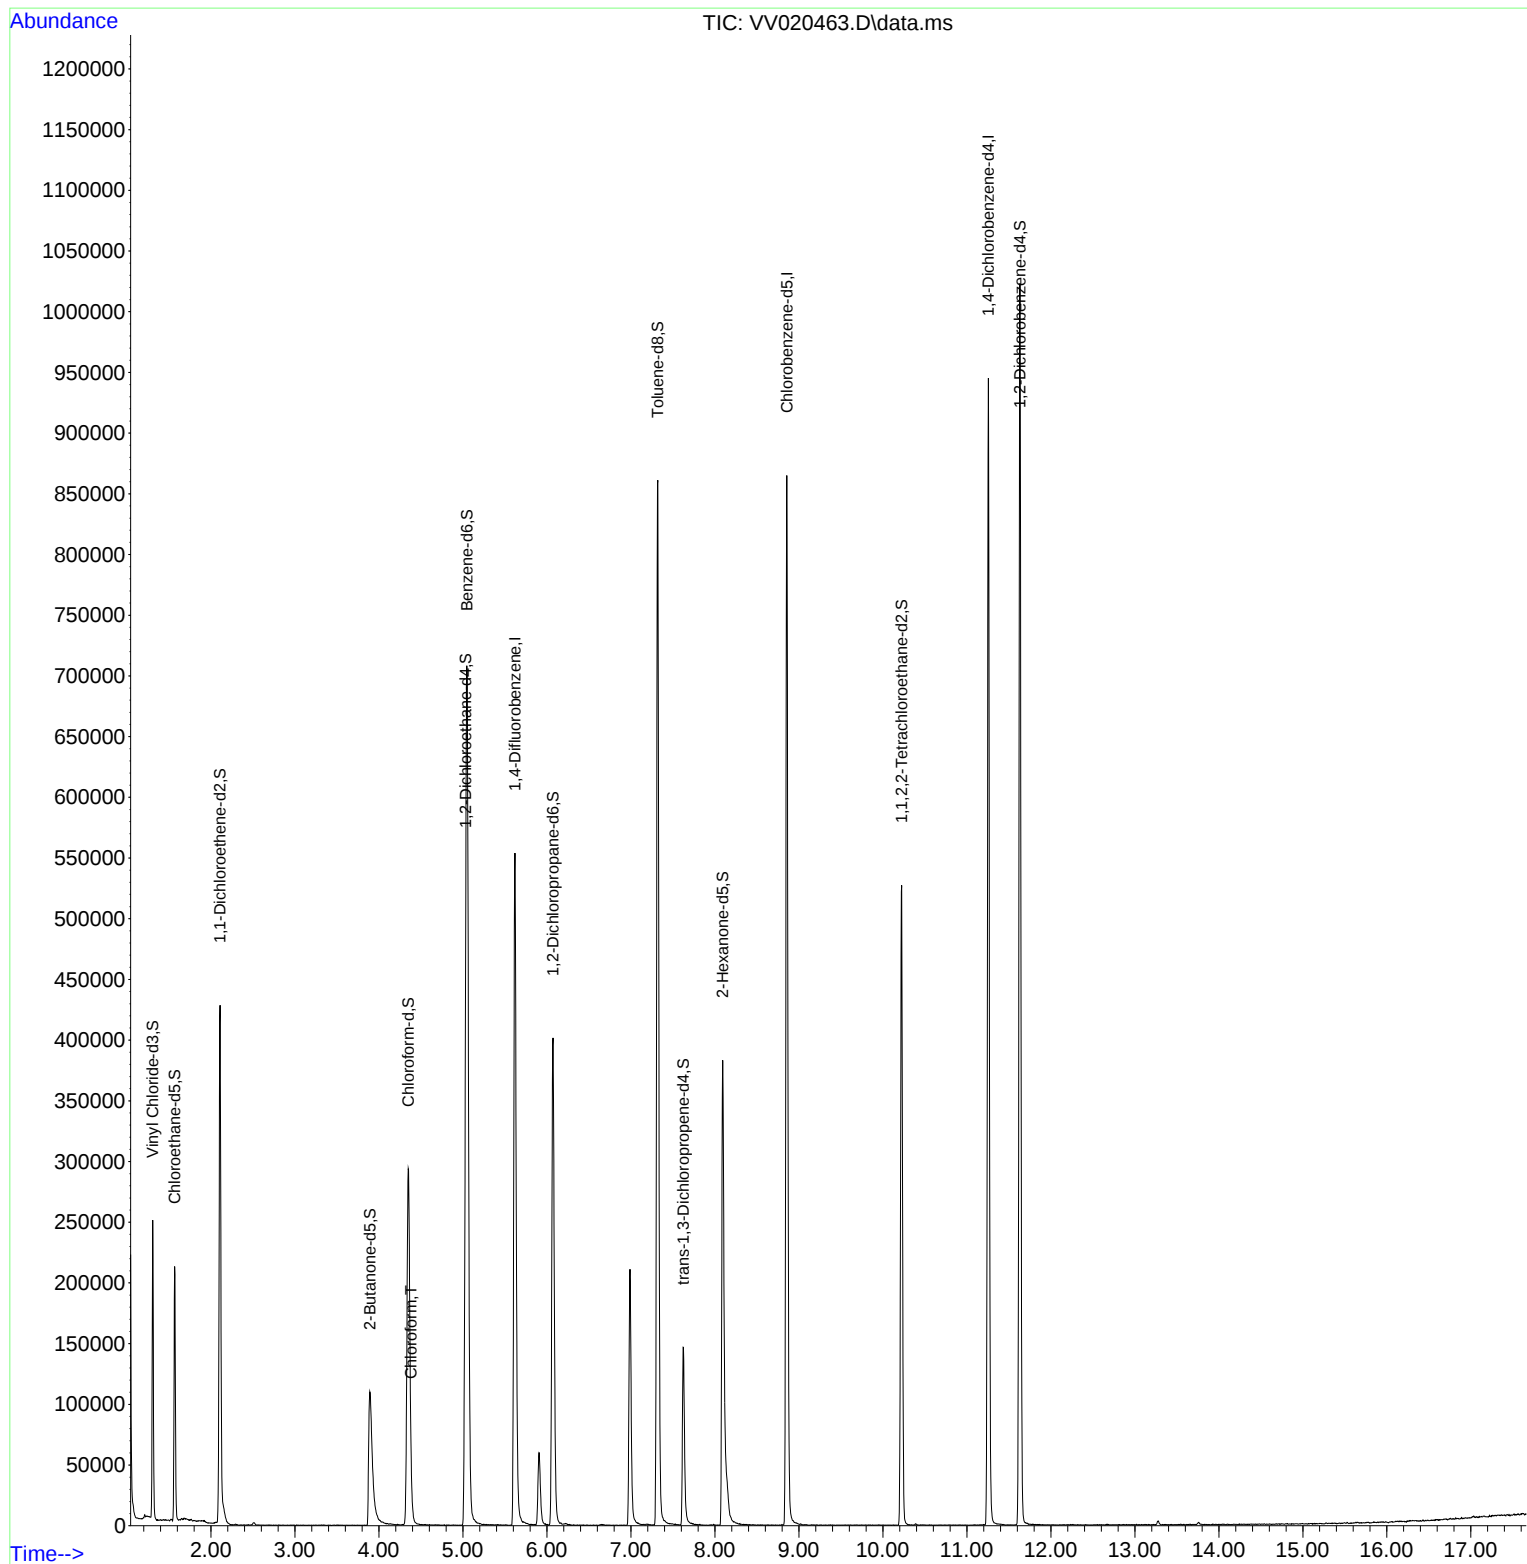

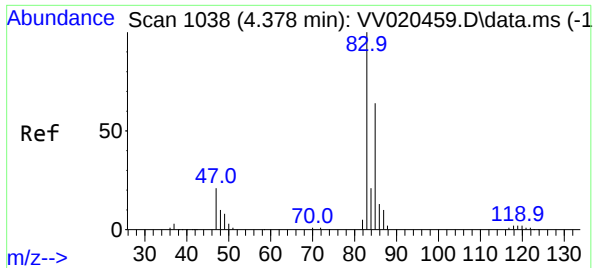

#25
Chloroform
Concen: 1.98 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VV020463.D
Acq: 04 Mar 2021 12:09

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tgt Ion: 83 Resp: 12189
Ion Ratio Lower Upper
83 100
85 72.9 44.2 82.2

