

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020444.D
 Acq On : 03 Mar 2021 13:38
 Operator : SY/MD
 Sample : VV0304WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	267981	272173	14.15%	1.820%
2	1.571	157	165	177	rBV	225148	258206	13.42%	1.727%
3	2.108	321	332	364	rVB	455616	695821	36.17%	4.653%
4	2.240	371	373	376	rBV	250	195	0.01%	0.001%
5	2.297	384	391	400	rVV2	1142	1984	0.10%	0.013%
6	2.342	402	405	411	rVB2	359	336	0.02%	0.002%
7	2.420	425	429	433	rBV2	265	231	0.01%	0.002%
8	2.510	449	457	469	rBV4	2530	4170	0.22%	0.028%
9	2.622	489	492	496	rVB2	292	241	0.01%	0.002%
10	2.645	496	499	502	rBV2	229	209	0.01%	0.001%
11	2.754	530	533	538	rVV2	312	246	0.01%	0.002%
12	2.780	538	541	545	rVB2	327	242	0.01%	0.002%
13	2.982	601	604	609	rVB2	309	261	0.01%	0.002%
14	3.024	613	617	622	rBV2	207	218	0.01%	0.001%
15	3.059	622	628	630	rBV	143	159	0.01%	0.001%
16	3.719	831	833	837	rVB2	238	154	0.01%	0.001%
17	3.757	837	845	848	rBV2	317	433	0.02%	0.003%
18	3.780	848	852	857	rBV	215	241	0.01%	0.002%
19	3.834	864	869	872	rBV	265	223	0.01%	0.001%
20	3.889	876	886	925	rBV	117593	358214	18.62%	2.395%
21	4.268	1002	1004	1008	rVB3	341	238	0.01%	0.002%
22	4.352	1013	1030	1063	rVV	308122	778092	40.45%	5.203%
23	4.728	1143	1147	1149	rBV	337	201	0.01%	0.001%
24	4.809	1168	1172	1175	rVV2	199	174	0.01%	0.001%
25	4.915	1197	1205	1209	rBV3	257	358	0.02%	0.002%
26	5.050	1230	1247	1288	rBV2	745535	1923805	100.00%	12.864%
27	5.413	1357	1360	1369	rBV3	560	622	0.03%	0.004%
28	5.458	1370	1374	1376	rVV2	263	171	0.01%	0.001%
29	5.474	1376	1379	1381	rVV3	330	181	0.01%	0.001%
30	5.503	1381	1388	1393	rVB4	343	411	0.02%	0.003%
31	5.619	1411	1424	1456	rBV	573045	1158803	60.23%	7.749%
32	5.831	1486	1490	1492	rBV2	423	329	0.02%	0.002%
33	5.908	1501	1514	1537	rBV2	59798	124385	6.47%	0.832%
34	6.072	1552	1565	1596	rBV	417391	850484	44.21%	5.687%
35	6.217	1606	1610	1613	rBV4	620	522	0.03%	0.003%
36	6.300	1635	1636	1643	rVB2	315	301	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020444.D
 Acq On : 03 Mar 2021 13:38
 Operator : SY/MD
 Sample : VV0304WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	6.352	1648	1652	1656	rBV3	269	280	0.01%	0.002%
38	6.509	1697	1701	1705	rBV2	185	171	0.01%	0.001%
39	6.567	1716	1719	1721	rBV	274	180	0.01%	0.001%
40	6.632	1736	1739	1741	rBV	372	238	0.01%	0.002%
41	6.683	1752	1755	1758	rBV2	234	169	0.01%	0.001%
42	6.789	1778	1788	1792	rBV2	345	450	0.02%	0.003%
43	6.989	1839	1850	1884	rBV	218881	403338	20.97%	2.697%
44	7.320	1940	1953	1985	rBV	911307	1576015	81.92%	10.539%
45	7.625	2037	2048	2086	rVV	154827	271750	14.13%	1.817%
46	7.808	2102	2105	2107	rBV2	490	369	0.02%	0.002%
47	7.886	2125	2129	2133	rVB3	602	479	0.02%	0.003%
48	7.972	2154	2156	2158	rBV	321	187	0.01%	0.001%
49	7.985	2158	2160	2166	rVB4	763	653	0.03%	0.004%
50	8.095	2183	2194	2230	rBV2	408927	836654	43.49%	5.595%
51	8.374	2278	2281	2282	rBV2	280	164	0.01%	0.001%
52	8.484	2313	2315	2321	rBB2	236	153	0.01%	0.001%
53	8.596	2347	2350	2353	rBV2	382	256	0.01%	0.002%
54	8.615	2353	2356	2358	rVV	413	209	0.01%	0.001%
55	8.857	2418	2431	2458	rBV	919629	1470248	76.42%	9.832%
56	9.030	2483	2485	2491	rVB3	816	592	0.03%	0.004%
57	9.159	2517	2525	2528	rBV3	918	847	0.04%	0.006%
58	9.275	2557	2561	2566	rVV2	349	307	0.02%	0.002%
59	9.336	2576	2580	2584	rBV2	235	289	0.02%	0.002%
60	9.397	2595	2599	2601	rBV	333	214	0.01%	0.001%
61	9.464	2616	2620	2623	rBV	181	162	0.01%	0.001%
62	9.558	2645	2649	2657	rVB2	388	470	0.02%	0.003%
63	9.593	2657	2660	2666	rBV	204	209	0.01%	0.001%
64	9.705	2692	2695	2699	rVB2	262	173	0.01%	0.001%
65	9.728	2699	2702	2710	rBV2	228	328	0.02%	0.002%
66	9.911	2753	2759	2760	rBV	232	188	0.01%	0.001%
67	10.040	2795	2799	2804	rBV2	215	244	0.01%	0.002%
68	10.130	2825	2827	2831	rVB	259	153	0.01%	0.001%
69	10.220	2843	2855	2878	rBV	546509	862760	44.85%	5.769%
70	10.377	2901	2904	2905	rBV	384	201	0.01%	0.001%
71	10.394	2905	2909	2914	rVB3	606	578	0.03%	0.004%
72	10.541	2952	2955	2958	rBV3	267	207	0.01%	0.001%
73	10.670	2991	2995	2998	rBV	227	204	0.01%	0.001%
74	10.760	3020	3023	3029	rVB3	374	283	0.01%	0.002%
75	10.795	3030	3034	3037	rBV2	270	246	0.01%	0.002%
76	10.863	3052	3055	3059	rVB2	317	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020444.D
 Acq On : 03 Mar 2021 13:38
 Operator : SY/MD
 Sample : VV0304WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

77	11.104	3127	3130	3132	rBV2	234	169	0.01%	0.001%
78	11.194	3153	3158	3165	rVB3	685	865	0.04%	0.006%
79	11.255	3165	3177	3209	rBV	963998	1478002	76.83%	9.883%
80	11.435	3229	3233	3236	rBV3	327	278	0.01%	0.002%
81	11.461	3238	3241	3244	rVV	418	258	0.01%	0.002%
82	11.548	3264	3268	3271	rBV2	304	165	0.01%	0.001%
83	11.570	3271	3275	3280	rBV2	267	273	0.01%	0.002%
84	11.631	3281	3294	3317	rBV	1035695	1599746	83.16%	10.697%
85	11.895	3373	3376	3378	rBV2	506	314	0.02%	0.002%
86	11.924	3382	3385	3390	rVB2	341	293	0.02%	0.002%
87	12.226	3476	3479	3482	rVB	339	204	0.01%	0.001%
88	12.258	3483	3489	3490	rBV	580	455	0.02%	0.003%
89	12.448	3543	3548	3557	rVB2	349	406	0.02%	0.003%
90	12.657	3609	3613	3622	rVB5	1456	1837	0.10%	0.012%
91	12.699	3624	3626	3629	rBV2	270	169	0.01%	0.001%
92	12.824	3663	3665	3667	rBV2	315	165	0.01%	0.001%
93	12.873	3675	3680	3683	rBV3	344	329	0.02%	0.002%
94	12.969	3707	3710	3714	rVB	354	224	0.01%	0.001%
95	13.172	3769	3773	3776	rBV2	281	207	0.01%	0.001%
96	13.191	3776	3779	3783	rVB	507	299	0.02%	0.002%
97	13.281	3799	3807	3818	rBV6	1627	2447	0.13%	0.016%
98	13.622	3910	3913	3916	rBV2	349	292	0.02%	0.002%
99	13.760	3949	3956	3964	rBV5	1704	2396	0.12%	0.016%
100	16.223	4720	4722	4725	rBV2	1138	711	0.04%	0.005%




Sum of corrected areas: 14954402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020444.D
Acq On : 03 Mar 2021 13:38
Operator : SY/MD
Sample : VV0304WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

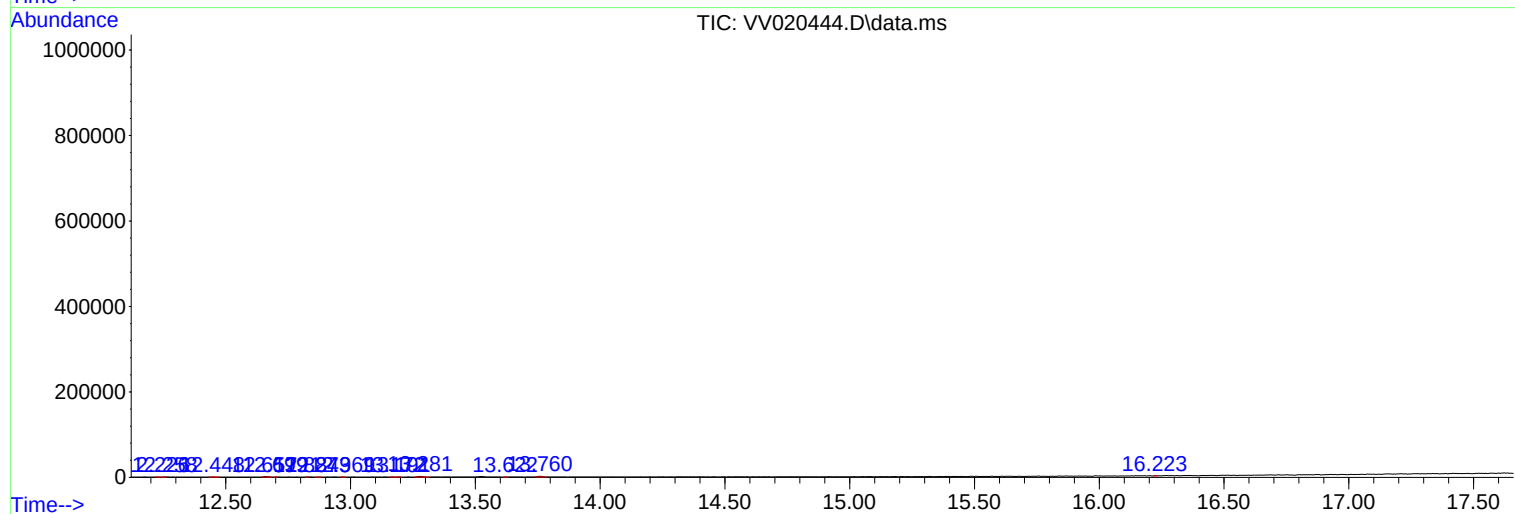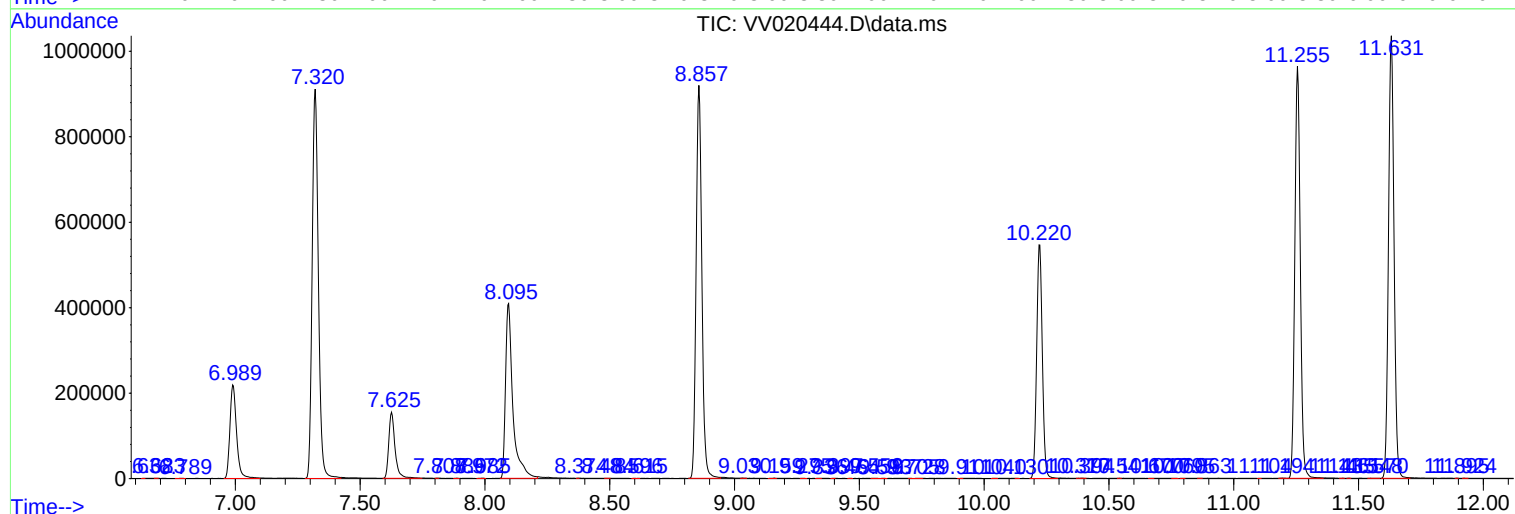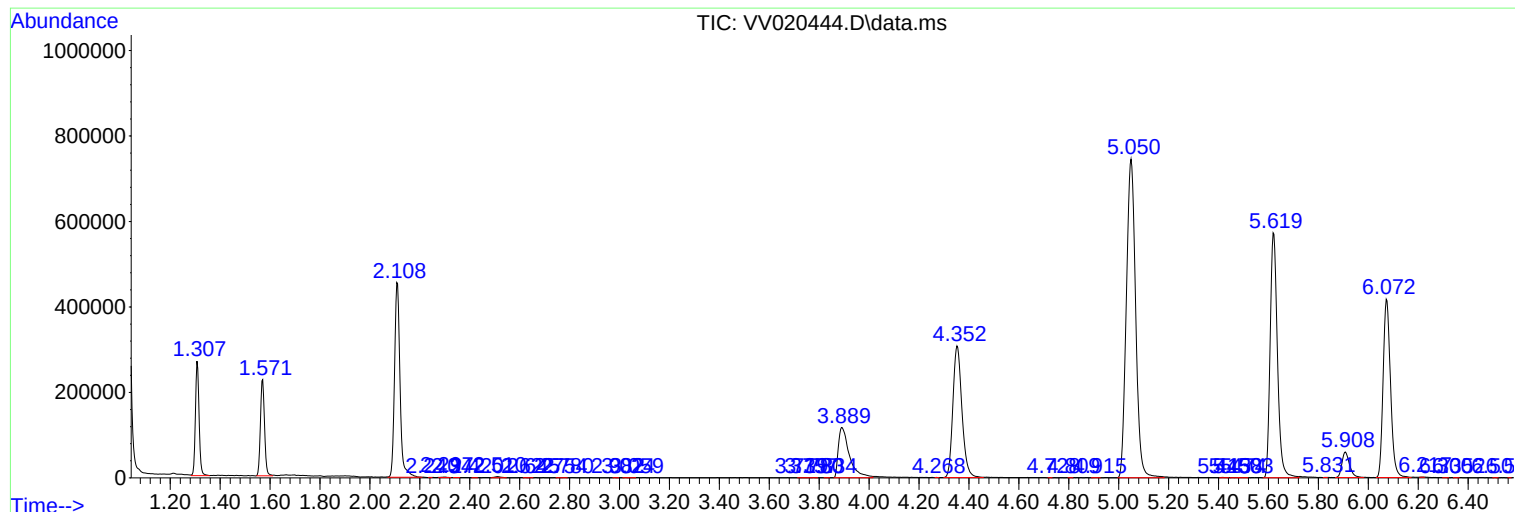

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020444.D
Acq On : 03 Mar 2021 13:38
Operator : SY/MD
Sample : VV0304WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020444.D
Acq On : 03 Mar 2021 13:38
Operator : SY/MD
Sample : VV0304WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
