

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020446.D
 Acq On : 03 Mar 2021 14:27
 Operator : SY/MD
 Sample : M1546-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	200531	201978	14.51%	1.805%
2	1.568	157	164	177	rVB	161998	185507	13.33%	1.658%
3	2.108	321	332	361	rVB	336441	507990	36.51%	4.540%
4	2.294	385	390	393	rVB3	353	321	0.02%	0.003%
5	2.426	427	431	434	rVB3	588	394	0.03%	0.004%
6	2.452	436	439	441	rBV2	504	271	0.02%	0.002%
7	2.507	451	456	465	rVB3	1211	1848	0.13%	0.017%
8	2.552	468	470	474	rBV2	300	208	0.01%	0.002%
9	2.619	481	491	501	rBV4	2118	4272	0.31%	0.038%
10	2.806	544	549	552	rBV2	307	289	0.02%	0.003%
11	2.925	583	586	591	rBV2	158	172	0.01%	0.002%
12	2.970	597	600	608	rVB2	235	292	0.02%	0.003%
13	3.063	627	629	637	rVB2	316	274	0.02%	0.002%
14	3.326	706	711	714	rVV2	189	206	0.01%	0.002%
15	3.352	715	719	723	rVV2	312	278	0.02%	0.002%
16	3.452	746	750	753	rVB3	266	230	0.02%	0.002%
17	3.645	806	810	813	rBV2	209	165	0.01%	0.001%
18	3.690	821	824	829	rVB2	176	160	0.01%	0.001%
19	3.725	830	835	839	rBV	171	167	0.01%	0.001%
20	3.902	871	890	930	rBV2	93726	349777	25.14%	3.126%
21	4.352	1013	1030	1058	rBV	223063	565722	40.65%	5.055%
22	4.622	1112	1114	1117	rVB2	284	179	0.01%	0.002%
23	4.712	1136	1142	1143	rBV3	311	290	0.02%	0.003%
24	4.761	1153	1157	1159	rBV	204	158	0.01%	0.001%
25	5.050	1229	1247	1280	rBV2	545702	1391530	100.00%	12.435%
26	5.188	1287	1290	1293	rVB3	638	405	0.03%	0.004%
27	5.275	1315	1317	1320	rVB2	443	194	0.01%	0.002%
28	5.384	1349	1351	1354	rVB	377	190	0.01%	0.002%
29	5.404	1354	1357	1360	rBV3	323	269	0.02%	0.002%
30	5.497	1382	1386	1388	rBV2	324	236	0.02%	0.002%
31	5.529	1394	1396	1399	rVB	338	171	0.01%	0.002%
32	5.548	1399	1402	1405	rBV2	213	163	0.01%	0.001%
33	5.619	1412	1424	1458	rBV	469029	944320	67.86%	8.439%
34	5.780	1472	1474	1479	rBV3	372	212	0.02%	0.002%
35	5.854	1495	1497	1501	rVB2	413	249	0.02%	0.002%
36	5.908	1501	1514	1536	rBV	63277	130446	9.37%	1.166%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020446.D
 Acq On : 03 Mar 2021 14:27
 Operator : SY/MD
 Sample : M1546-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1588	rBV	302597	612694	44.03%	5.475%
38	6.207	1605	1607	1609	rBV2	440	277	0.02%	0.002%
39	6.275	1625	1628	1632	rVB2	428	382	0.03%	0.003%
40	6.336	1645	1647	1650	rVB	296	188	0.01%	0.002%
41	6.394	1661	1665	1667	rBV2	272	241	0.02%	0.002%
42	6.436	1673	1678	1685	rVB2	228	291	0.02%	0.003%
43	6.603	1724	1730	1734	rBV2	194	264	0.02%	0.002%
44	6.841	1800	1804	1807	rBV2	260	192	0.01%	0.002%
45	6.915	1822	1827	1830	rVB2	192	189	0.01%	0.002%
46	6.989	1839	1850	1875	rBV	151505	280792	20.18%	2.509%
47	7.172	1905	1907	1912	rVB3	380	242	0.02%	0.002%
48	7.201	1912	1916	1917	rBV2	480	327	0.02%	0.003%
49	7.320	1940	1953	1986	rBV	646643	1123967	80.77%	10.044%
50	7.584	2029	2035	2037	rBV4	288	303	0.02%	0.003%
51	7.625	2037	2048	2071	rBV	104704	187855	13.50%	1.679%
52	7.944	2135	2147	2156	rVV3	4162	6980	0.50%	0.062%
53	8.095	2183	2194	2240	rBV2	242713	550940	39.59%	4.923%
54	8.352	2272	2274	2280	rVB4	317	280	0.02%	0.003%
55	8.458	2305	2307	2311	rVB2	324	161	0.01%	0.001%
56	8.484	2311	2315	2322	rBV2	480	436	0.03%	0.004%
57	8.526	2322	2328	2329	rBV	274	236	0.02%	0.002%
58	8.561	2335	2339	2342	rVB3	282	241	0.02%	0.002%
59	8.857	2419	2431	2473	rBV	739873	1204210	86.54%	10.761%
60	9.072	2495	2498	2499	rBV2	393	196	0.01%	0.002%
61	9.117	2509	2512	2520	rVB2	376	374	0.03%	0.003%
62	9.198	2533	2537	2541	rBV2	252	292	0.02%	0.003%
63	9.259	2552	2556	2558	rBV2	225	166	0.01%	0.001%
64	9.294	2564	2567	2572	rBV2	274	247	0.02%	0.002%
65	9.387	2592	2596	2602	rBV2	317	342	0.02%	0.003%
66	9.455	2615	2617	2622	rVB2	277	165	0.01%	0.001%
67	9.645	2671	2676	2680	rVB2	294	308	0.02%	0.003%
68	9.674	2682	2685	2689	rBV2	203	188	0.01%	0.002%
69	9.699	2689	2693	2697	rBV2	252	267	0.02%	0.002%
70	9.764	2710	2713	2717	rBV2	218	167	0.01%	0.001%
71	9.924	2759	2763	2766	rBV	257	179	0.01%	0.002%
72	9.950	2766	2771	2774	rBV2	317	309	0.02%	0.003%
73	10.018	2788	2792	2795	rBV2	181	173	0.01%	0.002%
74	10.220	2844	2855	2877	rVV	352061	552406	39.70%	4.936%
75	10.329	2885	2889	2893	rBV3	279	272	0.02%	0.002%
76	10.391	2899	2908	2918	rVB3	6852	11579	0.83%	0.103%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020446.D
 Acq On : 03 Mar 2021 14:27
 Operator : SY/MD
 Sample : M1546-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	10.837	3041	3047	3050	rBV2	286	314	0.02%	0.003%
78	11.030	3103	3107	3111	rBV	254	241	0.02%	0.002%
79	11.175	3148	3152	3155	rBV3	413	377	0.03%	0.003%
80	11.255	3165	3177	3207	rBV	782413	1205755	86.65%	10.775%
81	11.484	3246	3248	3252	rBV3	260	199	0.01%	0.002%
82	11.554	3266	3270	3273	rBV3	439	331	0.02%	0.003%
83	11.632	3281	3294	3318	rBV	722879	1145793	82.34%	10.239%
84	12.059	3421	3427	3430	rBV2	246	303	0.02%	0.003%
85	12.085	3432	3435	3438	rVV	283	181	0.01%	0.002%
86	12.265	3482	3491	3496	rVB2	1495	2362	0.17%	0.021%
87	12.374	3522	3525	3530	rBV2	388	397	0.03%	0.004%
88	12.635	3604	3606	3608	rBV	293	167	0.01%	0.001%
89	12.667	3612	3616	3621	rVB3	616	434	0.03%	0.004%
90	12.911	3689	3692	3695	rVV	254	173	0.01%	0.002%
91	12.931	3695	3698	3702	rVB2	353	284	0.02%	0.003%
92	13.021	3723	3726	3728	rBV2	287	177	0.01%	0.002%
93	13.281	3800	3807	3808	rBV3	862	741	0.05%	0.007%
94	13.609	3907	3909	3912	rBV2	302	161	0.01%	0.001%
95	13.660	3922	3925	3931	rBV3	289	192	0.01%	0.002%
96	13.760	3952	3956	3961	rVB2	921	811	0.06%	0.007%
97	13.786	3961	3964	3966	rBV2	305	188	0.01%	0.002%
98	14.496	4182	4185	4187	rBV	404	282	0.02%	0.003%
99	15.406	4466	4468	4471	rBV2	700	526	0.04%	0.005%
100	15.509	4497	4500	4506	rBV5	1182	1177	0.08%	0.011%




Sum of corrected areas: 11190417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020446.D
Acq On : 03 Mar 2021 14:27
Operator : SY/MD
Sample : M1546-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

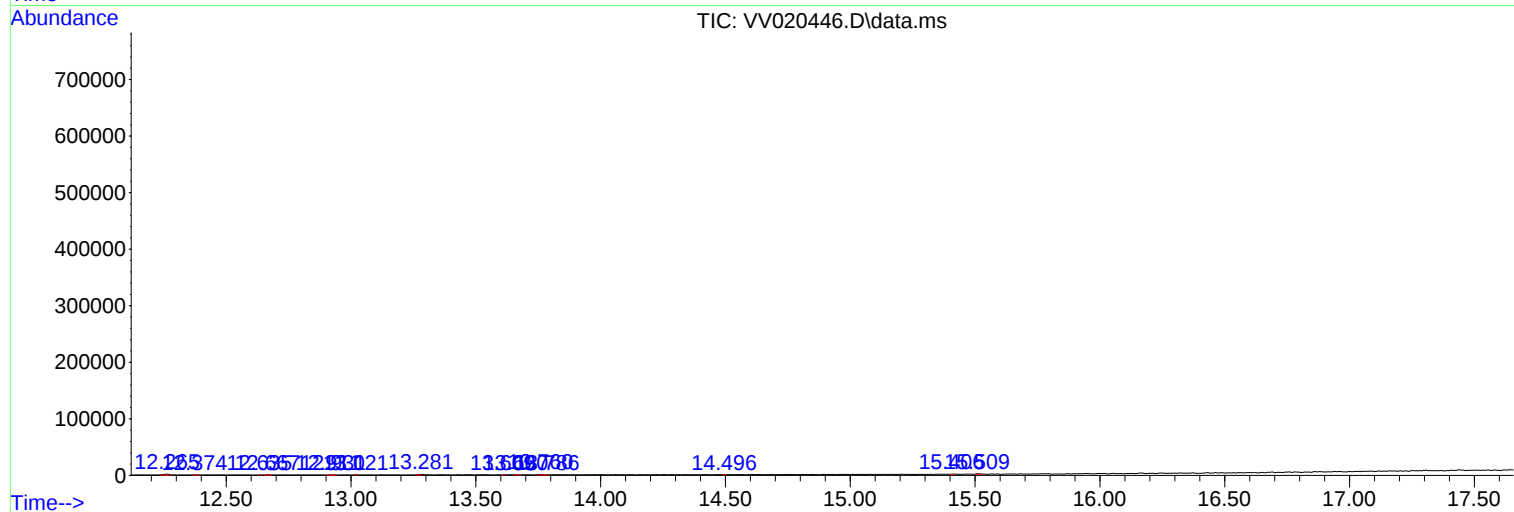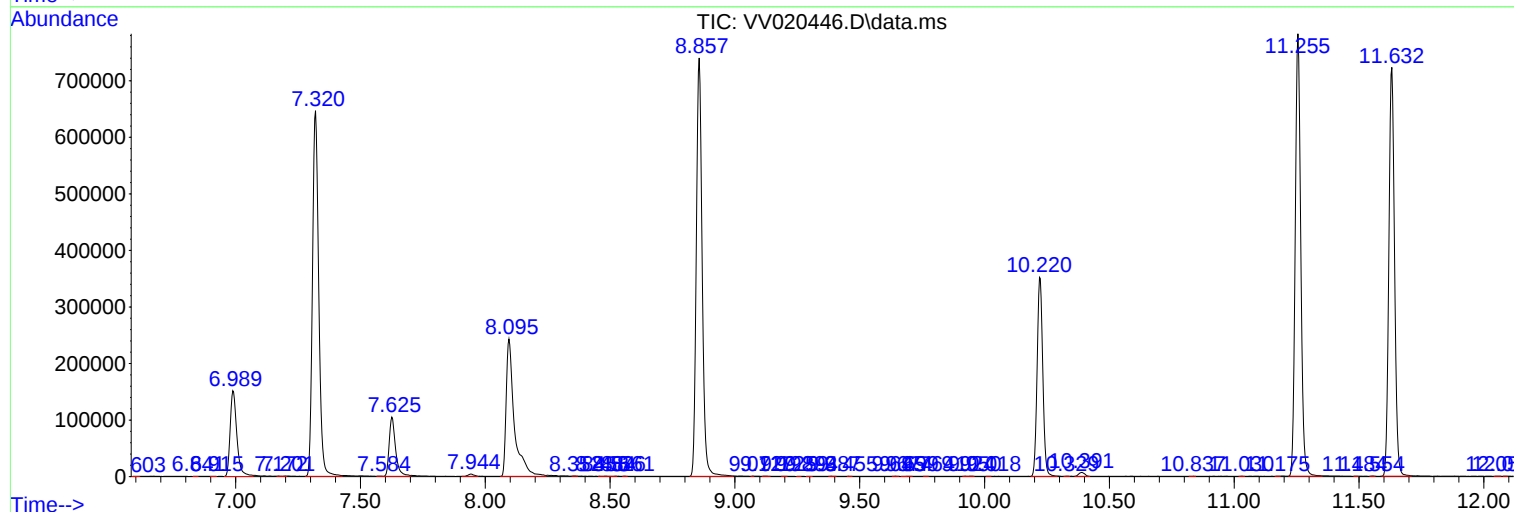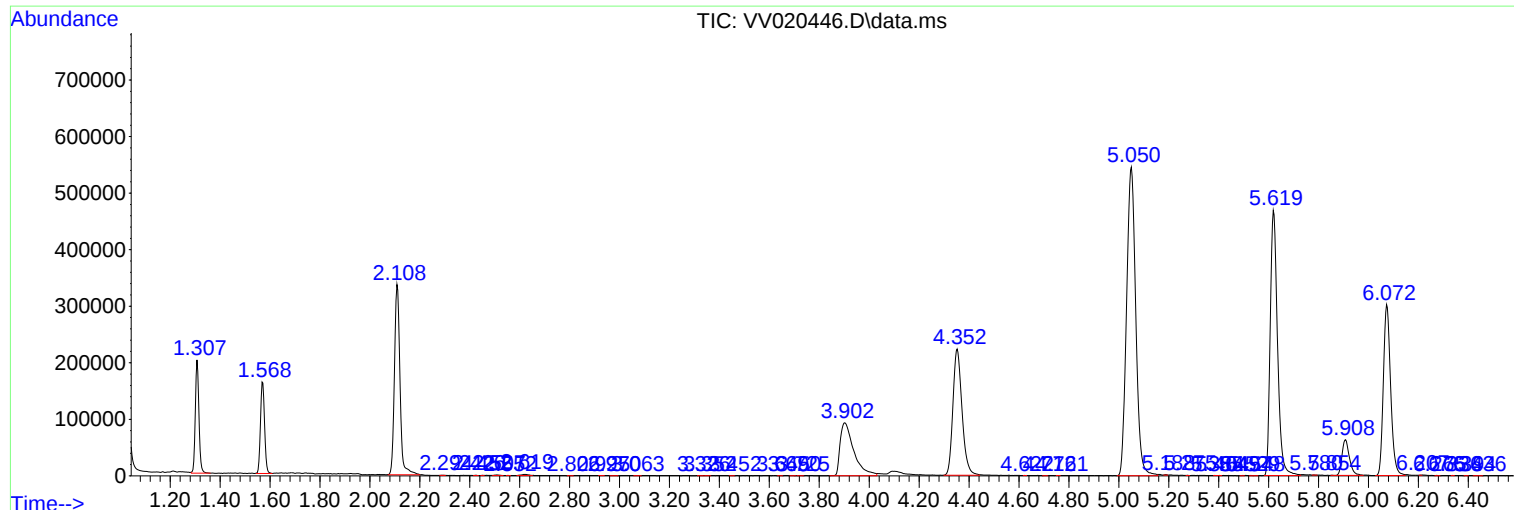

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020446.D
Acq On : 03 Mar 2021 14:27
Operator : SY/MD
Sample : M1546-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020446.D
Acq On : 03 Mar 2021 14:27
Operator : SY/MD
Sample : M1546-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
