

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020448.D
 Acq On : 03 Mar 2021 15:14
 Operator : SY/MD
 Sample : M1546-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	259126	258620	13.81%	1.764%
2	1.568	156	164	179	rBV	213747	245853	13.13%	1.677%
3	2.060	315	317	320	rVB4	850	459	0.02%	0.003%
4	2.108	321	332	363	rVV	445511	673648	35.97%	4.596%
5	2.291	386	389	391	rBV3	243	201	0.01%	0.001%
6	2.426	427	431	433	rBV2	206	169	0.01%	0.001%
7	2.442	433	436	439	rVB	271	183	0.01%	0.001%
8	2.510	451	457	469	rVB5	1280	1917	0.10%	0.013%
9	2.568	469	475	479	rBV2	143	222	0.01%	0.002%
10	2.619	481	491	506	rVV3	2701	5906	0.32%	0.040%
11	2.870	566	569	573	rVB	243	179	0.01%	0.001%
12	2.899	573	578	586	rBV	296	453	0.02%	0.003%
13	2.986	601	605	608	rVB2	342	234	0.01%	0.002%
14	3.005	608	611	613	rBV2	213	154	0.01%	0.001%
15	3.265	686	692	695	rBV2	282	342	0.02%	0.002%
16	3.384	725	729	732	rBV	175	169	0.01%	0.001%
17	3.494	760	763	766	rBV2	204	154	0.01%	0.001%
18	3.622	794	803	806	rBV	266	288	0.02%	0.002%
19	3.654	810	813	818	rBV2	188	188	0.01%	0.001%
20	3.683	818	822	826	rVB	221	160	0.01%	0.001%
21	3.716	829	832	838	rBV	229	257	0.01%	0.002%
22	3.896	876	888	935	rBV2	128944	447941	23.92%	3.056%
23	4.352	1013	1030	1058	rBV	308910	818477	43.71%	5.584%
24	4.712	1139	1142	1148	rVB2	515	415	0.02%	0.003%
25	4.777	1158	1162	1166	rBV2	304	257	0.01%	0.002%
26	4.806	1169	1171	1176	rVB	414	296	0.02%	0.002%
27	4.834	1176	1180	1184	rBV2	445	402	0.02%	0.003%
28	4.928	1201	1209	1212	rBV	504	504	0.03%	0.003%
29	5.050	1229	1247	1273	rBV2	731719	1872729	100.00%	12.775%
30	5.301	1324	1325	1330	rBV2	356	233	0.01%	0.002%
31	5.420	1358	1362	1363	rBV2	327	239	0.01%	0.002%
32	5.510	1386	1390	1391	rVV	230	179	0.01%	0.001%
33	5.619	1412	1424	1458	rBV	552016	1113979	59.48%	7.599%
34	5.908	1502	1514	1531	rBV2	75484	155384	8.30%	1.060%
35	6.072	1550	1565	1595	rBV	416363	833179	44.49%	5.684%
36	6.207	1605	1607	1608	rBV2	418	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020448.D
 Acq On : 03 Mar 2021 15:14
 Operator : SY/MD
 Sample : M1546-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.275	1624	1628	1632	rVB3	458	402	0.02%	0.003%
38	6.297	1632	1635	1637	rVB3	234	161	0.01%	0.001%
39	6.362	1651	1655	1660	rVB2	309	319	0.02%	0.002%
40	6.645	1734	1743	1749	rBV3	633	1028	0.05%	0.007%
41	6.677	1751	1753	1757	rVB3	441	308	0.02%	0.002%
42	6.773	1782	1783	1789	rVB2	255	210	0.01%	0.001%
43	6.802	1789	1792	1796	rBV2	200	193	0.01%	0.001%
44	6.989	1839	1850	1874	rBV	211760	384460	20.53%	2.623%
45	7.194	1908	1914	1915	rBV2	606	597	0.03%	0.004%
46	7.320	1941	1953	1994	rBV	882446	1529463	81.67%	10.434%
47	7.625	2037	2048	2079	rBV	151217	262238	14.00%	1.789%
48	7.783	2095	2097	2100	rVB3	438	189	0.01%	0.001%
49	7.815	2105	2107	2112	rVV3	670	315	0.02%	0.002%
50	7.838	2112	2114	2118	rVB3	410	289	0.02%	0.002%
51	7.860	2120	2121	2128	rVB2	320	214	0.01%	0.001%
52	7.940	2138	2146	2147	rBV2	1486	1491	0.08%	0.010%
53	7.985	2157	2160	2163	rVV3	609	376	0.02%	0.003%
54	8.095	2181	2194	2238	rBV2	377746	807127	43.10%	5.506%
55	8.378	2280	2282	2285	rVB2	317	203	0.01%	0.001%
56	8.403	2287	2290	2293	rVV2	373	249	0.01%	0.002%
57	8.442	2297	2302	2305	rBV3	338	332	0.02%	0.002%
58	8.493	2316	2318	2323	rBV3	197	166	0.01%	0.001%
59	8.596	2345	2350	2354	rBV2	255	282	0.02%	0.002%
60	8.686	2373	2378	2381	rBV	157	184	0.01%	0.001%
61	8.857	2418	2431	2455	rBV	877321	1416915	75.66%	9.666%
62	9.124	2509	2514	2517	rBV3	406	414	0.02%	0.003%
63	9.223	2542	2545	2549	rBV	359	274	0.01%	0.002%
64	9.362	2586	2588	2595	rVB2	337	271	0.01%	0.002%
65	9.439	2608	2612	2615	rBV2	188	167	0.01%	0.001%
66	9.731	2700	2703	2708	rBV2	364	365	0.02%	0.002%
67	9.815	2726	2729	2734	rVV	206	175	0.01%	0.001%
68	9.944	2766	2769	2771	rVB2	275	161	0.01%	0.001%
69	10.223	2842	2856	2875	rBV	502471	792187	42.30%	5.404%
70	10.391	2898	2908	2919	rVB2	2419	4202	0.22%	0.029%
71	10.686	2997	3000	3003	rBV	204	155	0.01%	0.001%
72	10.747	3015	3019	3023	rBV2	198	190	0.01%	0.001%
73	10.831	3042	3045	3047	rBV	224	161	0.01%	0.001%
74	10.911	3066	3070	3073	rBV2	308	256	0.01%	0.002%
75	11.011	3096	3101	3106	rVB2	240	286	0.02%	0.002%
76	11.040	3107	3110	3113	rBV2	173	158	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020448.D
 Acq On : 03 Mar 2021 15:14
 Operator : SY/MD
 Sample : M1546-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.255	3165	3177	3201	rBV	934267	1421067	75.88%	9.694%
78	11.490	3248	3250	3253	rBV2	259	202	0.01%	0.001%
79	11.574	3273	3276	3280	rVB2	188	174	0.01%	0.001%
80	11.632	3280	3294	3316	rBV	999726	1584415	84.60%	10.809%
81	11.966	3395	3398	3400	rBV	272	177	0.01%	0.001%
82	12.001	3404	3409	3411	rBV3	311	315	0.02%	0.002%
83	12.030	3415	3418	3420	rBV	354	213	0.01%	0.001%
84	12.361	3516	3521	3523	rBV	368	381	0.02%	0.003%
85	12.487	3552	3560	3563	rBV2	481	542	0.03%	0.004%
86	12.532	3570	3574	3582	rBV2	409	535	0.03%	0.004%
87	12.619	3598	3601	3604	rBV3	363	213	0.01%	0.001%
88	12.657	3611	3613	3620	rVB3	373	342	0.02%	0.002%
89	12.699	3623	3626	3630	rVV	265	216	0.01%	0.001%
90	12.744	3637	3640	3643	rBV2	341	260	0.01%	0.002%
91	12.866	3676	3678	3681	rVB	418	156	0.01%	0.001%
92	12.908	3688	3691	3695	rBV	363	363	0.02%	0.002%
93	13.114	3752	3755	3756	rBV	280	165	0.01%	0.001%
94	13.246	3793	3796	3798	rBV2	305	206	0.01%	0.001%
95	13.275	3798	3805	3818	rVB6	2445	4271	0.23%	0.029%
96	13.326	3818	3821	3825	rBV	363	264	0.01%	0.002%
97	13.760	3950	3956	3962	rBV3	1375	1715	0.09%	0.012%
98	14.754	4261	4265	4269	rBV3	539	612	0.03%	0.004%
99	14.840	4290	4292	4295	rBV2	390	218	0.01%	0.001%
100	15.866	4609	4611	4615	rBV3	852	536	0.03%	0.004%

Sum of corrected areas: 14658833




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020448.D
Acq On : 03 Mar 2021 15:14
Operator : SY/MD
Sample : M1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

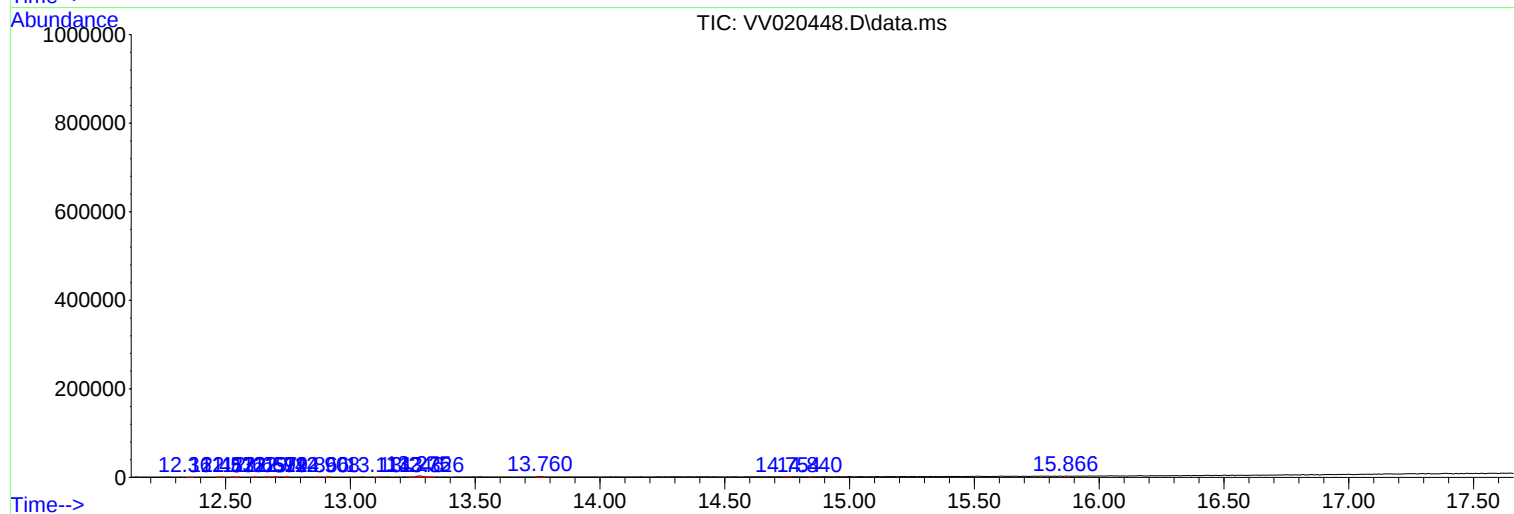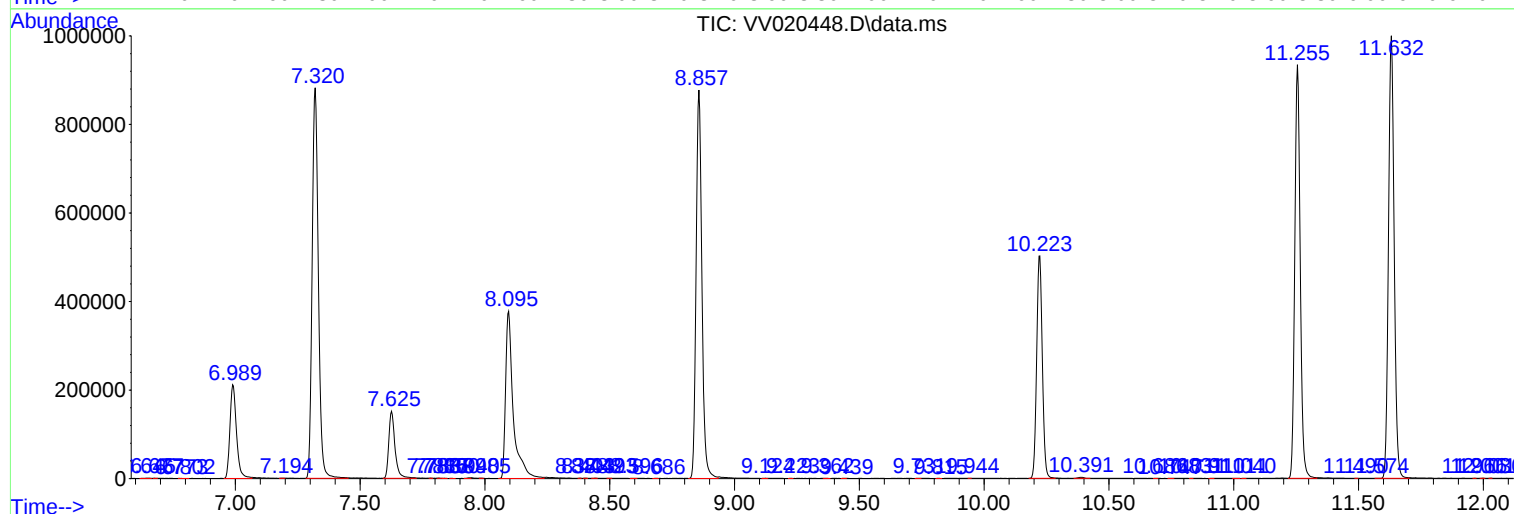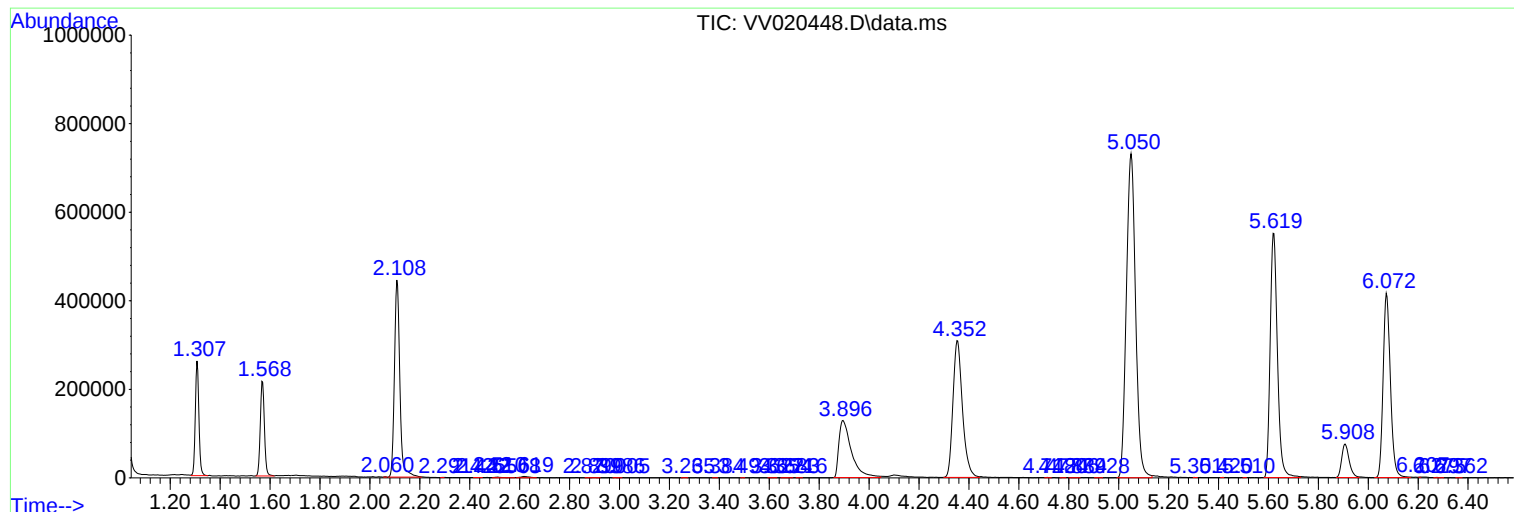

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020448.D
Acq On : 03 Mar 2021 15:14
Operator : SY/MD
Sample : M1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020448.D
Acq On : 03 Mar 2021 15:14
Operator : SY/MD
Sample : M1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
