

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020449.D
 Acq On : 03 Mar 2021 15:38
 Operator : SY/MD
 Sample : M1546-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	248340	252396	13.64%	1.751%
2	1.568	156	164	176	rBV	216478	247775	13.39%	1.719%
3	2.108	321	332	365	rVB	443257	665794	35.98%	4.620%
4	2.304	391	393	397	rVB	578	300	0.02%	0.002%
5	2.449	435	438	441	rBV2	326	236	0.01%	0.002%
6	2.507	451	456	465	rVB4	1163	1700	0.09%	0.012%
7	2.619	479	491	509	rBV2	3294	7956	0.43%	0.055%
8	2.700	513	516	520	rVV2	193	159	0.01%	0.001%
9	2.748	528	531	538	rVB2	147	157	0.01%	0.001%
10	2.786	538	543	546	rBV2	301	247	0.01%	0.002%
11	2.966	594	599	601	rBV2	345	285	0.02%	0.002%
12	3.114	642	645	649	rVB	256	166	0.01%	0.001%
13	3.291	698	700	704	rVB2	354	201	0.01%	0.001%
14	3.433	739	744	750	rVB	395	397	0.02%	0.003%
15	3.558	779	783	784	rBV	261	161	0.01%	0.001%
16	3.619	798	802	805	rBV	219	159	0.01%	0.001%
17	3.661	810	815	818	rBV	177	184	0.01%	0.001%
18	3.896	874	888	924	rBV3	128105	443337	23.95%	3.076%
19	4.352	1012	1030	1063	rBV	297034	753982	40.74%	5.232%
20	4.516	1079	1081	1085	rBV4	363	234	0.01%	0.002%
21	4.613	1107	1111	1117	rBV3	503	527	0.03%	0.004%
22	4.680	1128	1132	1135	rBV3	232	193	0.01%	0.001%
23	4.699	1135	1138	1141	rBV	279	208	0.01%	0.001%
24	4.738	1148	1150	1153	rVB3	363	161	0.01%	0.001%
25	4.809	1168	1172	1177	rVV3	324	269	0.01%	0.002%
26	4.889	1192	1197	1200	rBV2	329	296	0.02%	0.002%
27	4.941	1210	1213	1217	rVB	303	180	0.01%	0.001%
28	4.989	1222	1228	1230	rBV2	251	195	0.01%	0.001%
29	5.050	1230	1247	1270	rBV2	725457	1850711	100.00%	12.842%
30	5.243	1304	1307	1309	rBV2	391	282	0.02%	0.002%
31	5.442	1366	1369	1373	rVB2	263	158	0.01%	0.001%
32	5.484	1378	1382	1390	rBV3	464	701	0.04%	0.005%
33	5.619	1412	1424	1454	rBV	548897	1107196	59.83%	7.683%
34	5.905	1500	1513	1533	rBV2	75100	155425	8.40%	1.078%
35	6.072	1551	1565	1601	rBV	401935	822969	44.47%	5.710%
36	6.195	1601	1603	1605	rBV2	375	223	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020449.D
 Acq On : 03 Mar 2021 15:38
 Operator : SY/MD
 Sample : M1546-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.368	1654	1657	1661	rVB	408	232	0.01%	0.002%
38	6.465	1684	1687	1690	rBV2	209	160	0.01%	0.001%
39	6.654	1737	1746	1753	rBV4	622	1031	0.06%	0.007%
40	6.989	1838	1850	1879	rBV	209978	382825	20.69%	2.656%
41	7.137	1894	1896	1902	rVB4	547	520	0.03%	0.004%
42	7.320	1940	1953	1974	rBV	869578	1507394	81.45%	10.460%
43	7.625	2038	2048	2079	rBV	147976	258817	13.98%	1.796%
44	7.805	2101	2104	2105	rBV	345	224	0.01%	0.002%
45	7.944	2138	2147	2156	rBV2	1917	3325	0.18%	0.023%
46	7.979	2156	2158	2161	rVV3	474	217	0.01%	0.002%
47	8.095	2183	2194	2243	rBV2	374850	797009	43.07%	5.530%
48	8.381	2281	2283	2286	rBV2	277	167	0.01%	0.001%
49	8.439	2299	2301	2304	rVB	429	178	0.01%	0.001%
50	8.468	2308	2310	2317	rVB3	283	313	0.02%	0.002%
51	8.500	2317	2320	2322	rBV	419	249	0.01%	0.002%
52	8.529	2327	2329	2333	rVB2	433	269	0.01%	0.002%
53	8.551	2333	2336	2337	rBV2	508	247	0.01%	0.002%
54	8.600	2347	2351	2353	rVB2	280	225	0.01%	0.002%
55	8.619	2353	2357	2361	rBV2	193	198	0.01%	0.001%
56	8.664	2367	2371	2376	rBV3	255	254	0.01%	0.002%
57	8.857	2419	2431	2464	rBV	864696	1398594	75.57%	9.705%
58	9.075	2497	2499	2503	rVB2	387	183	0.01%	0.001%
59	9.111	2508	2510	2513	rBV	326	166	0.01%	0.001%
60	9.159	2519	2525	2530	rVB4	348	404	0.02%	0.003%
61	9.259	2552	2556	2559	rVB2	320	247	0.01%	0.002%
62	9.368	2586	2590	2595	rVB2	189	183	0.01%	0.001%
63	9.436	2609	2611	2615	rVV2	241	168	0.01%	0.001%
64	9.471	2619	2622	2625	rVB	259	168	0.01%	0.001%
65	9.712	2694	2697	2702	rBV	276	235	0.01%	0.002%
66	9.760	2709	2712	2716	rBV2	176	161	0.01%	0.001%
67	9.886	2748	2751	2758	rBV2	172	211	0.01%	0.001%
68	9.995	2775	2785	2789	rBV2	262	428	0.02%	0.003%
69	10.223	2843	2856	2876	rBV	500585	787217	42.54%	5.462%
70	10.391	2901	2908	2923	rVB4	3051	4646	0.25%	0.032%
71	10.542	2953	2955	2960	rVV2	223	169	0.01%	0.001%
72	10.593	2969	2971	2979	rVB	282	245	0.01%	0.002%
73	10.799	3031	3035	3042	rBV2	219	251	0.01%	0.002%
74	11.182	3148	3154	3156	rBV2	458	454	0.02%	0.003%
75	11.255	3165	3177	3202	rBV	898916	1391511	75.19%	9.655%
76	11.400	3220	3222	3225	rBV2	384	214	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020449.D
 Acq On : 03 Mar 2021 15:38
 Operator : SY/MD
 Sample : M1546-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.545	3263	3267	3271	rBV2	594	522	0.03%	0.004%
78	11.632	3281	3294	3319	rBV	987384	1548314	83.66%	10.743%
79	11.905	3377	3379	3384	rVV2	448	284	0.02%	0.002%
80	11.931	3385	3387	3391	rVB3	304	163	0.01%	0.001%
81	11.956	3391	3395	3400	rVB2	245	223	0.01%	0.002%
82	11.998	3400	3408	3411	rBV3	392	561	0.03%	0.004%
83	12.017	3411	3414	3418	rVV	272	188	0.01%	0.001%
84	12.085	3433	3435	3441	rVB3	292	207	0.01%	0.001%
85	12.143	3451	3453	3458	rVB2	294	179	0.01%	0.001%
86	12.230	3478	3480	3482	rBV2	300	156	0.01%	0.001%
87	12.481	3552	3558	3560	rBV2	341	389	0.02%	0.003%
88	12.638	3605	3607	3610	rVB3	309	161	0.01%	0.001%
89	12.661	3611	3614	3622	rVB	481	384	0.02%	0.003%
90	12.940	3696	3701	3703	rBV2	279	266	0.01%	0.002%
91	13.075	3740	3743	3747	rVB	589	382	0.02%	0.003%
92	13.133	3758	3761	3762	rBV2	271	152	0.01%	0.001%
93	13.191	3774	3779	3781	rBV2	458	422	0.02%	0.003%
94	13.271	3801	3804	3805	rBV2	580	377	0.02%	0.003%
95	13.281	3805	3807	3813	rVB2	904	573	0.03%	0.004%
96	13.461	3859	3863	3865	rBV	465	290	0.02%	0.002%
97	14.374	4145	4147	4151	rBV2	399	186	0.01%	0.001%
98	14.406	4155	4157	4159	rBV2	339	160	0.01%	0.001%
99	15.130	4379	4382	4385	rBV3	579	491	0.03%	0.003%
100	15.513	4496	4501	4504	rBV3	1430	1383	0.07%	0.010%




Sum of corrected areas: 14411642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020449.D
Acq On : 03 Mar 2021 15:38
Operator : SY/MD
Sample : M1546-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

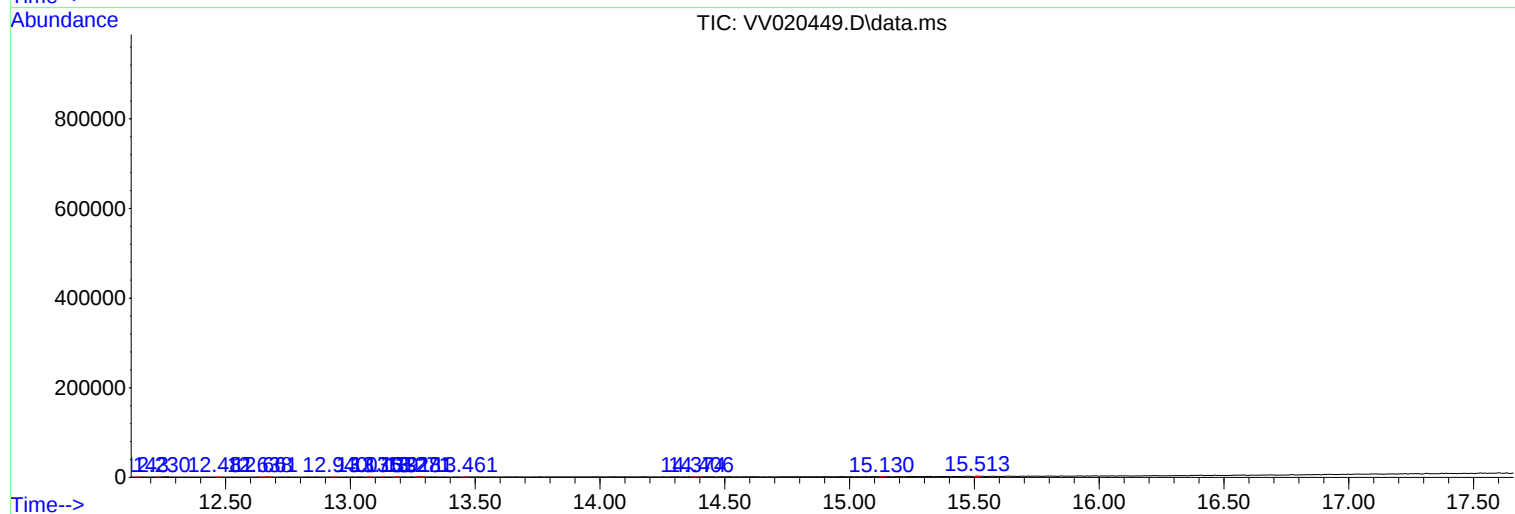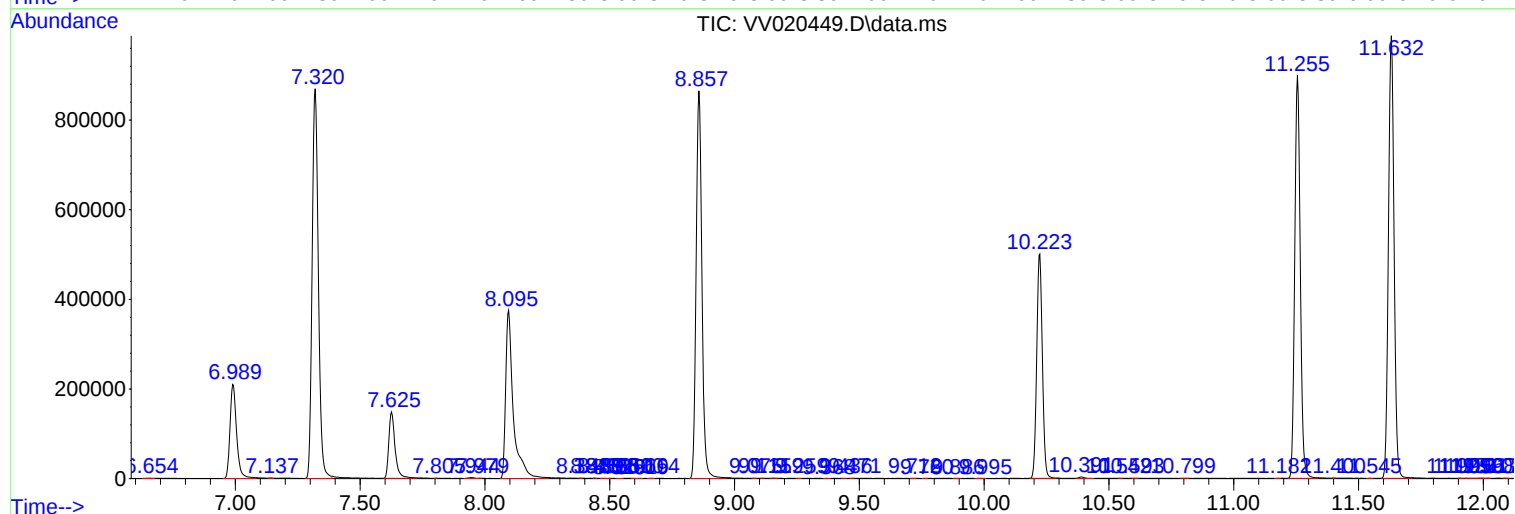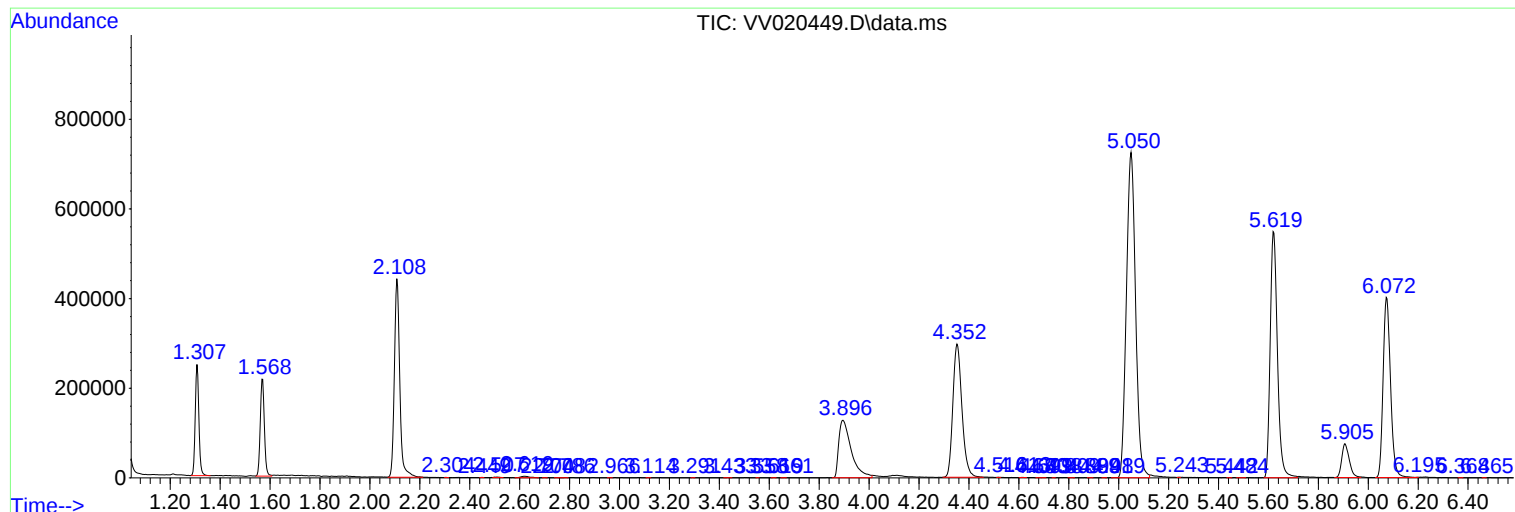

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020449.D
Acq On : 03 Mar 2021 15:38
Operator : SY/MD
Sample : M1546-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020449.D
Acq On : 03 Mar 2021 15:38
Operator : SY/MD
Sample : M1546-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------