

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020450.D
 Acq On : 03 Mar 2021 16:02
 Operator : SY/MD
 Sample : M1546-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	246530	249683	2.76%	0.886%
2	1.568	156	164	178	rBV	215178	242850	2.68%	0.862%
3	2.108	320	332	349	rBV	432601	643819	7.12%	2.285%
4	2.507	451	456	464	rVB3	1054	1530	0.02%	0.005%
5	2.552	468	470	476	rVB3	244	162	0.00%	0.001%
6	2.619	479	491	502	rVB4	2026	3983	0.04%	0.014%
7	2.860	560	566	568	rBV2	147	168	0.00%	0.001%
8	2.892	572	576	582	rBV2	215	260	0.00%	0.001%
9	3.073	630	632	636	rVB2	310	212	0.00%	0.001%
10	3.381	724	728	733	rBB2	161	162	0.00%	0.001%
11	3.619	797	802	805	rBV2	189	194	0.00%	0.001%
12	3.687	819	823	826	rBV2	182	169	0.00%	0.001%
13	3.892	873	887	928	rBV2	129603	439480	4.86%	1.559%
14	4.352	1013	1030	1062	rVV	294166	743687	8.22%	2.639%
15	4.580	1098	1101	1103	rVB	365	234	0.00%	0.001%
16	4.600	1103	1107	1109	rBV3	395	308	0.00%	0.001%
17	4.613	1109	1111	1115	rVB3	319	205	0.00%	0.001%
18	4.671	1127	1129	1132	rVB3	475	323	0.00%	0.001%
19	4.699	1132	1138	1139	rBV2	257	270	0.00%	0.001%
20	4.786	1162	1165	1169	rVV3	234	179	0.00%	0.001%
21	5.050	1229	1247	1283	rBV2	715175	1889317	20.88%	6.704%
22	5.246	1306	1308	1310	rBV2	292	163	0.00%	0.001%
23	5.352	1339	1341	1347	rBV2	336	274	0.00%	0.001%
24	5.404	1354	1357	1361	rBV	184	181	0.00%	0.001%
25	5.494	1381	1385	1390	rVV3	348	355	0.00%	0.001%
26	5.619	1410	1424	1455	rBV	532006	1064066	11.76%	3.776%
27	5.857	1495	1498	1500	rBV3	311	182	0.00%	0.001%
28	5.908	1501	1514	1534	rBV	52114	108002	1.19%	0.383%
29	6.002	1541	1543	1549	rVB3	675	567	0.01%	0.002%
30	6.072	1549	1565	1592	rBV	400079	808411	8.94%	2.869%
31	6.207	1604	1607	1610	rBV3	842	599	0.01%	0.002%
32	6.256	1620	1622	1630	rVB3	929	964	0.01%	0.003%
33	6.516	1699	1703	1707	rBV2	363	312	0.00%	0.001%
34	6.638	1734	1741	1746	rBV3	764	997	0.01%	0.004%
35	6.664	1746	1749	1752	rVB2	251	184	0.00%	0.001%
36	6.703	1758	1761	1765	rBV	341	261	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020450.D
 Acq On : 03 Mar 2021 16:02
 Operator : SY/MD
 Sample : M1546-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.754	1775	1777	1778	rBV	407	162	0.00%	0.001%
38	6.786	1785	1787	1791	rVB2	240	189	0.00%	0.001%
39	6.812	1791	1795	1798	rBV2	436	473	0.01%	0.002%
40	6.989	1839	1850	1876	rBV	209492	376078	4.16%	1.335%
41	7.185	1908	1911	1915	rBV3	648	538	0.01%	0.002%
42	7.243	1927	1929	1933	rVB2	477	292	0.00%	0.001%
43	7.262	1933	1935	1938	rVB	425	228	0.00%	0.001%
44	7.320	1939	1953	1988	rBV	872976	1504862	16.63%	5.340%
45	7.625	2035	2048	2073	rBV	145992	256227	2.83%	0.909%
46	7.773	2093	2094	2097	rVB	505	174	0.00%	0.001%
47	7.802	2102	2103	2106	rBV2	382	253	0.00%	0.001%
48	7.822	2107	2109	2111	rVB2	444	202	0.00%	0.001%
49	7.838	2111	2114	2117	rVB2	253	182	0.00%	0.001%
50	7.870	2117	2124	2128	rVB3	446	419	0.00%	0.001%
51	7.892	2128	2131	2137	rVB3	255	268	0.00%	0.001%
52	7.928	2138	2142	2144	rBV	471	384	0.00%	0.001%
53	7.985	2156	2160	2163	rVB2	609	422	0.00%	0.001%
54	8.092	2182	2193	2233	rBV2	404924	798202	8.82%	2.832%
55	8.539	2330	2332	2335	rBV2	371	206	0.00%	0.001%
56	8.857	2419	2431	2435	rBV	880157	1364220	15.08%	4.841%
57	9.104	2506	2508	2511	rVB2	411	223	0.00%	0.001%
58	9.149	2520	2522	2523	rBV2	376	167	0.00%	0.001%
59	9.284	2560	2564	2571	rBV2	191	302	0.00%	0.001%
60	9.320	2573	2575	2579	rVB3	355	187	0.00%	0.001%
61	9.342	2580	2582	2591	rVB2	238	240	0.00%	0.001%
62	9.394	2595	2598	2604	rBV2	327	317	0.00%	0.001%
63	9.506	2630	2633	2640	rVB2	311	311	0.00%	0.001%
64	9.702	2689	2694	2699	rBV2	214	250	0.00%	0.001%
65	9.953	2768	2772	2779	rVB3	407	491	0.01%	0.002%
66	10.220	2843	2855	2877	rBV	524623	835886	9.24%	2.966%
67	10.391	2900	2908	2917	rBV3	1298	1927	0.02%	0.007%
68	10.551	2955	2958	2960	rVB	369	200	0.00%	0.001%
69	10.706	3002	3006	3008	rBV	290	189	0.00%	0.001%
70	10.725	3009	3012	3017	rVV	257	234	0.00%	0.001%
71	10.892	3060	3064	3067	rVV2	188	187	0.00%	0.001%
72	10.934	3073	3077	3080	rVB	344	274	0.00%	0.001%
73	11.011	3098	3101	3104	rBV	219	160	0.00%	0.001%
74	11.188	3145	3156	3166	rBV	180014	274881	3.04%	0.975%
75	11.278	3166	3184	3205	rVB2	1769094	3967906	43.86%	14.080%
76	11.548	3266	3268	3275	rVB3	351	197	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020450.D
 Acq On : 03 Mar 2021 16:02
 Operator : SY/MD
 Sample : M1546-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.648	3280	3299	3326	rBV3	5101352	9047559	100.00%	32.105%
78	11.815	3349	3351	3356	rVB3	860	633	0.01%	0.002%
79	11.918	3381	3383	3387	rVB3	565	373	0.00%	0.001%
80	12.024	3414	3416	3421	rVB2	351	240	0.00%	0.001%
81	12.114	3440	3444	3449	rBV5	513	580	0.01%	0.002%
82	12.194	3466	3469	3471	rBV	278	169	0.00%	0.001%
83	12.304	3500	3503	3506	rBV	344	226	0.00%	0.001%
84	12.326	3508	3510	3514	rBV2	246	182	0.00%	0.001%
85	12.371	3521	3524	3527	rBV2	311	219	0.00%	0.001%
86	12.407	3527	3535	3547	rVB3	8109	12231	0.14%	0.043%
87	12.564	3581	3584	3587	rBV2	347	216	0.00%	0.001%
88	12.583	3588	3590	3593	rVB	372	214	0.00%	0.001%
89	12.644	3600	3609	3629	rBV2	39314	67614	0.75%	0.240%
90	12.757	3636	3644	3654	rVB2	9874	14623	0.16%	0.052%
91	12.853	3672	3674	3679	rBV2	427	251	0.00%	0.001%
92	13.220	3784	3788	3790	rBV3	720	458	0.01%	0.002%
93	13.268	3791	3803	3831	rVV	1423056	2159309	23.87%	7.662%
94	13.519	3876	3881	3893	rVB6	1697	2897	0.03%	0.010%
95	13.754	3941	3954	3975	rBV	687669	1077522	11.91%	3.824%
96	14.156	4071	4079	4092	rBV3	11592	18781	0.21%	0.067%
97	14.654	4231	4234	4235	rBV2	607	365	0.00%	0.001%
98	14.831	4277	4289	4302	rVB2	18911	30649	0.34%	0.109%
99	14.950	4323	4326	4327	rBV3	524	252	0.00%	0.001%
100	15.406	4458	4468	4485	rVB	98926	154099	1.70%	0.547%




Sum of corrected areas: 28180885

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020450.D
Acq On : 03 Mar 2021 16:02
Operator : SY/MD
Sample : M1546-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

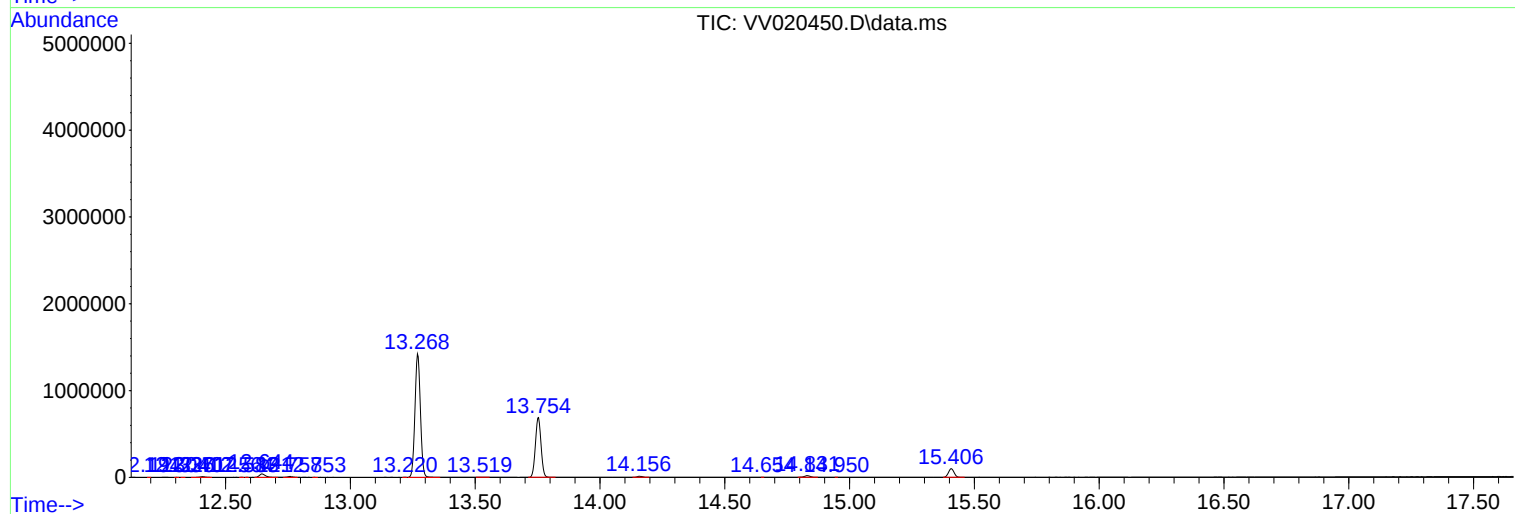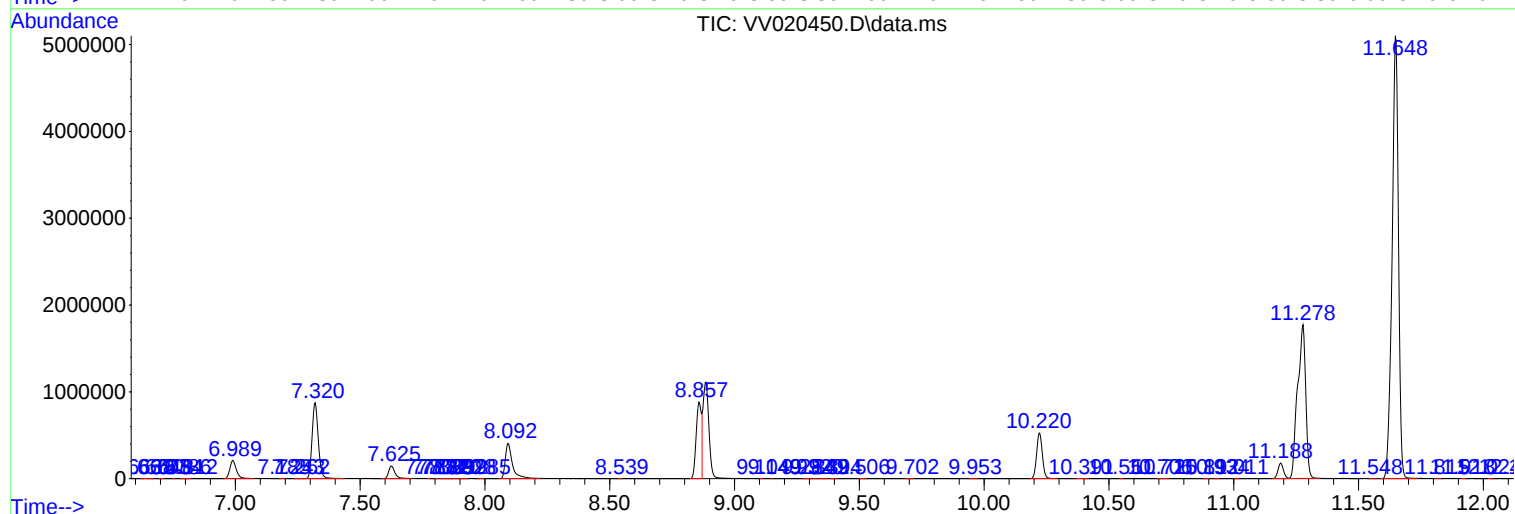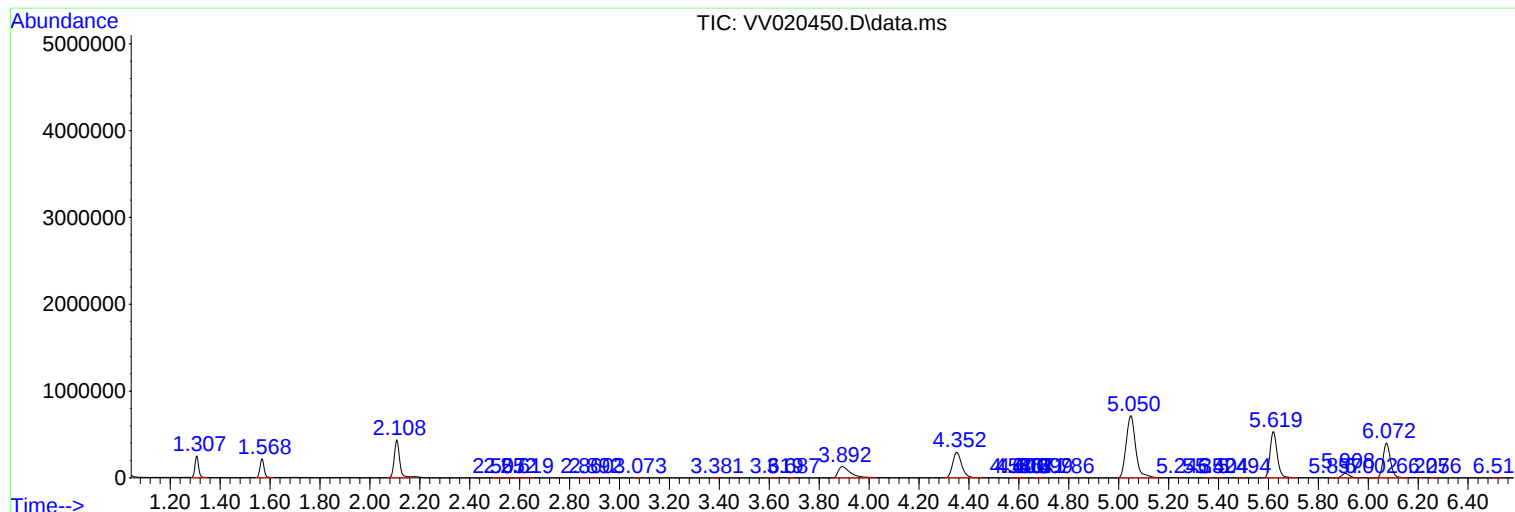

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020450.D
Acq On : 03 Mar 2021 16:02
Operator : SY/MD
Sample : M1546-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020450.D
Acq On : 03 Mar 2021 16:02
Operator : SY/MD
Sample : M1546-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
