

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020451.D
 Acq On : 03 Mar 2021 16:25
 Operator : SY/MD
 Sample : VIBLK91
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	229149	234373	12.98%	1.675%
2	1.571	157	165	179	rVB	201429	231329	12.81%	1.653%
3	2.108	321	332	360	rVB	402146	610445	33.81%	4.363%
4	2.372	411	414	418	rBV	244	194	0.01%	0.001%
5	2.391	418	420	425	rVB3	238	179	0.01%	0.001%
6	2.452	435	439	442	rBV3	307	274	0.02%	0.002%
7	2.510	450	457	467	rVB4	2488	3991	0.22%	0.029%
8	2.577	475	478	482	rVB	271	159	0.01%	0.001%
9	2.741	525	529	536	rBV	242	229	0.01%	0.002%
10	2.802	545	548	552	rVB2	208	164	0.01%	0.001%
11	2.944	588	592	595	rBV	239	185	0.01%	0.001%
12	3.098	633	640	643	rBV2	162	183	0.01%	0.001%
13	3.404	730	735	738	rBV2	367	388	0.02%	0.003%
14	3.696	820	826	828	rBV2	235	227	0.01%	0.002%
15	3.896	877	888	922	rBV	117792	365243	20.23%	2.611%
16	4.288	1005	1010	1013	rVV2	346	393	0.02%	0.003%
17	4.352	1014	1030	1065	rVV	294650	729735	40.42%	5.216%
18	4.654	1121	1124	1128	rVB2	309	232	0.01%	0.002%
19	4.716	1138	1143	1145	rBV	223	200	0.01%	0.001%
20	4.751	1150	1154	1157	rBV3	316	371	0.02%	0.003%
21	4.809	1170	1172	1176	rBV2	355	197	0.01%	0.001%
22	4.835	1176	1180	1187	rVV3	353	310	0.02%	0.002%
23	4.873	1189	1192	1195	rBV2	241	176	0.01%	0.001%
24	4.918	1200	1206	1213	rBV2	147	217	0.01%	0.002%
25	5.050	1228	1247	1281	rBV2	702383	1805525	100.00%	12.905%
26	5.298	1321	1324	1326	rBV	303	158	0.01%	0.001%
27	5.407	1354	1358	1363	rVV3	351	407	0.02%	0.003%
28	5.449	1367	1371	1374	rVB3	440	312	0.02%	0.002%
29	5.468	1374	1377	1380	rBV3	297	236	0.01%	0.002%
30	5.539	1397	1399	1404	rVB	255	205	0.01%	0.001%
31	5.571	1404	1409	1412	rBV2	233	272	0.02%	0.002%
32	5.622	1412	1425	1458	rBV	529740	1061179	58.77%	7.585%
33	5.908	1501	1514	1538	rBV	58362	121899	6.75%	0.871%
34	6.021	1546	1549	1552	rBV3	507	283	0.02%	0.002%
35	6.072	1552	1565	1593	rBV	395210	812738	45.01%	5.809%
36	6.220	1607	1611	1619	rVB5	1178	1611	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020451.D
 Acq On : 03 Mar 2021 16:25
 Operator : SY/MD
 Sample : VIBLK91
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.256	1619	1622	1627	rVB3	681	502	0.03%	0.004%
38	6.281	1627	1630	1634	rVB5	368	206	0.01%	0.001%
39	6.519	1701	1704	1708	rVB2	313	222	0.01%	0.002%
40	6.642	1737	1742	1744	rBV	761	632	0.04%	0.005%
41	6.654	1744	1746	1756	rVV3	761	1097	0.06%	0.008%
42	6.696	1756	1759	1764	rVB3	232	239	0.01%	0.002%
43	6.786	1783	1787	1791	rBV2	211	243	0.01%	0.002%
44	6.989	1838	1850	1880	rBV	206747	378518	20.96%	2.705%
45	7.179	1907	1909	1911	rBV	378	175	0.01%	0.001%
46	7.249	1927	1931	1934	rBV2	389	360	0.02%	0.003%
47	7.320	1940	1953	1983	rBV	829548	1438470	79.67%	10.282%
48	7.503	2008	2010	2021	rVB5	954	891	0.05%	0.006%
49	7.561	2026	2028	2032	rBV3	317	273	0.02%	0.002%
50	7.625	2036	2048	2078	rBV	148084	259494	14.37%	1.855%
51	7.780	2094	2096	2099	rVB2	303	172	0.01%	0.001%
52	7.941	2144	2146	2148	rBV2	286	174	0.01%	0.001%
53	7.960	2149	2152	2155	rVV2	316	218	0.01%	0.002%
54	7.982	2155	2159	2166	rVB5	355	380	0.02%	0.003%
55	8.095	2183	2194	2230	rBV2	409810	842793	46.68%	6.024%
56	8.387	2282	2285	2288	rBV4	378	218	0.01%	0.002%
57	8.445	2298	2303	2307	rBV3	300	304	0.02%	0.002%
58	8.500	2316	2320	2322	rBV2	304	250	0.01%	0.002%
59	8.548	2330	2335	2337	rBV3	469	401	0.02%	0.003%
60	8.593	2342	2349	2352	rBV	305	270	0.01%	0.002%
61	8.613	2352	2355	2360	rVB2	286	234	0.01%	0.002%
62	8.793	2408	2411	2415	rVB	350	243	0.01%	0.002%
63	8.857	2419	2431	2461	rBV	834657	1340229	74.23%	9.579%
64	9.014	2478	2480	2484	rVB2	405	247	0.01%	0.002%
65	9.207	2536	2540	2544	rBV3	299	263	0.01%	0.002%
66	9.330	2574	2578	2582	rBV2	326	278	0.02%	0.002%
67	9.902	2753	2756	2760	rVB	253	178	0.01%	0.001%
68	9.966	2767	2776	2778	rBV2	282	396	0.02%	0.003%
69	10.223	2843	2856	2878	rBV	543729	853715	47.28%	6.102%
70	10.384	2900	2906	2907	rBV2	641	527	0.03%	0.004%
71	10.468	2926	2932	2935	rVB2	233	258	0.01%	0.002%
72	10.490	2935	2939	2947	rBV2	272	281	0.02%	0.002%
73	10.612	2974	2977	2981	rBV	179	179	0.01%	0.001%
74	10.709	3002	3007	3009	rVV	328	274	0.02%	0.002%
75	10.934	3075	3077	3083	rVB3	350	277	0.02%	0.002%
76	11.117	3129	3134	3136	rBV2	293	280	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020451.D
 Acq On : 03 Mar 2021 16:25
 Operator : SY/MD
 Sample : VIBLK91
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.198	3155	3159	3164	rVB4	876	866	0.05%	0.006%
78	11.256	3164	3177	3207	rBV	865217	1339018	74.16%	9.571%
79	11.535	3262	3264	3268	rBV2	347	227	0.01%	0.002%
80	11.632	3280	3294	3316	rBV	969008	1504181	83.31%	10.751%
81	11.995	3401	3407	3410	rBV2	330	284	0.02%	0.002%
82	12.014	3410	3413	3416	rVB2	346	185	0.01%	0.001%
83	12.146	3451	3454	3456	rBV2	330	209	0.01%	0.001%
84	12.262	3486	3490	3495	rBV3	580	555	0.03%	0.004%
85	12.368	3520	3523	3527	rBV2	287	226	0.01%	0.002%
86	12.609	3594	3598	3601	rBV2	295	262	0.01%	0.002%
87	12.670	3613	3617	3621	rVV3	402	390	0.02%	0.003%
88	12.722	3630	3633	3634	rBV	306	174	0.01%	0.001%
89	12.808	3658	3660	3663	rVB2	288	174	0.01%	0.001%
90	12.950	3699	3704	3706	rBV2	265	264	0.01%	0.002%
91	13.162	3768	3770	3775	rVB2	522	279	0.02%	0.002%
92	13.275	3796	3805	3818	rVB2	13423	20135	1.12%	0.144%
93	13.358	3825	3831	3832	rBV3	275	269	0.01%	0.002%
94	13.429	3849	3853	3858	rBV3	356	439	0.02%	0.003%
95	13.757	3947	3955	3964	rBV3	7345	11102	0.61%	0.079%
96	13.850	3981	3984	3988	rBV3	330	306	0.02%	0.002%
97	14.416	4157	4160	4164	rBV	573	371	0.02%	0.003%
98	15.098	4370	4372	4373	rBV	554	169	0.01%	0.001%
99	15.242	4415	4417	4419	rBV2	502	281	0.02%	0.002%
100	15.406	4462	4468	4471	rBV4	1551	1805	0.10%	0.013%




Sum of corrected areas: 13990751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020451.D
Acq On : 03 Mar 2021 16:25
Operator : SY/MD
Sample : VIBLK91
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

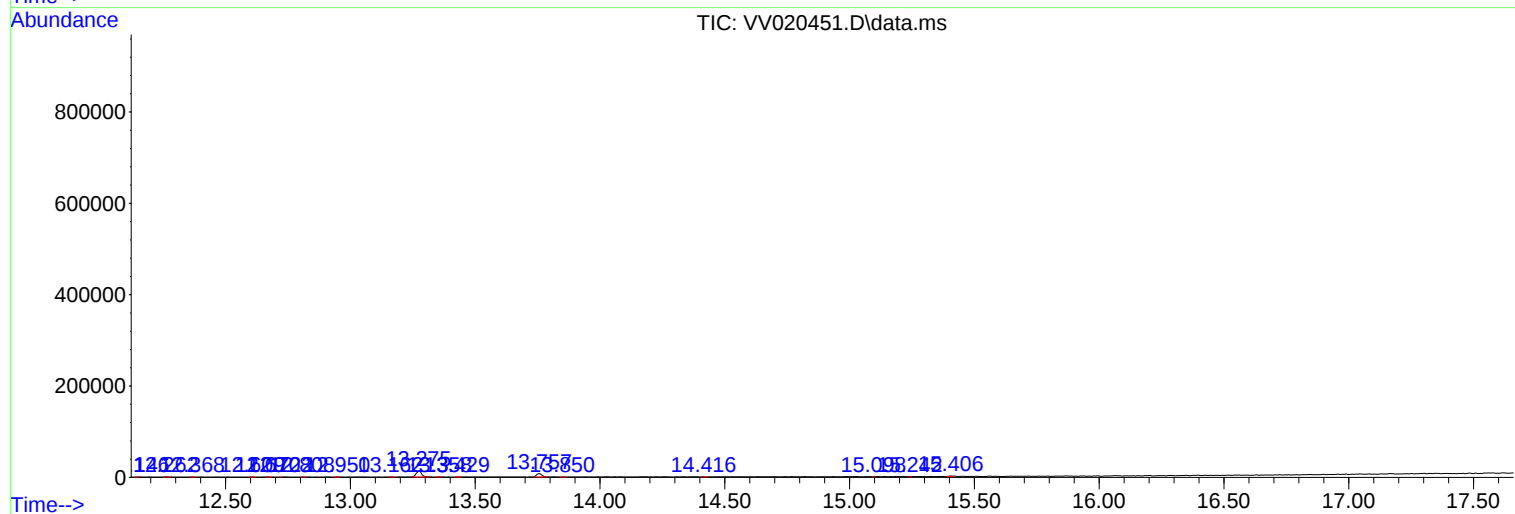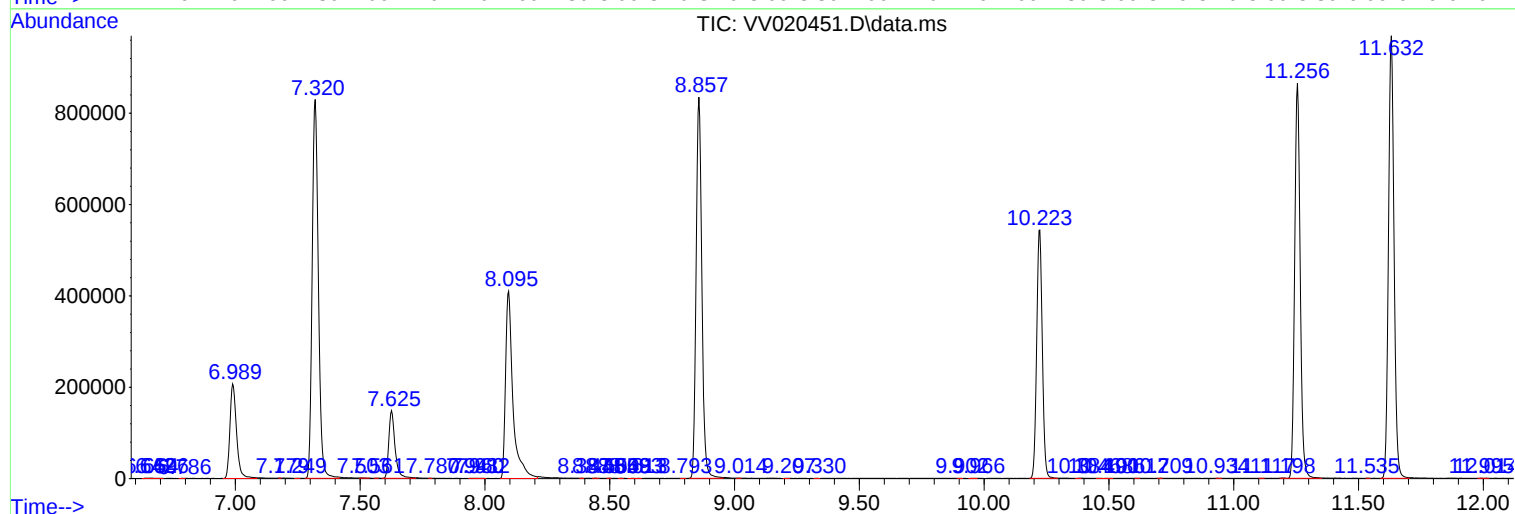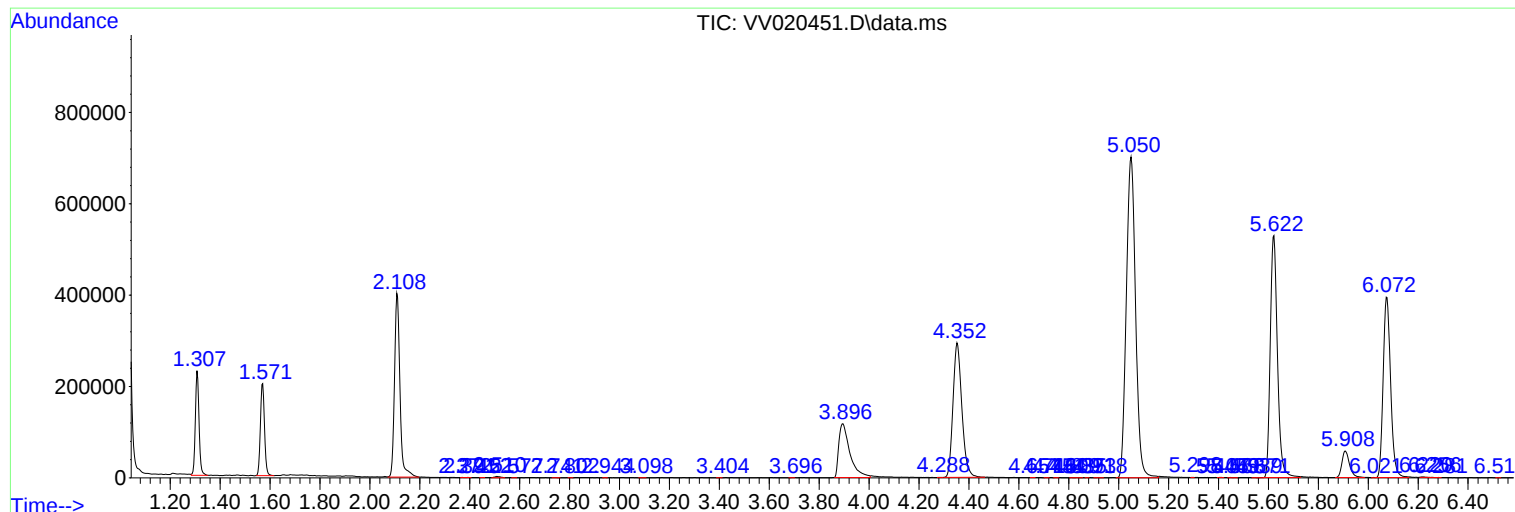

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020451.D
Acq On : 03 Mar 2021 16:25
Operator : SY/MD
Sample : VIBLK91
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020451.D
Acq On : 03 Mar 2021 16:25
Operator : SY/MD
Sample : VIBLK91
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------