

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020452.D
 Acq On : 03 Mar 2021 16:49
 Operator : SY/MD
 Sample : M1546-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	257960	264700	3.35%	0.861%
2	1.571	157	165	178	rVB	226888	251672	3.18%	0.819%
3	2.111	321	333	360	rVB	448126	680450	8.61%	2.213%
4	2.413	421	427	433	rBV2	301	361	0.00%	0.001%
5	2.439	433	435	440	rVV2	364	217	0.00%	0.001%
6	2.516	450	459	465	rBV3	1831	3117	0.04%	0.010%
7	2.574	474	477	480	rBV2	310	214	0.00%	0.001%
8	2.651	497	501	505	rVB2	271	236	0.00%	0.001%
9	2.674	505	508	511	rBV	278	193	0.00%	0.001%
10	3.031	615	619	621	rBV	198	163	0.00%	0.001%
11	3.117	641	646	651	rBV2	404	492	0.01%	0.002%
12	3.159	656	659	664	rVV2	250	282	0.00%	0.001%
13	3.185	664	667	675	rVV2	239	354	0.00%	0.001%
14	3.757	838	845	846	rBV	646	635	0.01%	0.002%
15	3.892	876	887	926	rBV	115574	357888	4.53%	1.164%
16	4.288	1008	1010	1013	rBV2	321	187	0.00%	0.001%
17	4.352	1013	1030	1064	rVV	308725	790530	10.00%	2.571%
18	4.616	1109	1112	1117	rBV3	333	332	0.00%	0.001%
19	4.658	1121	1125	1126	rBV2	211	144	0.00%	0.000%
20	4.828	1168	1178	1179	rBV2	2436	2495	0.03%	0.008%
21	4.902	1195	1201	1205	rBV2	346	367	0.00%	0.001%
22	5.050	1230	1247	1257	rBV2	755449	1919420	24.27%	6.243%
23	5.397	1353	1355	1358	rBV	294	180	0.00%	0.001%
24	5.468	1374	1377	1378	rBV2	293	139	0.00%	0.000%
25	5.503	1386	1388	1393	rVB3	298	249	0.00%	0.001%
26	5.526	1393	1395	1399	rVB3	394	281	0.00%	0.001%
27	5.622	1411	1425	1458	rBV	580475	1168570	14.78%	3.801%
28	5.854	1494	1497	1501	rBV2	211	179	0.00%	0.001%
29	5.908	1502	1514	1531	rBV	43929	88378	1.12%	0.287%
30	6.002	1539	1543	1544	rBV	379	222	0.00%	0.001%
31	6.072	1551	1565	1595	rBV	420860	854331	10.80%	2.779%
32	6.355	1650	1653	1658	rVB3	285	265	0.00%	0.001%
33	6.542	1708	1711	1715	rVB2	165	153	0.00%	0.000%
34	6.567	1715	1719	1723	rBV	237	197	0.00%	0.001%
35	6.645	1740	1743	1747	rBV3	541	443	0.01%	0.001%
36	6.715	1761	1765	1770	rBV3	177	202	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020452.D
 Acq On : 03 Mar 2021 16:49
 Operator : SY/MD
 Sample : M1546-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.809	1789	1794	1797	rBV2	205	171	0.00%	0.001%
38	6.908	1822	1825	1828	rBV	212	145	0.00%	0.000%
39	6.989	1839	1850	1881	rBV	215769	394734	4.99%	1.284%
40	7.246	1928	1930	1935	rVB3	418	237	0.00%	0.001%
41	7.320	1940	1953	1987	rBV	929344	1577306	19.95%	5.130%
42	7.625	2038	2048	2073	rBV	153606	269256	3.41%	0.876%
43	7.847	2114	2117	2119	rBV2	370	199	0.00%	0.001%
44	7.985	2155	2160	2164	rVB3	706	622	0.01%	0.002%
45	8.092	2183	2193	2225	rBV	437392	831580	10.52%	2.705%
46	8.403	2288	2290	2292	rVB2	345	132	0.00%	0.000%
47	8.593	2344	2349	2353	rBV2	441	376	0.00%	0.001%
48	8.622	2354	2358	2363	rVB3	397	322	0.00%	0.001%
49	8.654	2364	2368	2371	rVV2	312	311	0.00%	0.001%
50	8.674	2371	2374	2376	rVV2	266	164	0.00%	0.001%
51	8.690	2376	2379	2383	rVV2	302	175	0.00%	0.001%
52	8.712	2384	2386	2390	rVV2	217	131	0.00%	0.000%
53	8.773	2402	2405	2409	rBV2	240	175	0.00%	0.001%
54	8.886	2418	2440	2490	rBV2	4128788	7906994	100.00%	25.717%
55	9.101	2505	2507	2511	rVB2	755	471	0.01%	0.002%
56	9.120	2511	2513	2515	rVB	394	170	0.00%	0.001%
57	9.159	2521	2525	2527	rBV3	489	303	0.00%	0.001%
58	9.207	2532	2540	2543	rVB5	378	487	0.01%	0.002%
59	9.243	2549	2551	2554	rVB2	356	164	0.00%	0.001%
60	9.307	2568	2571	2574	rVB2	681	417	0.01%	0.001%
61	9.326	2574	2577	2578	rBV	257	168	0.00%	0.001%
62	9.387	2592	2596	2598	rBV2	289	259	0.00%	0.001%
63	9.490	2624	2628	2629	rBV2	315	181	0.00%	0.001%
64	9.587	2655	2658	2660	rBV2	274	177	0.00%	0.001%
65	9.690	2685	2690	2691	rBV2	239	200	0.00%	0.001%
66	9.915	2758	2760	2764	rVB2	239	149	0.00%	0.000%
67	9.944	2766	2769	2774	rVB2	349	235	0.00%	0.001%
68	9.973	2775	2778	2784	rBV2	358	243	0.00%	0.001%
69	10.220	2843	2855	2879	rBV	577352	911356	11.53%	2.964%
70	10.381	2903	2905	2908	rBV	391	297	0.00%	0.001%
71	10.571	2959	2964	2967	rVB2	354	324	0.00%	0.001%
72	10.670	2993	2995	2998	rVB	345	219	0.00%	0.001%
73	10.696	2998	3003	3005	rBV2	329	342	0.00%	0.001%
74	10.744	3013	3018	3022	rBV2	448	488	0.01%	0.002%
75	10.911	3068	3070	3073	rBV	256	160	0.00%	0.001%
76	10.969	3085	3088	3091	rBV	315	246	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020452.D
 Acq On : 03 Mar 2021 16:49
 Operator : SY/MD
 Sample : M1546-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

77	10.985	3091	3093	3098	rVV	202	172	0.00%	0.001%
78	11.059	3112	3116	3119	rBV2	290	239	0.00%	0.001%
79	11.188	3145	3156	3167	rBV	269957	421622	5.33%	1.371%
80	11.278	3167	3184	3208	rVB2	2352006	4992338	63.14%	16.237%
81	11.648	3279	3299	3325	rBV2	3020097	5959290	75.37%	19.382%
82	12.088	3431	3436	3437	rBV3	274	222	0.00%	0.001%
83	12.255	3483	3488	3495	rVV3	626	843	0.01%	0.003%
84	12.313	3503	3506	3508	rBV2	313	158	0.00%	0.001%
85	12.410	3529	3536	3548	rVB4	3117	4685	0.06%	0.015%
86	12.590	3585	3592	3594	rBV	516	563	0.01%	0.002%
87	12.760	3638	3645	3652	rBV5	1099	1812	0.02%	0.006%
88	13.149	3764	3766	3771	rBV2	452	306	0.00%	0.001%
89	13.268	3791	3803	3829	rBV	553046	846024	10.70%	2.752%
90	13.677	3928	3930	3934	rBV2	461	272	0.00%	0.001%
91	13.754	3942	3954	3971	rVB2	134433	211361	2.67%	0.687%
92	13.815	3971	3973	3974	rBV2	380	199	0.00%	0.001%
93	13.914	4002	4004	4008	rBV2	333	281	0.00%	0.001%
94	14.287	4117	4120	4124	rVB3	472	363	0.00%	0.001%
95	14.622	4222	4224	4226	rBV	397	164	0.00%	0.001%
96	14.673	4237	4240	4244	rBV	558	511	0.01%	0.002%
97	14.834	4282	4290	4298	rVB6	3407	4912	0.06%	0.016%
98	14.866	4298	4300	4304	rBV	374	231	0.00%	0.001%
99	15.406	4461	4468	4478	rBV4	6338	10571	0.13%	0.034%
100	15.503	4494	4498	4503	rBV4	706	944	0.01%	0.003%




Sum of corrected areas: 30746407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020452.D
Acq On : 03 Mar 2021 16:49
Operator : SY/MD
Sample : M1546-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

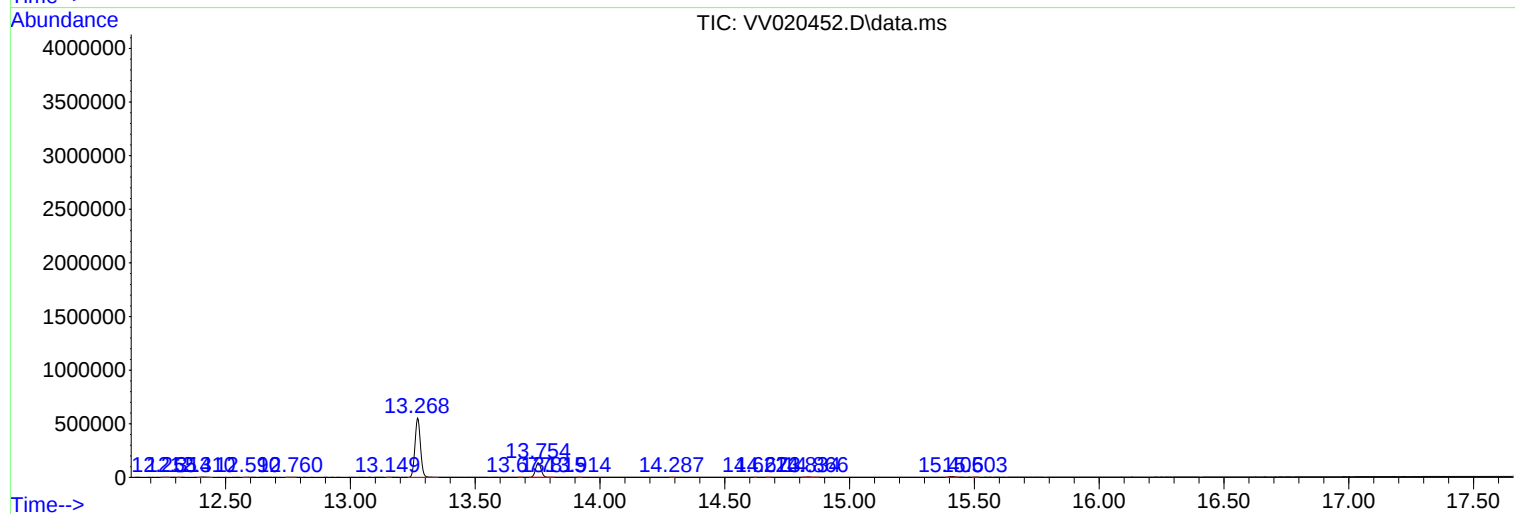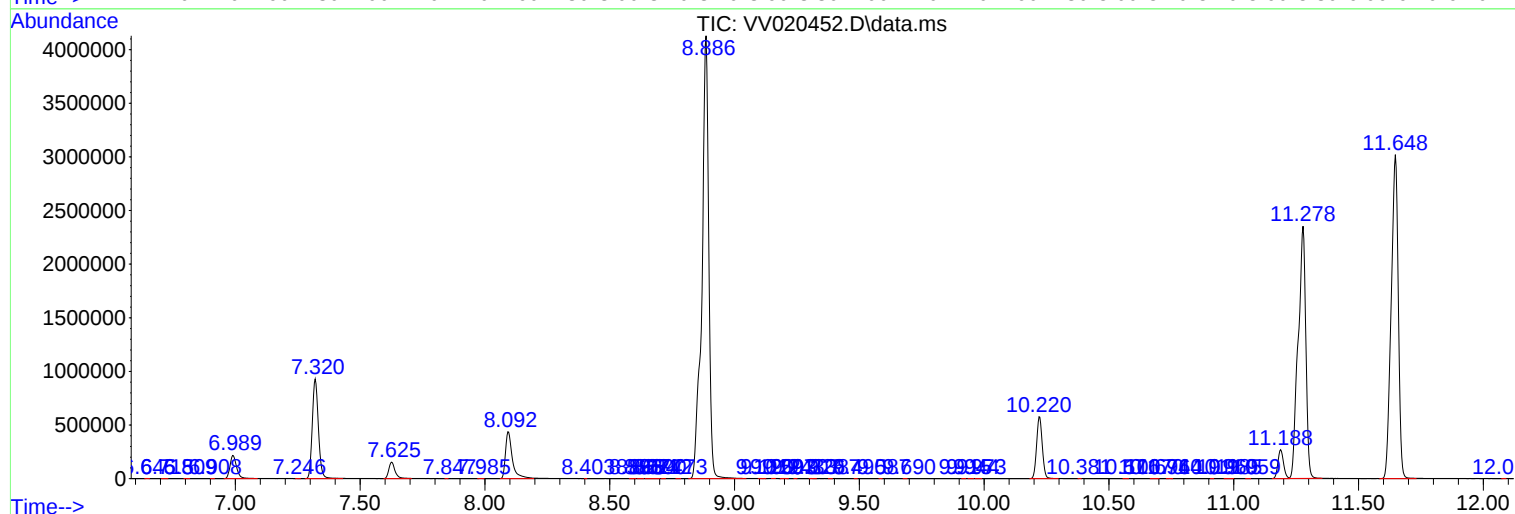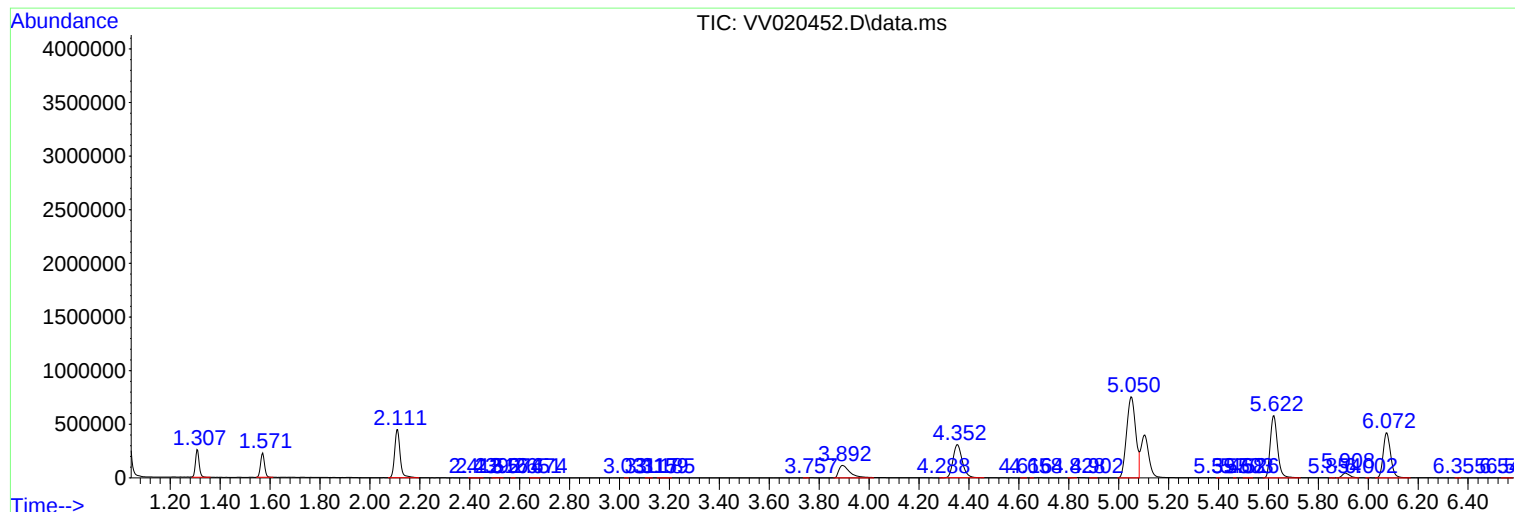

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020452.D
Acq On : 03 Mar 2021 16:49
Operator : SY/MD
Sample : M1546-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020452.D
Acq On : 03 Mar 2021 16:49
Operator : SY/MD
Sample : M1546-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
