

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020454.D
 Acq On : 03 Mar 2021 17:36
 Operator : SY/MD
 Sample : M1546-03 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	254146	262426	1.40%	0.450%
2	1.571	157	165	179	rVB	216139	246667	1.31%	0.423%
3	2.108	322	332	364	rVB	436993	667881	3.55%	1.145%
4	2.510	451	457	467	rVB4	2106	3228	0.02%	0.006%
5	2.574	473	477	481	rBV2	423	350	0.00%	0.001%
6	2.619	488	491	494	rBV2	312	217	0.00%	0.000%
7	2.748	526	531	534	rBV3	258	239	0.00%	0.000%
8	2.880	566	572	576	rVB2	275	299	0.00%	0.001%
9	3.153	655	657	663	rVB	220	208	0.00%	0.000%
10	3.195	663	670	673	rBV	391	472	0.00%	0.001%
11	3.288	695	699	702	rVV	186	192	0.00%	0.000%
12	3.494	757	763	766	rBV2	242	236	0.00%	0.000%
13	3.606	792	798	803	rBV2	186	229	0.00%	0.000%
14	3.651	807	812	818	rVB2	260	287	0.00%	0.000%
15	3.767	838	848	850	rBV3	2668	3909	0.02%	0.007%
16	3.825	861	866	871	rVB2	233	251	0.00%	0.000%
17	3.896	877	888	924	rBV	118221	374376	1.99%	0.642%
18	4.281	1006	1008	1013	rVB	456	362	0.00%	0.001%
19	4.352	1013	1030	1070	rBV	309220	796062	4.23%	1.365%
20	4.561	1092	1095	1099	rVB4	397	308	0.00%	0.001%
21	4.580	1099	1101	1105	rVB3	420	270	0.00%	0.000%
22	4.606	1106	1109	1110	rBV	389	216	0.00%	0.000%
23	4.680	1123	1132	1133	rBV3	1057	1418	0.01%	0.002%
24	4.754	1152	1155	1159	rBV2	240	221	0.00%	0.000%
25	4.777	1159	1162	1166	rVV2	229	180	0.00%	0.000%
26	4.838	1166	1181	1193	rBV4	6660	16220	0.09%	0.028%
27	4.963	1217	1220	1228	rVB2	181	198	0.00%	0.000%
28	5.050	1228	1247	1255	rBV2	748992	1853826	9.86%	3.180%
29	5.449	1365	1371	1373	rBV2	274	197	0.00%	0.000%
30	5.461	1373	1375	1379	rVB	393	276	0.00%	0.000%
31	5.490	1379	1384	1385	rBV2	461	376	0.00%	0.001%
32	5.622	1412	1425	1451	rBV	574715	1155358	6.14%	1.982%
33	5.908	1503	1514	1542	rVB2	32523	69596	0.37%	0.119%
34	6.008	1542	1545	1548	rBV2	246	181	0.00%	0.000%
35	6.072	1551	1565	1598	rBV	412895	840549	4.47%	1.442%
36	6.330	1641	1645	1648	rBV2	264	236	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020454.D
 Acq On : 03 Mar 2021 17:36
 Operator : SY/MD
 Sample : M1546-03 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.432	1674	1677	1682	rBV2	189	209	0.00%	0.000%
38	6.638	1737	1741	1742	rBV	454	352	0.00%	0.001%
39	6.670	1749	1751	1755	rVB3	381	183	0.00%	0.000%
40	6.844	1802	1805	1811	rVV2	296	245	0.00%	0.000%
41	6.989	1839	1850	1875	rBV	215440	391936	2.08%	0.672%
42	7.188	1908	1912	1914	rBV4	437	342	0.00%	0.001%
43	7.320	1940	1953	1980	rBV	907624	1555014	8.27%	2.667%
44	7.522	2014	2016	2020	rBV2	484	417	0.00%	0.001%
45	7.625	2037	2048	2078	rBV	151474	265588	1.41%	0.456%
46	7.911	2134	2137	2141	rVV	329	238	0.00%	0.000%
47	7.989	2154	2161	2168	rVV6	1135	1387	0.01%	0.002%
48	8.091	2182	2193	2226	rBV	459267	860122	4.57%	1.475%
49	8.291	2253	2255	2258	rVB3	679	323	0.00%	0.001%
50	8.358	2274	2276	2278	rVB2	352	182	0.00%	0.000%
51	8.619	2351	2357	2360	rVB3	407	321	0.00%	0.001%
52	8.651	2362	2367	2371	rBV2	286	288	0.00%	0.000%
53	8.886	2419	2440	2486	rBV	11023160	18802547	100.00%	32.249%
54	9.519	2634	2637	2638	rBV2	343	198	0.00%	0.000%
55	9.551	2643	2647	2648	rBV	364	231	0.00%	0.000%
56	9.686	2686	2689	2694	rVB2	408	388	0.00%	0.001%
57	9.818	2726	2730	2734	rBV2	263	228	0.00%	0.000%
58	10.098	2814	2817	2823	rVB3	238	232	0.00%	0.000%
59	10.220	2842	2855	2877	rBV	594954	942455	5.01%	1.616%
60	10.317	2883	2885	2889	rVB3	505	311	0.00%	0.001%
61	10.339	2889	2892	2897	rVB2	308	235	0.00%	0.000%
62	10.384	2901	2906	2911	rBV4	413	623	0.00%	0.001%
63	10.439	2918	2923	2930	rVB2	750	700	0.00%	0.001%
64	10.551	2955	2958	2961	rBV2	303	230	0.00%	0.000%
65	10.673	2991	2996	2999	rBV	257	253	0.00%	0.000%
66	10.741	3010	3017	3022	rBV	366	640	0.00%	0.001%
67	10.783	3027	3030	3032	rVV2	416	265	0.00%	0.000%
68	10.805	3033	3037	3041	rVV2	288	297	0.00%	0.001%
69	11.088	3119	3125	3128	rBV2	313	306	0.00%	0.001%
70	11.114	3128	3133	3139	rVB2	274	325	0.00%	0.001%
71	11.188	3144	3156	3167	rBV	786854	1204230	6.40%	2.065%
72	11.278	3167	3184	3212	rVB2	6536344	11218433	59.66%	19.241%
73	11.445	3234	3236	3242	rVB4	812	552	0.00%	0.001%
74	11.587	3276	3280	3281	rBV	417	329	0.00%	0.001%
75	11.648	3281	3299	3322	rBV2	7871018	13478548	71.68%	23.117%
76	11.905	3378	3379	3383	rVB2	584	221	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020454.D
 Acq On : 03 Mar 2021 17:36
 Operator : SY/MD
 Sample : M1546-03 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FZ4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

77	11.927	3383	3386	3387	rBV2	415	216	0.00%	0.000%
78	11.976	3399	3401	3404	rVB2	532	232	0.00%	0.000%
79	12.072	3429	3431	3434	rVB2	530	290	0.00%	0.000%
80	12.107	3439	3442	3444	rBV3	382	276	0.00%	0.000%
81	12.230	3478	3480	3485	rBV2	329	299	0.00%	0.001%
82	12.374	3522	3525	3527	rBV2	345	213	0.00%	0.000%
83	12.406	3527	3535	3547	rVB4	8972	14802	0.08%	0.025%
84	12.593	3582	3593	3601	rBV4	2468	4877	0.03%	0.008%
85	12.657	3607	3613	3621	rBV5	2400	2766	0.01%	0.005%
86	12.760	3637	3645	3655	rVB5	4831	7306	0.04%	0.013%
87	13.021	3722	3726	3728	rBV3	384	316	0.00%	0.001%
88	13.149	3764	3766	3770	rBV2	377	273	0.00%	0.000%
89	13.213	3781	3786	3789	rBV2	262	285	0.00%	0.000%
90	13.268	3791	3803	3824	rBV	1720286	2566255	13.65%	4.401%
91	13.422	3849	3851	3854	rBV3	384	223	0.00%	0.000%
92	13.490	3868	3872	3873	rBV2	445	280	0.00%	0.000%
93	13.750	3941	3953	3970	rBV	405175	622979	3.31%	1.068%
94	14.094	4059	4060	4063	rBV2	306	217	0.00%	0.000%
95	14.512	4187	4190	4196	rBV2	646	526	0.00%	0.001%
96	14.680	4240	4242	4244	rBV4	463	199	0.00%	0.000%
97	14.802	4277	4280	4281	rBV3	799	477	0.00%	0.001%
98	14.831	4281	4289	4302	rVB4	10173	16336	0.09%	0.028%
99	14.956	4325	4328	4332	rBV2	513	341	0.00%	0.001%
100	15.410	4458	4469	4480	rBV2	23879	37553	0.20%	0.064%




Sum of corrected areas: 58304978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020454.D
Acq On : 03 Mar 2021 17:36
Operator : SY/MD
Sample : M1546-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

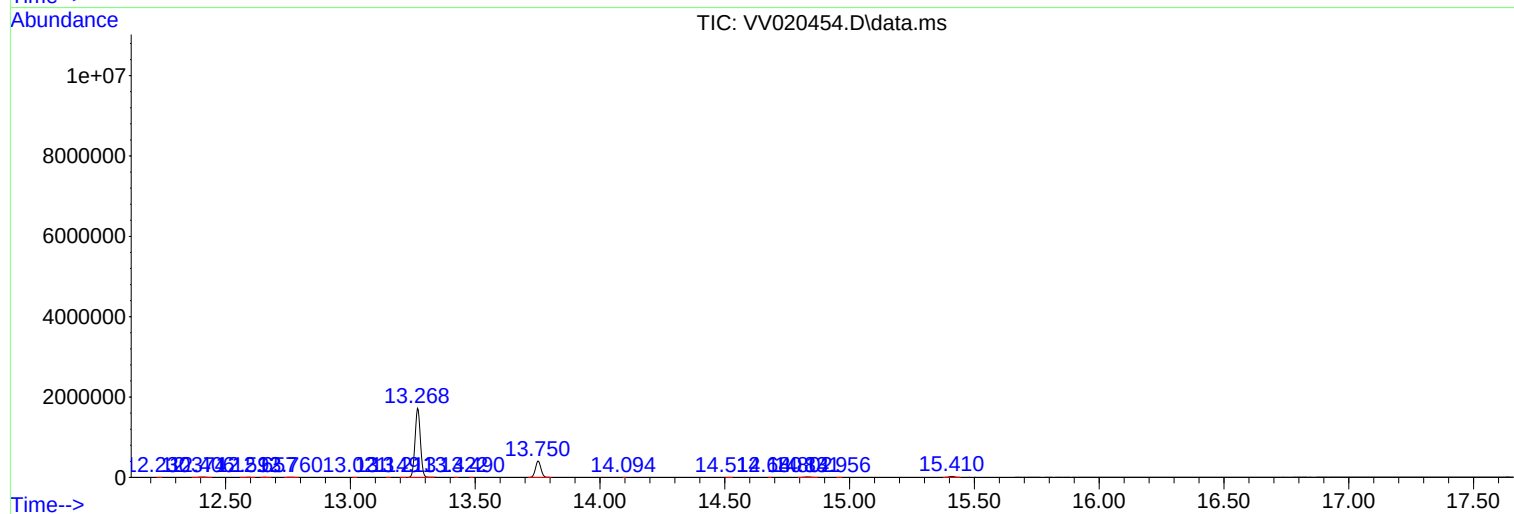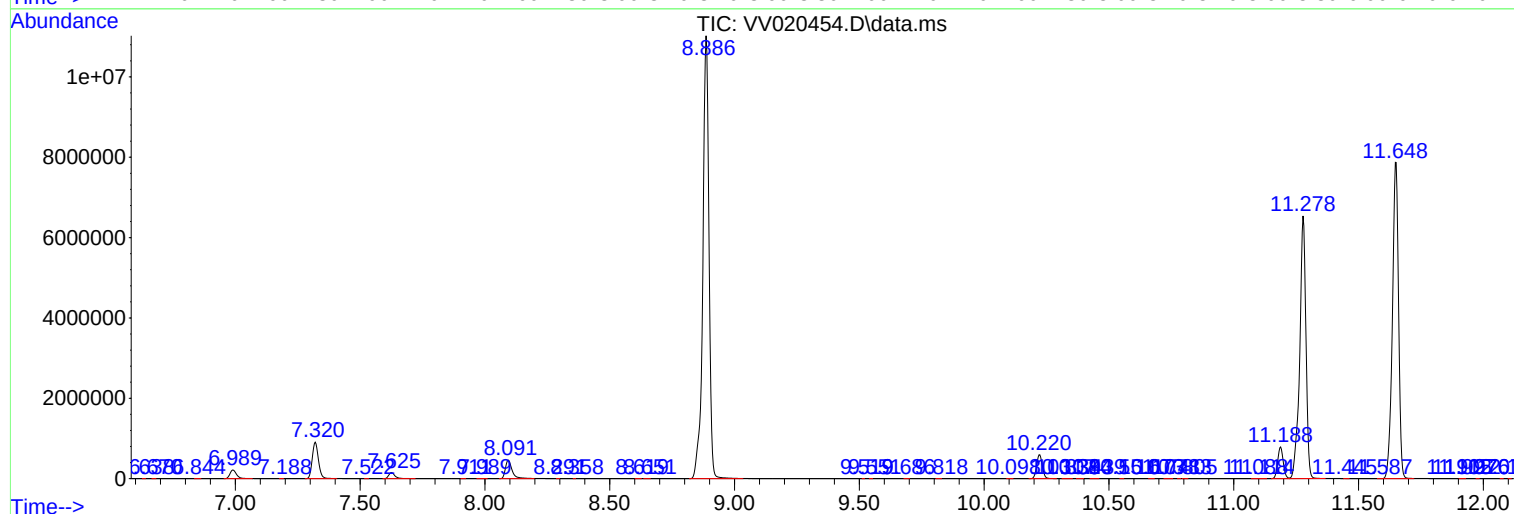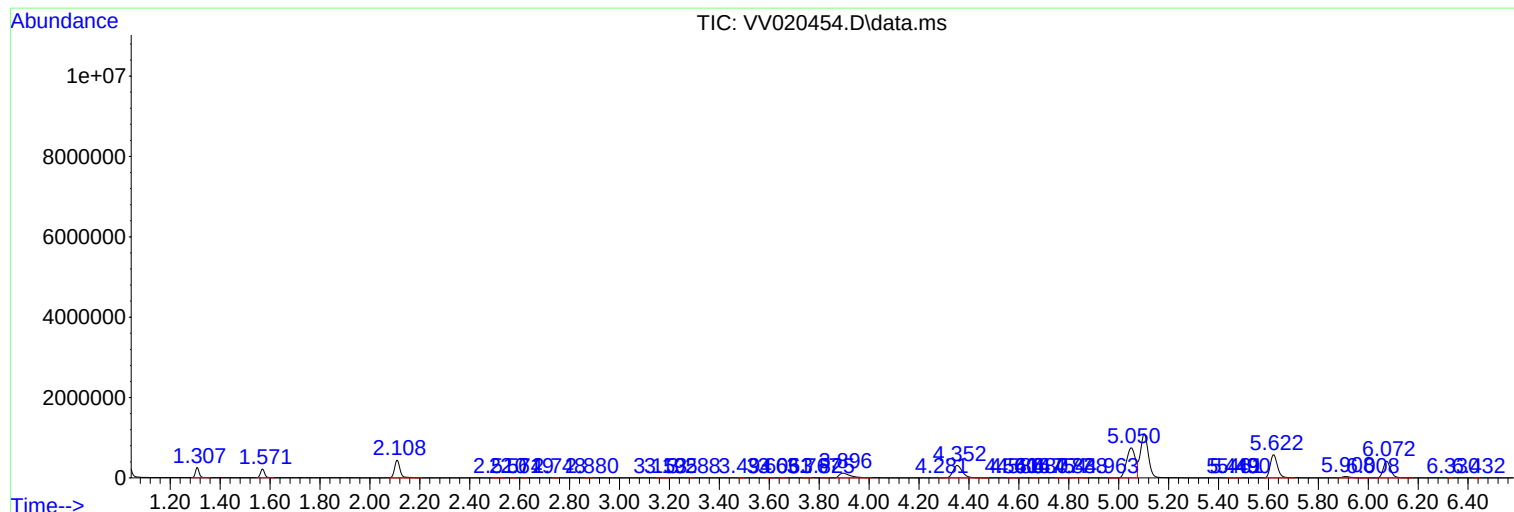

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020454.D
Acq On : 03 Mar 2021 17:36
Operator : SY/MD
Sample : M1546-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020454.D
Acq On : 03 Mar 2021 17:36
Operator : SY/MD
Sample : M1546-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
