

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020455.D
 Acq On : 03 Mar 2021 17:59
 Operator : SY/MD
 Sample : VIBLK93
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	252651	257642	13.49%	1.719%
2	1.571	157	165	177	rBV	219256	249237	13.05%	1.663%
3	2.108	321	332	370	rVB	445029	682711	35.74%	4.554%
4	2.375	411	415	420	rBV2	458	453	0.02%	0.003%
5	2.423	426	430	435	rVB2	389	413	0.02%	0.003%
6	2.462	438	442	448	rVB3	385	334	0.02%	0.002%
7	2.513	449	458	465	rBV4	2164	3426	0.18%	0.023%
8	2.683	508	511	514	rBV	265	160	0.01%	0.001%
9	2.767	535	537	540	rVB	284	163	0.01%	0.001%
10	2.806	547	549	556	rVB3	229	207	0.01%	0.001%
11	3.256	686	689	692	rBV	315	205	0.01%	0.001%
12	3.304	702	704	712	rVB2	290	239	0.01%	0.002%
13	3.487	758	761	765	rBV2	312	290	0.02%	0.002%
14	3.510	765	768	776	rBB2	170	212	0.01%	0.001%
15	3.613	797	800	806	rBV2	199	195	0.01%	0.001%
16	3.896	877	888	930	rBV	116747	367794	19.26%	2.453%
17	4.269	1002	1004	1009	rBV4	244	161	0.01%	0.001%
18	4.352	1012	1030	1058	rBV	305743	772806	40.46%	5.155%
19	4.548	1088	1091	1096	rBV3	382	378	0.02%	0.003%
20	4.603	1104	1108	1112	rBB3	437	419	0.02%	0.003%
21	4.831	1176	1179	1182	rVB3	268	170	0.01%	0.001%
22	4.908	1201	1203	1206	rVB2	242	158	0.01%	0.001%
23	4.950	1210	1216	1218	rBV3	248	263	0.01%	0.002%
24	5.050	1229	1247	1280	rBV2	749794	1909983	100.00%	12.741%
25	5.259	1309	1312	1316	rVB4	646	525	0.03%	0.004%
26	5.410	1355	1359	1364	rVB4	564	487	0.03%	0.003%
27	5.436	1364	1367	1370	rBV	301	243	0.01%	0.002%
28	5.487	1377	1383	1384	rBV2	358	252	0.01%	0.002%
29	5.619	1411	1424	1458	rBV	579765	1159518	60.71%	7.735%
30	5.838	1489	1492	1495	rBV3	328	235	0.01%	0.002%
31	5.908	1502	1514	1532	rBV2	58751	118998	6.23%	0.794%
32	6.072	1552	1565	1590	rBV	411785	839906	43.97%	5.603%
33	6.217	1606	1610	1617	rVB5	835	1112	0.06%	0.007%
34	6.342	1646	1649	1652	rVV2	432	356	0.02%	0.002%
35	6.365	1652	1656	1661	rVV3	420	515	0.03%	0.003%
36	6.400	1663	1667	1669	rVV	309	242	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020455.D
 Acq On : 03 Mar 2021 17:59
 Operator : SY/MD
 Sample : VIBLK93
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.429	1674	1676	1679	rVV2	389	274	0.01%	0.002%
38	6.452	1679	1683	1687	rVB3	418	344	0.02%	0.002%
39	6.641	1738	1742	1745	rBV2	633	480	0.03%	0.003%
40	6.741	1768	1773	1775	rBV3	359	262	0.01%	0.002%
41	6.789	1785	1788	1795	rVB	204	183	0.01%	0.001%
42	6.828	1795	1800	1802	rBV	300	200	0.01%	0.001%
43	6.873	1811	1814	1817	rVV	234	169	0.01%	0.001%
44	6.895	1817	1821	1824	rVB2	223	193	0.01%	0.001%
45	6.989	1838	1850	1873	rBV	214974	390464	20.44%	2.605%
46	7.191	1910	1913	1915	rBV3	632	368	0.02%	0.002%
47	7.320	1937	1953	1992	rBV	918769	1574967	82.46%	10.506%
48	7.555	2024	2026	2030	rVB2	306	213	0.01%	0.001%
49	7.625	2037	2048	2075	rBV	152527	266628	13.96%	1.779%
50	7.828	2109	2111	2115	rVB2	337	176	0.01%	0.001%
51	7.854	2117	2119	2122	rVB2	310	190	0.01%	0.001%
52	7.876	2122	2126	2128	rBV2	280	201	0.01%	0.001%
53	7.982	2157	2159	2162	rBV3	459	313	0.02%	0.002%
54	8.095	2183	2194	2229	rBV2	415172	844630	44.22%	5.634%
55	8.362	2275	2277	2281	rVB2	647	372	0.02%	0.002%
56	8.416	2292	2294	2297	rVB2	448	242	0.01%	0.002%
57	8.519	2324	2326	2328	rVV3	288	166	0.01%	0.001%
58	8.532	2328	2330	2334	rVB2	343	246	0.01%	0.002%
59	8.600	2346	2351	2355	rBV2	246	225	0.01%	0.002%
60	8.629	2355	2360	2361	rBV2	282	233	0.01%	0.002%
61	8.677	2372	2375	2377	rBV	352	185	0.01%	0.001%
62	8.857	2418	2431	2456	rBV	900568	1484090	77.70%	9.900%
63	9.082	2499	2501	2509	rVB4	474	405	0.02%	0.003%
64	9.712	2694	2697	2700	rBV	281	194	0.01%	0.001%
65	9.731	2700	2703	2709	rVB2	317	190	0.01%	0.001%
66	10.043	2795	2800	2803	rBV2	338	311	0.02%	0.002%
67	10.220	2843	2855	2876	rBV	555751	868088	45.45%	5.791%
68	10.384	2899	2906	2909	rBV2	634	757	0.04%	0.005%
69	10.995	3090	3096	3098	rBV2	186	179	0.01%	0.001%
70	11.108	3128	3131	3135	rBV	219	168	0.01%	0.001%
71	11.198	3150	3159	3165	rBV6	2546	4125	0.22%	0.028%
72	11.255	3165	3177	3201	rVV	958702	1499899	78.53%	10.005%
73	11.442	3233	3235	3238	rBV2	465	245	0.01%	0.002%
74	11.632	3281	3294	3317	rBV	1036270	1642214	85.98%	10.955%
75	11.751	3329	3331	3333	rBV2	425	210	0.01%	0.001%
76	11.857	3362	3364	3367	rVB	322	174	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020455.D
 Acq On : 03 Mar 2021 17:59
 Operator : SY/MD
 Sample : VIBLK93
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.911	3379	3381	3386	rVB2	396	202	0.01%	0.001%
78	12.024	3414	3416	3419	rBV2	332	216	0.01%	0.001%
79	12.066	3427	3429	3434	rVB2	353	193	0.01%	0.001%
80	12.291	3496	3499	3504	rVB3	234	202	0.01%	0.001%
81	12.342	3512	3515	3518	rBV	236	160	0.01%	0.001%
82	12.500	3560	3564	3568	rBV2	357	318	0.02%	0.002%
83	12.561	3578	3583	3586	rBV	316	303	0.02%	0.002%
84	12.770	3645	3648	3651	rVV3	301	257	0.01%	0.002%
85	13.062	3736	3739	3743	rBV	260	182	0.01%	0.001%
86	13.095	3747	3749	3754	rBV2	262	209	0.01%	0.001%
87	13.140	3760	3763	3765	rBV3	231	165	0.01%	0.001%
88	13.275	3796	3805	3819	rBV2	16697	24892	1.30%	0.166%
89	13.352	3826	3829	3832	rBV	409	377	0.02%	0.003%
90	13.416	3846	3849	3854	rBV2	375	368	0.02%	0.002%
91	13.525	3880	3883	3885	rBV2	381	235	0.01%	0.002%
92	13.612	3907	3910	3913	rBV	226	175	0.01%	0.001%
93	13.680	3929	3931	3935	rBV	307	239	0.01%	0.002%
94	13.760	3946	3956	3964	rBV4	4776	6610	0.35%	0.044%
95	13.914	4001	4004	4012	rBV2	461	578	0.03%	0.004%
96	13.972	4020	4022	4027	rVB3	385	195	0.01%	0.001%
97	15.094	4369	4371	4374	rBV	586	260	0.01%	0.002%
98	15.394	4462	4464	4465	rBV2	567	219	0.01%	0.001%
99	15.500	4494	4497	4501	rBV3	683	600	0.03%	0.004%
100	15.557	4513	4515	4517	rBV3	689	411	0.02%	0.003%


Sum of corrected areas: 14991147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020455.D
Acq On : 03 Mar 2021 17:59
Operator : SY/MD
Sample : VIBLK93
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

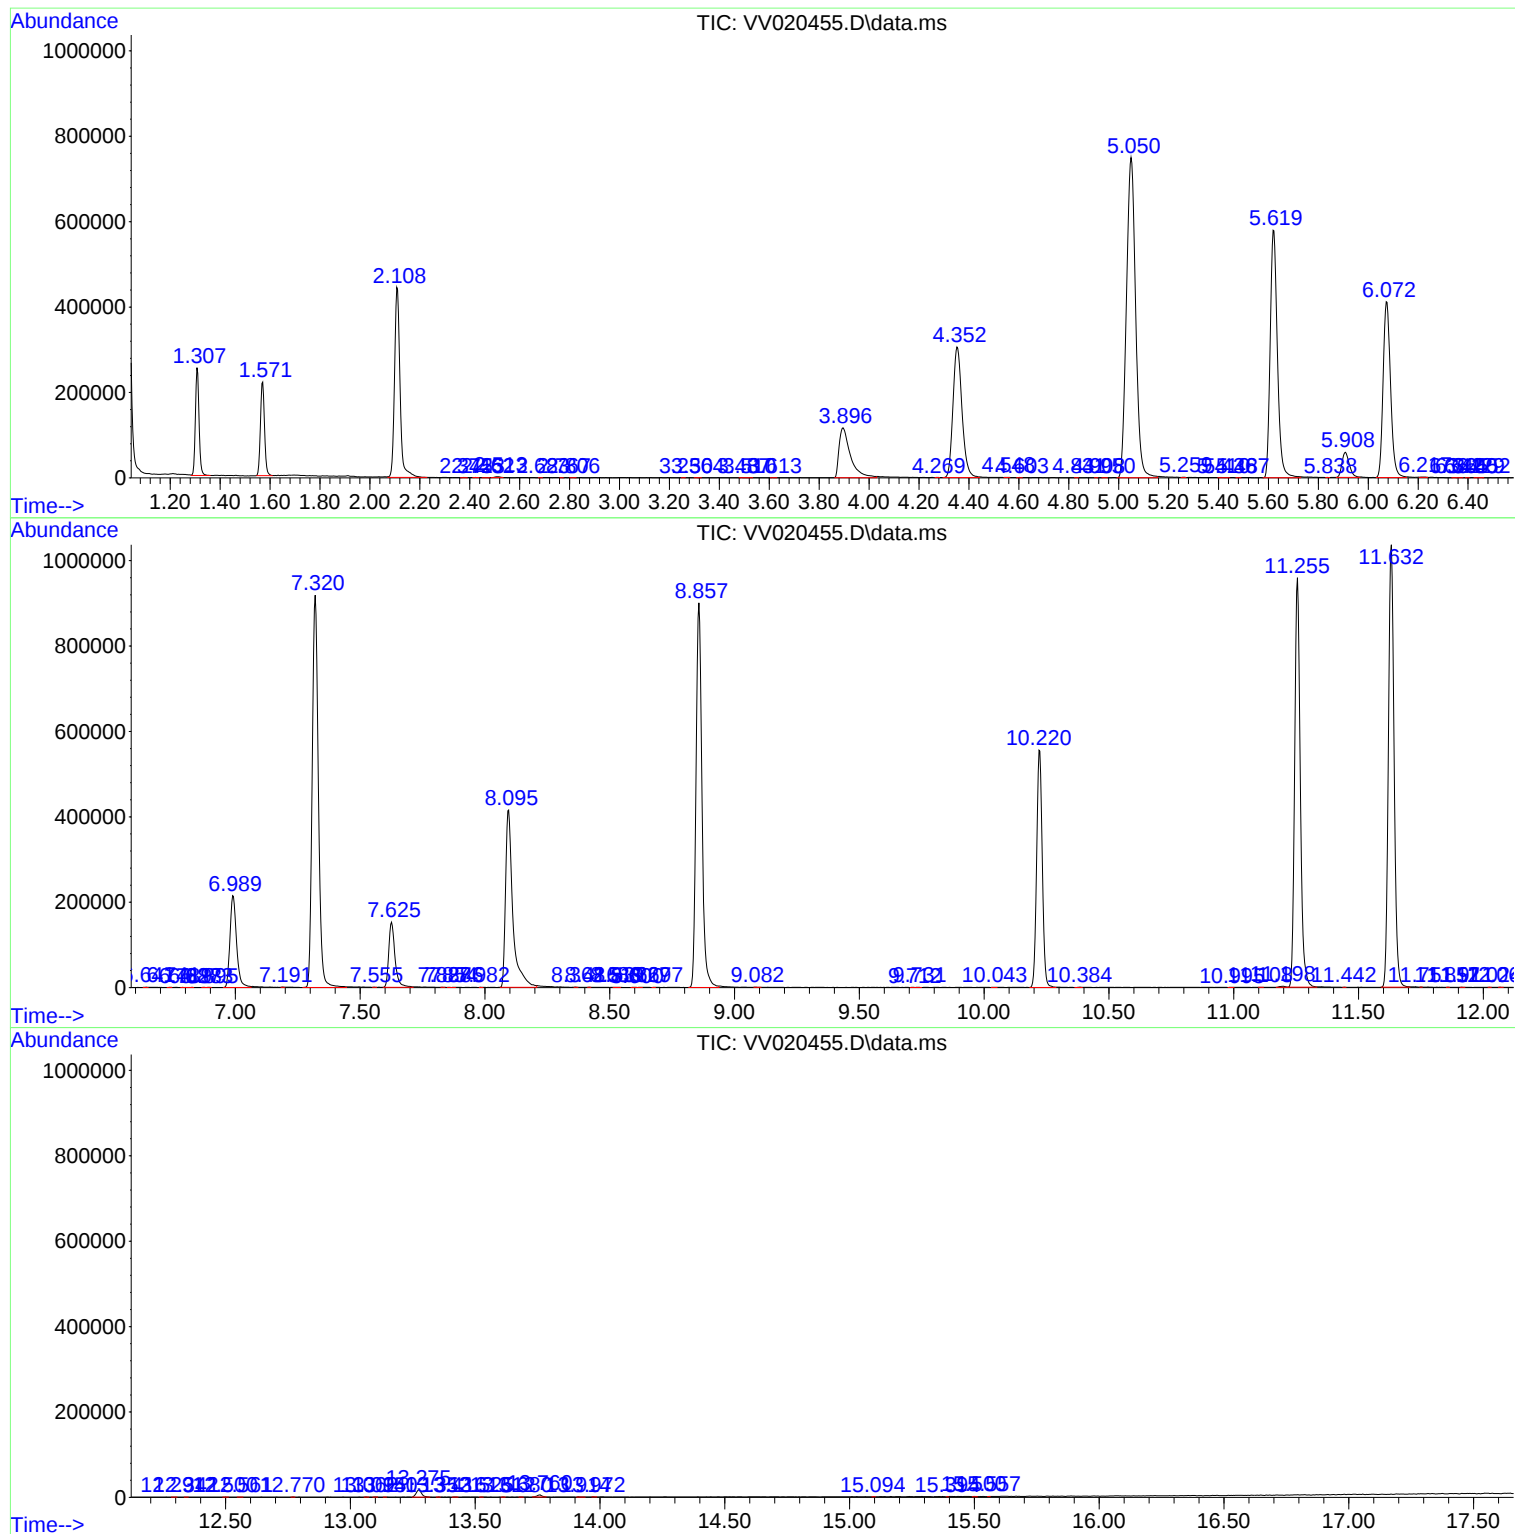

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020455.D
Acq On : 03 Mar 2021 17:59
Operator : SY/MD
Sample : VIBLK93
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020455.D
Acq On : 03 Mar 2021 17:59
Operator : SY/MD
Sample : VIBLK93
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------