

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020456.D
 Acq On : 03 Mar 2021 18:46
 Operator : SY/MD
 Sample : M1546-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	243937	247154	13.31%	1.715%
2	1.571	157	165	181	rBV	213363	241949	13.03%	1.679%
3	2.111	321	333	361	rBV	434304	659040	35.50%	4.574%
4	2.262	377	380	383	rVB2	384	239	0.01%	0.002%
5	2.323	396	399	402	rBV3	343	282	0.02%	0.002%
6	2.375	411	415	419	rBV3	701	761	0.04%	0.005%
7	2.513	451	458	466	rVB4	2514	4156	0.22%	0.029%
8	2.552	466	470	474	rVV3	474	416	0.02%	0.003%
9	2.574	474	477	480	rVV2	344	205	0.01%	0.001%
10	2.590	480	482	487	rVV2	277	174	0.01%	0.001%
11	2.661	498	504	507	rBV2	333	248	0.01%	0.002%
12	2.793	539	545	548	rBV2	344	315	0.02%	0.002%
13	3.307	702	705	708	rVB2	335	247	0.01%	0.002%
14	3.507	762	767	771	rBV	231	248	0.01%	0.002%
15	3.590	787	793	794	rBV2	239	183	0.01%	0.001%
16	3.670	816	818	825	rBV	239	205	0.01%	0.001%
17	3.815	860	863	867	rVB2	245	201	0.01%	0.001%
18	3.896	877	888	926	rBV2	109920	353304	19.03%	2.452%
19	4.281	1005	1008	1011	rBV3	414	289	0.02%	0.002%
20	4.352	1011	1030	1063	rVV	298599	753355	40.58%	5.229%
21	4.635	1116	1118	1124	rVB4	331	253	0.01%	0.002%
22	4.670	1124	1129	1132	rVB4	325	288	0.02%	0.002%
23	4.693	1132	1136	1139	rBV	309	177	0.01%	0.001%
24	4.796	1162	1168	1170	rBV3	259	311	0.02%	0.002%
25	4.889	1193	1197	1201	rBV2	216	171	0.01%	0.001%
26	5.050	1224	1247	1287	rBV2	727942	1856594	100.00%	12.886%
27	5.352	1338	1341	1344	rVB	311	218	0.01%	0.002%
28	5.532	1393	1397	1400	rVB2	232	178	0.01%	0.001%
29	5.622	1411	1425	1455	rBV	551253	1123325	60.50%	7.797%
30	5.812	1482	1484	1489	rVB2	347	201	0.01%	0.001%
31	5.908	1502	1514	1537	rVV2	60354	123899	6.67%	0.860%
32	6.011	1544	1546	1550	rVB4	469	244	0.01%	0.002%
33	6.072	1550	1565	1586	rBV	407751	822723	44.31%	5.710%
34	6.413	1667	1671	1675	rVB2	285	213	0.01%	0.001%
35	6.445	1675	1681	1684	rBV	152	191	0.01%	0.001%
36	6.641	1739	1742	1744	rBV2	454	323	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020456.D
 Acq On : 03 Mar 2021 18:46
 Operator : SY/MD
 Sample : M1546-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	6.989	1839	1850	1881	rBV	204007	378876	20.41%	2.630%
38	7.185	1909	1911	1914	rBV2	472	278	0.01%	0.002%
39	7.320	1941	1953	1976	rBV	874943	1508822	81.27%	10.472%
40	7.590	2034	2037	2038	rBV2	366	233	0.01%	0.002%
41	7.625	2038	2048	2081	rVV	145000	256230	13.80%	1.778%
42	7.747	2083	2086	2091	rVB5	719	736	0.04%	0.005%
43	7.818	2104	2108	2110	rVB2	383	265	0.01%	0.002%
44	7.905	2131	2135	2138	rBV3	275	212	0.01%	0.001%
45	7.944	2138	2147	2149	rBV3	1807	2419	0.13%	0.017%
46	7.995	2160	2163	2165	rVB2	487	268	0.01%	0.002%
47	8.095	2183	2194	2235	rBV2	396233	813396	43.81%	5.646%
48	8.391	2282	2286	2289	rBV3	385	273	0.01%	0.002%
49	8.423	2295	2296	2297	rBV	583	182	0.01%	0.001%
50	8.484	2310	2315	2318	rBV3	331	358	0.02%	0.002%
51	8.538	2328	2332	2335	rVB2	333	226	0.01%	0.002%
52	8.609	2350	2354	2357	rBV	261	181	0.01%	0.001%
53	8.632	2359	2361	2367	rVV	370	295	0.02%	0.002%
54	8.674	2370	2374	2380	rBV2	237	223	0.01%	0.002%
55	8.857	2419	2431	2459	rBV	884827	1419467	76.46%	9.852%
56	9.021	2480	2482	2485	rBV3	472	248	0.01%	0.002%
57	9.098	2500	2506	2507	rBV2	263	202	0.01%	0.001%
58	9.165	2518	2527	2531	rBV3	510	660	0.04%	0.005%
59	9.191	2531	2535	2536	rBV	301	183	0.01%	0.001%
60	9.429	2605	2609	2611	rBV	178	178	0.01%	0.001%
61	9.583	2654	2657	2661	rVB	358	222	0.01%	0.002%
62	9.760	2708	2712	2716	rBV2	164	173	0.01%	0.001%
63	9.837	2733	2736	2739	rVB2	255	175	0.01%	0.001%
64	10.220	2843	2855	2881	rBV	528135	833406	44.89%	5.784%
65	10.390	2897	2908	2918	rVB3	3750	6014	0.32%	0.042%
66	10.432	2918	2921	2926	rVB2	190	177	0.01%	0.001%
67	10.481	2932	2936	2939	rBV2	225	174	0.01%	0.001%
68	10.879	3056	3060	3063	rBV	243	261	0.01%	0.002%
69	10.979	3087	3091	3094	rBV	212	188	0.01%	0.001%
70	11.191	3155	3157	3165	rVB3	676	594	0.03%	0.004%
71	11.255	3165	3177	3209	rBV	932143	1421469	76.56%	9.866%
72	11.435	3232	3233	3237	rVB2	622	299	0.02%	0.002%
73	11.461	3239	3241	3247	rVV3	225	194	0.01%	0.001%
74	11.632	3281	3294	3322	rBV	1006501	1557768	83.90%	10.812%
75	11.763	3332	3335	3338	rBV3	507	320	0.02%	0.002%
76	11.837	3354	3358	3360	rBV2	445	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020456.D
 Acq On : 03 Mar 2021 18:46
 Operator : SY/MD
 Sample : M1546-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	11.898	3375	3377	3382	rVB3	407	300	0.02%	0.002%
78	12.037	3418	3420	3427	rBV3	213	197	0.01%	0.001%
79	12.101	3435	3440	3444	rBV2	331	306	0.02%	0.002%
80	12.320	3503	3508	3509	rBV2	210	171	0.01%	0.001%
81	12.329	3509	3511	3514	rVV	329	177	0.01%	0.001%
82	12.384	3525	3528	3538	rVB2	450	372	0.02%	0.003%
83	12.458	3546	3551	3557	rBV2	419	440	0.02%	0.003%
84	12.545	3575	3578	3581	rBV2	236	214	0.01%	0.001%
85	12.593	3590	3593	3595	rBV	242	170	0.01%	0.001%
86	12.696	3622	3625	3627	rBV	306	186	0.01%	0.001%
87	13.178	3773	3775	3778	rVV	263	178	0.01%	0.001%
88	13.249	3793	3797	3799	rBV2	400	313	0.02%	0.002%
89	13.278	3799	3806	3813	rVV4	2074	2837	0.15%	0.020%
90	13.349	3825	3828	3833	rBV2	209	242	0.01%	0.002%
91	13.477	3864	3868	3871	rVB2	448	400	0.02%	0.003%
92	13.496	3871	3874	3876	rBV2	444	269	0.01%	0.002%
93	13.532	3881	3885	3886	rBV2	384	256	0.01%	0.002%
94	13.876	3989	3992	3995	rBV2	386	274	0.01%	0.002%
95	13.921	4001	4006	4008	rBV3	380	391	0.02%	0.003%
96	14.278	4114	4117	4121	rBV	423	352	0.02%	0.002%
97	14.458	4170	4173	4176	rVB3	384	254	0.01%	0.002%
98	14.940	4320	4323	4326	rBV2	648	473	0.03%	0.003%
99	14.959	4327	4329	4331	rVV	480	194	0.01%	0.001%
100	14.972	4331	4333	4339	rVB2	443	394	0.02%	0.003%




Sum of corrected areas: 14407767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020456.D
Acq On : 03 Mar 2021 18:46
Operator : SY/MD
Sample : M1546-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

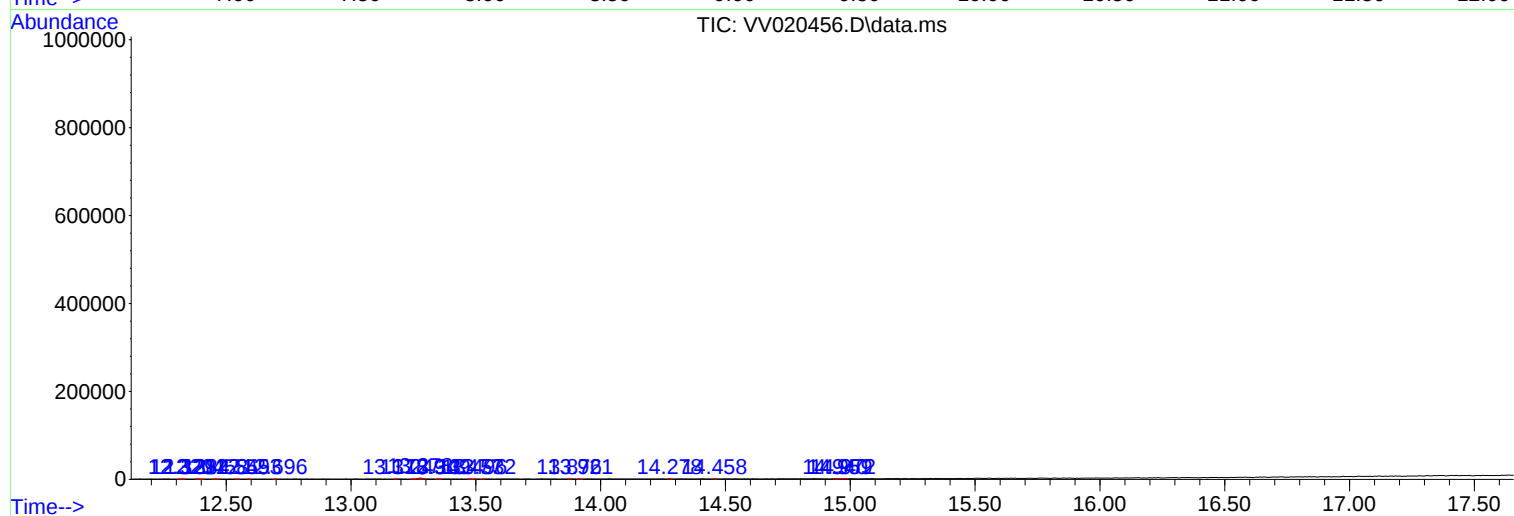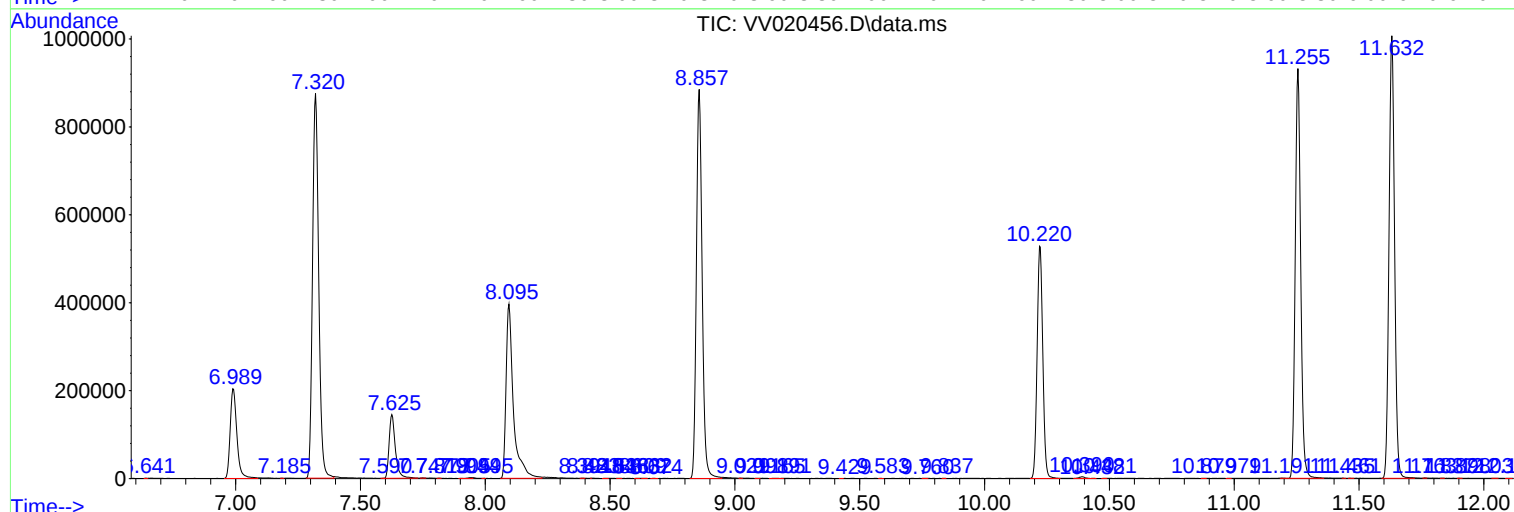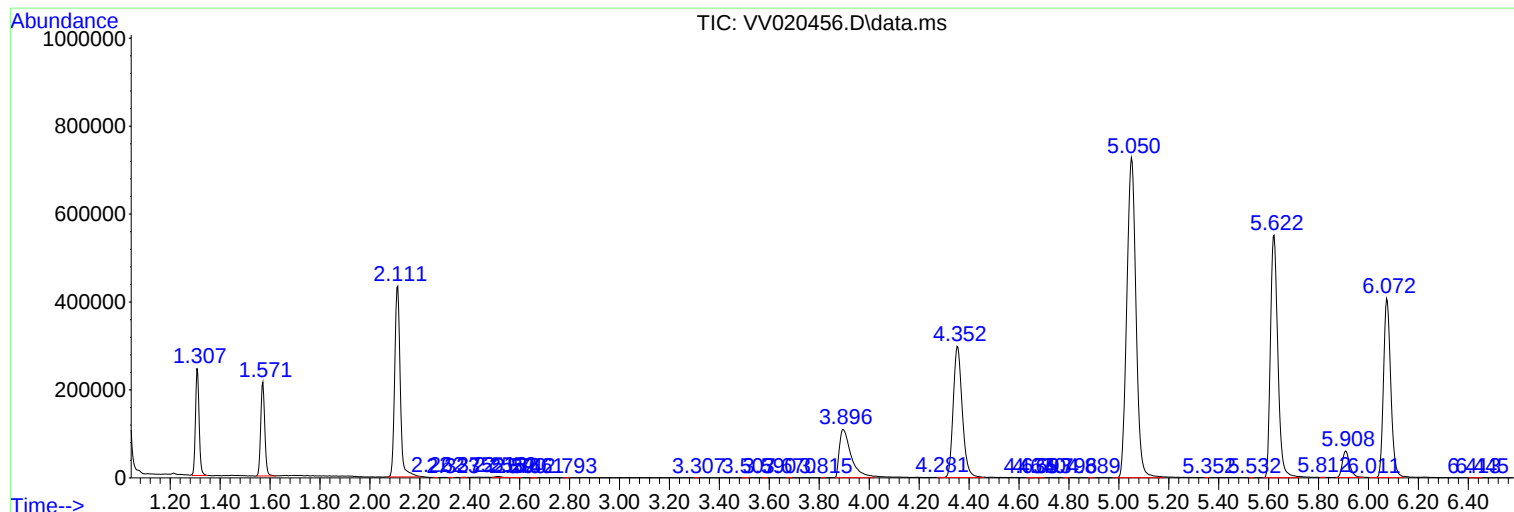

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020456.D
Acq On : 03 Mar 2021 18:46
Operator : SY/MD
Sample : M1546-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
Data File : VV020456.D
Acq On : 03 Mar 2021 18:46
Operator : SY/MD
Sample : M1546-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
