
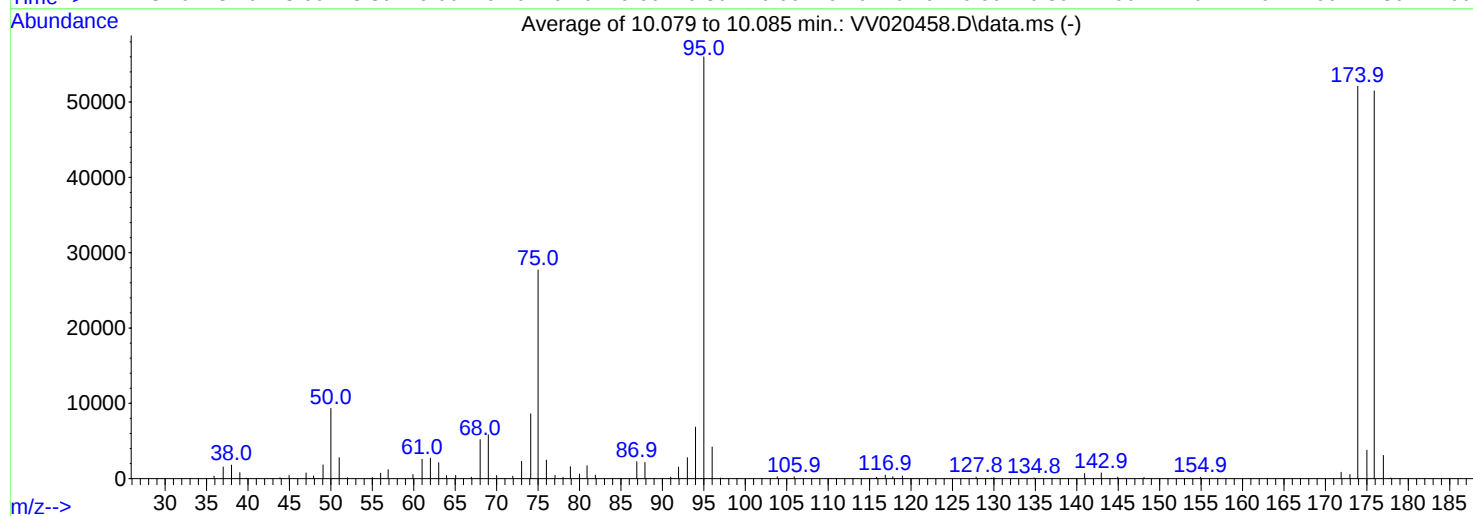


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030421\
 Data File : VV020458.D
 Acq On : 04 Mar 2021 09:19
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 04 00:36:40 2021

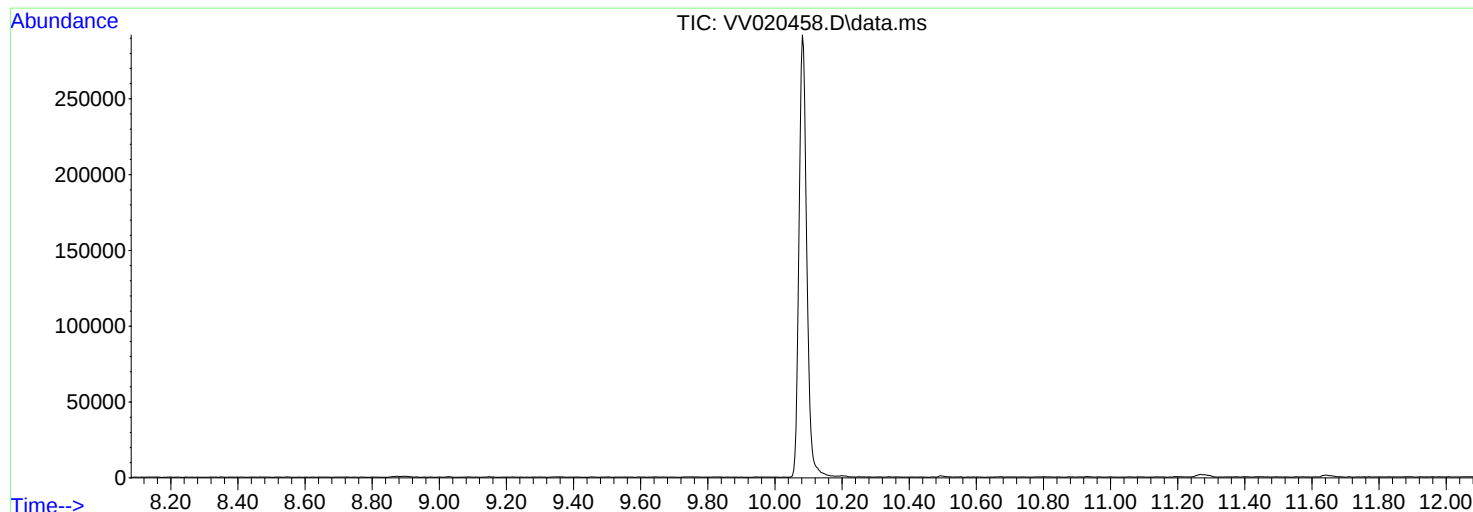

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9324	PASS
75	95	30	80	49.5	27699	PASS
95	95	100	100	100.0	56003	PASS
96	95	5	9	7.5	4206	PASS
173	174	0.00	2	1.1	548	PASS
174	95	50	120	93.0	52083	PASS
175	174	5	9	7.2	3776	PASS
176	174	95	101	98.9	51504	PASS
177	176	5	9	6.0	3091	PASS

m/z	Abundance
35.90	316.0
37.00	1468.0
38.00	1847.0
39.00	815.0
39.80	225.0
43.90	445.0
44.90	415.0
47.00	637.0
47.90	359.0
49.10	1802.0
50.00	9164.0
51.00	2787.0
52.00	122.0
55.00	125.0
56.00	708.0
56.90	1250.0
59.90	498.0
61.00	2505.0
62.00	2747.0
63.00	2025.0
63.90	410.0
65.10	462.0
67.00	175.0
68.00	5156.0
69.00	5772.0
70.00	384.0
72.00	365.0
73.00	2339.0
74.10	8500.0
75.00	26976.0
76.00	2382.0
77.00	442.0
78.00	221.0
78.90	1521.0
80.00	539.0
80.90	1654.0
81.90	497.0
86.90	2189.0
87.90	2205.0
91.00	261.0
91.90	1558.0
93.00	2526.0
94.00	6352.0
95.00	54832.0
96.00	4251.0
97.30	104.0
103.80	249.0
105.90	267.0
115.80	160.0
116.90	463.0
117.80	249.0
118.90	322.0
127.80	197.0
130.00	238.0
134.90	122.0
141.00	696.0
143.00	698.0
144.90	230.0
146.00	144.0
148.10	128.0
155.00	176.0
171.90	777.0
172.90	510.0
173.90	49216.0
175.00	3626.0
175.90	47904.0
177.00	3022.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.90	347.0
37.00	1563.0
38.00	1855.0
39.00	837.0
39.80	219.0
43.80	463.0
44.90	448.0
47.00	801.0
47.90	400.0
49.10	1880.0
50.00	9619.0
51.00	2878.0
52.00	120.0
55.00	167.0
56.00	746.0
56.90	1225.0
59.90	563.0
61.00	2677.0
62.00	2816.0
63.00	2208.0
63.90	447.0
65.10	445.0
66.90	206.0
68.00	5384.0
69.00	6085.0
70.00	446.0
71.90	338.0
73.00	2384.0
74.10	8876.0
75.00	28552.0
76.00	2588.0
77.00	468.0
78.00	207.0
78.90	1645.0
80.00	628.0
80.90	1786.0
81.90	495.0
86.90	2339.0
87.90	2196.0
91.00	213.0
92.00	1541.0
93.00	2903.0
94.00	7102.0
95.00	57720.0
96.00	4413.0
97.00	111.0
103.90	248.0
105.90	261.0
115.80	193.0
116.90	486.0
117.80	287.0
119.00	374.0
127.90	243.0
130.00	217.0
134.80	107.0
137.00	103.0
140.90	721.0
142.90	793.0
144.90	215.0
145.90	125.0
148.10	174.0
154.90	189.0
159.00	115.0
171.90	908.0
173.00	551.0
173.90	53736.0
175.00	3959.0
175.90	53424.0
177.00	3190.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.90	360.0
37.00	1643.0
38.00	1728.0
39.00	798.0
39.80	214.0
43.90	497.0
45.00	434.0
47.00	844.0
47.90	356.0
49.00	1835.0
50.00	9190.0
51.00	2673.0
52.00	119.0
55.00	153.0
56.00	707.0
56.90	1104.0
59.90	595.0
61.00	2528.0
62.00	2578.0
63.00	2114.0
64.00	385.0
65.00	459.0
66.90	179.0
68.00	5032.0
69.00	5615.0
70.00	424.0
71.90	310.0
73.00	2141.0
74.10	8469.0
75.00	27568.0
76.00	2411.0
77.10	441.0
78.00	178.0
78.90	1647.0
80.00	675.0
80.90	1725.0
81.90	437.0
86.90	2227.0
87.90	2011.0
90.70	159.0
91.00	155.0
92.00	1468.0
93.00	2914.0
94.00	7065.0
95.00	55456.0
96.00	3953.0
97.00	140.0
103.90	256.0
105.90	237.0
115.90	212.0
116.90	451.0
117.80	252.0
119.00	400.0
127.80	224.0
129.70	199.0
134.80	113.0
140.90	626.0
142.90	814.0
145.00	179.0
148.10	143.0
154.90	191.0
160.90	103.0
171.90	884.0
173.00	582.0
173.90	53296.0
175.00	3744.0
175.90	53184.0
177.00	3061.0
177.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
39.90	148.0
43.90	344.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95