


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030519\
 Data File : VV009481.D
 Acq On : 05 Mar 2019 09:08
 Operator : SY/MD
 Sample : BFB69
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
 Title : VOC Analysis
 Last Update : Thu Mar 07 02:53:16 2019

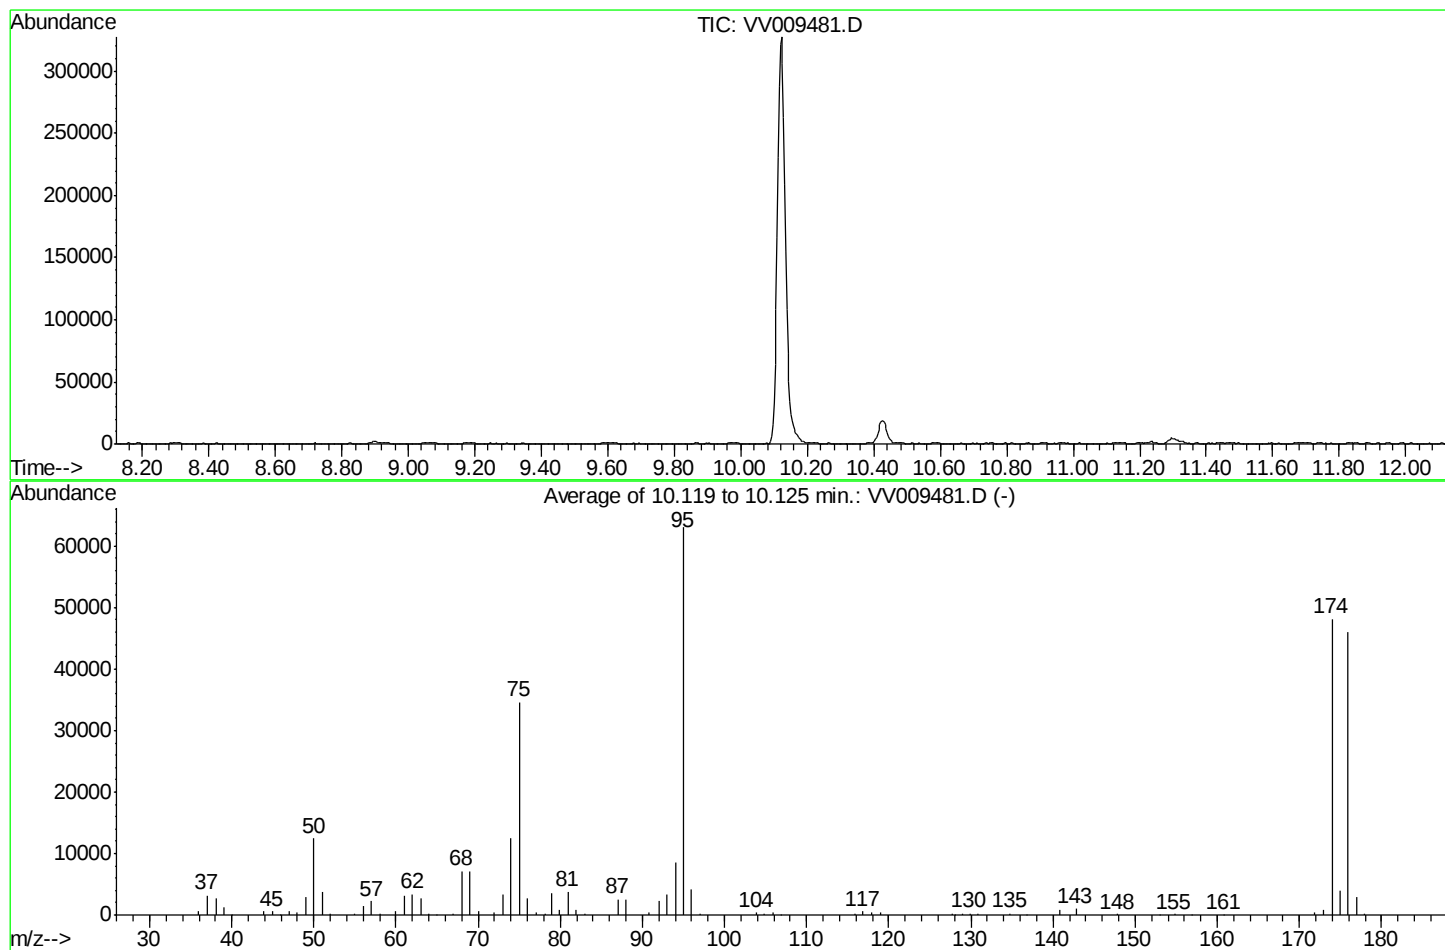

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	12397	PASS
75	95	30	80	54.9	34605	PASS
95	95	100	100	100.0	63056	PASS
96	95	5	9	6.7	4226	PASS
173	174	0.00	2	1.6	764	PASS
174	95	50	120	76.4	48176	PASS
175	174	5	9	8.2	3966	PASS
176	174	95	101	95.6	46048	PASS
177	176	5	9	6.3	2922	PASS

m/z	Abundance
36.00	629.0
37.00	3249.0
38.10	2680.0
39.00	1212.0
39.90	334.0
43.90	761.0
45.00	621.0
46.90	651.0
47.90	499.0
49.00	3130.0
50.00	13006.0
51.00	3858.0
51.90	250.0
55.00	185.0
56.00	1484.0
57.00	2258.0
58.00	130.0
60.00	731.0
61.00	3396.0
62.00	3461.0
63.00	3019.0
63.90	252.0
67.00	227.0
68.00	7225.0
69.00	7389.0
70.10	614.0
72.00	281.0
73.00	3384.0
74.00	12766.0
75.00	35216.0
76.00	2609.0
77.00	432.0
78.10	233.0
78.90	3533.0
79.90	942.0
80.90	3937.0
81.90	877.0
82.90	127.0
87.00	2718.0
87.90	2706.0
90.80	441.0
92.00	2277.0
93.00	3381.0
94.00	8391.0
95.00	63848.0
96.00	4449.0
96.90	185.0
103.90	466.0
104.80	133.0
105.90	353.0
106.80	111.0
116.00	250.0
116.90	542.0
117.90	354.0
118.90	394.0
127.80	288.0
128.80	186.0
129.90	295.0
130.90	139.0
134.70	182.0
140.90	915.0
142.80	963.0
147.80	105.0
154.80	211.0
171.80	336.0
173.00	847.0
174.00	47848.0
175.00	4058.0
176.00	45696.0
177.00	2861.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :

m/z	Abundance
36.00	609.0
37.00	3274.0
38.00	2722.0
39.00	1306.0
39.90	326.0
43.90	783.0
44.90	602.0
46.90	696.0
47.90	475.0
49.00	3107.0
50.00	12764.0
51.00	3881.0
51.90	212.0
55.00	216.0
56.00	1503.0
57.00	2361.0
58.10	125.0
60.00	763.0
61.00	3271.0
62.00	3447.0
63.00	2846.0
63.90	307.0
64.90	120.0
67.00	278.0
68.00	7294.0
69.00	7178.0
70.00	625.0
71.90	337.0
73.00	3366.0
74.00	12913.0
75.00	35544.0
76.10	2747.0
77.00	485.0
78.10	228.0
78.90	3604.0
79.90	961.0
80.90	3926.0
81.90	921.0
82.90	140.0
87.00	2684.0
87.90	2663.0
90.80	424.0
92.00	2342.0
93.00	3307.0
94.00	8806.0
95.00	64776.0
96.00	4358.0
96.90	162.0
104.00	417.0
104.80	147.0
105.90	415.0
115.80	287.0
116.90	554.0
118.00	376.0
118.90	467.0
127.80	260.0
128.90	186.0
129.90	311.0
130.90	138.0
134.80	205.0
136.80	122.0
140.90	964.0
142.80	1050.0
147.80	133.0
154.80	208.0
156.80	102.0
160.80	101.0
171.90	369.0
173.00	783.0
174.00	49616.0
175.00	4083.0
175.90	47472.0
177.00	2978.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :

m/z	Abundance
35.90	577.0
37.00	3097.0
38.00	2680.0
39.00	1362.0
39.90	273.0
43.90	723.0
44.90	536.0
45.90	112.0
47.00	635.0
47.80	387.0
49.00	2738.0
50.00	11422.0
51.00	3613.0
51.90	165.0
54.90	233.0
56.00	1320.0
57.00	2219.0
58.00	108.0
60.00	663.0
61.00	2945.0
62.00	3201.0
63.00	2558.0
63.90	355.0
64.90	116.0
67.00	257.0
68.00	6745.0
69.00	6637.0
70.00	600.0
71.80	397.0
73.00	2977.0
74.00	11943.0
75.00	33056.0
76.10	2616.0
77.00	461.0
78.90	3381.0
79.90	877.0
80.90	3425.0
81.90	864.0
83.00	125.0
87.00	2418.0
88.00	2358.0
90.80	336.0
92.00	2171.0
93.00	3086.0
94.00	8275.0
95.00	60544.0
96.00	3872.0
97.00	138.0
103.90	360.0
104.80	150.0
105.90	396.0
115.90	315.0
116.80	502.0
118.00	327.0
119.00	491.0
128.00	237.0
129.00	169.0
129.90	325.0
130.90	140.0
134.90	256.0
136.80	148.0
140.90	883.0
142.90	967.0
147.90	164.0
153.00	107.0
154.80	171.0
156.80	127.0
171.90	333.0
173.00	663.0
174.00	47064.0
175.00	3758.0
175.90	44976.0
177.00	2928.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :

Scan 2796 (10.080 min): VV009481.D
BFB69

m/z	Abundance
39.90	266.0
43.90	226.0

Instrument :
MSVOA_V
ClientSampleId :