
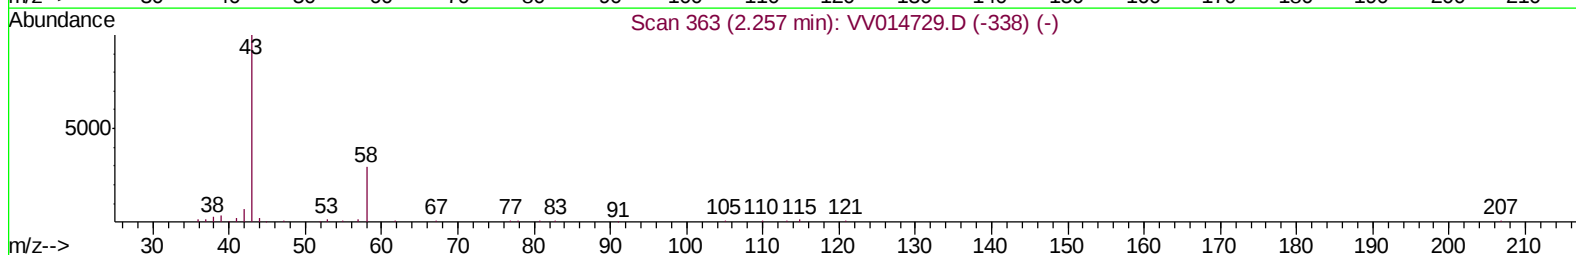
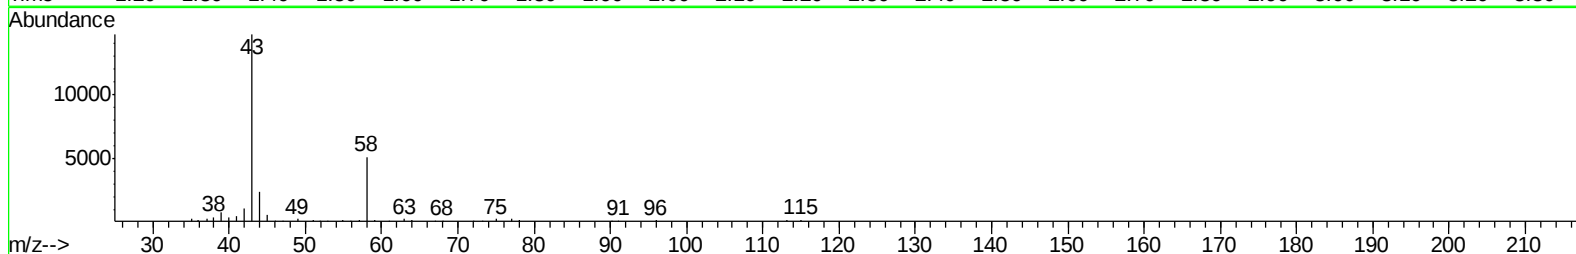


Data File : VV014750.D
Acq On : 05 Mar 2020 10:07
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 06 02:02:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Mar 05 15:29:01 2020
Response via : Initial Calibration

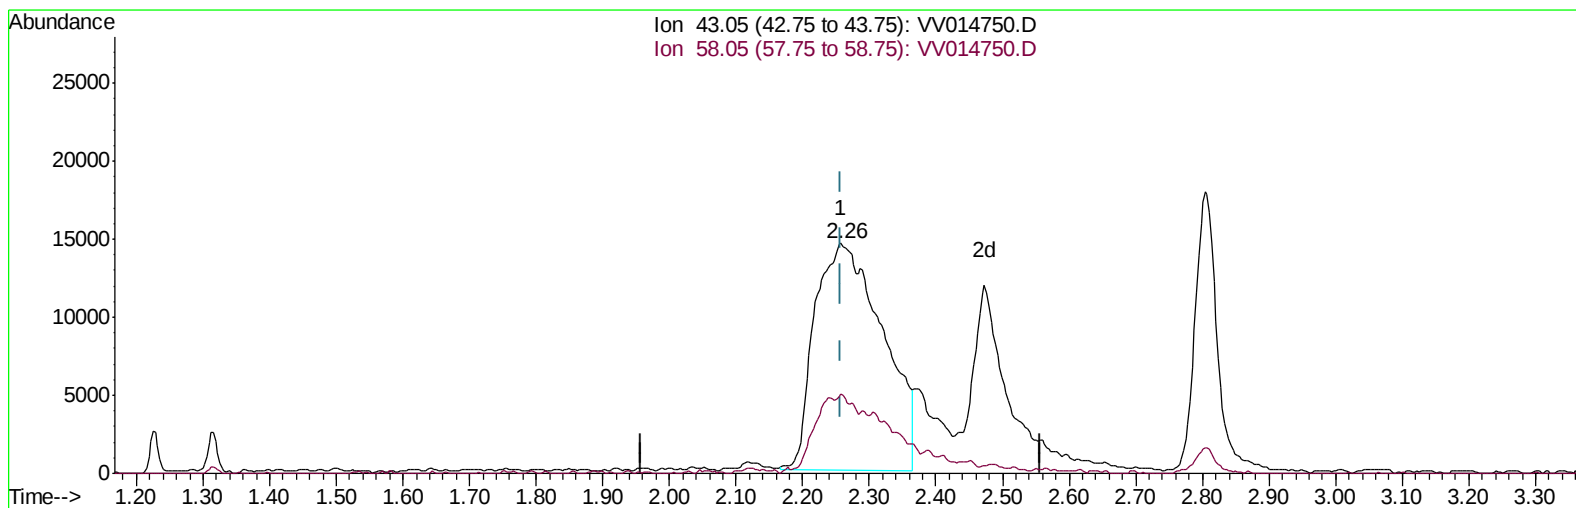

TIC: VV014750.D

(13) Acetone (T)

2.258min (+0.000) 37.35ug/L m

response 103315

Ion	Exp%	Act%
43.05	100	100
58.05	10.00	9.62
0.00	0.00	0.00
0.00	0.00	0.00