
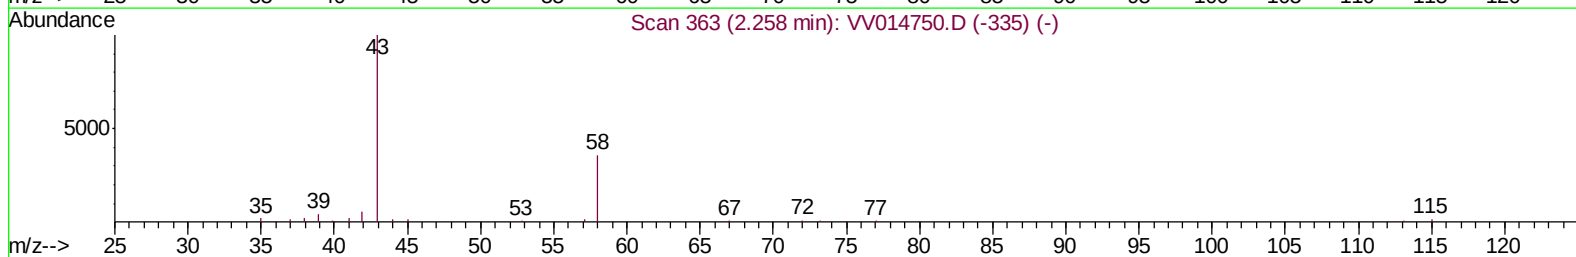
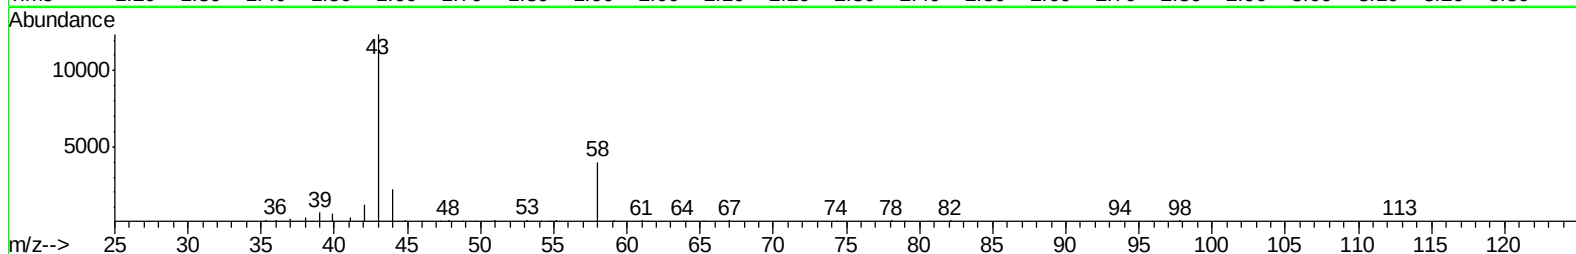


Data File : VV014758.D
Acq On : 05 Mar 2020 16:26
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Mar 06 02:42:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 06 02:39:22 2020
Response via : Initial Calibration

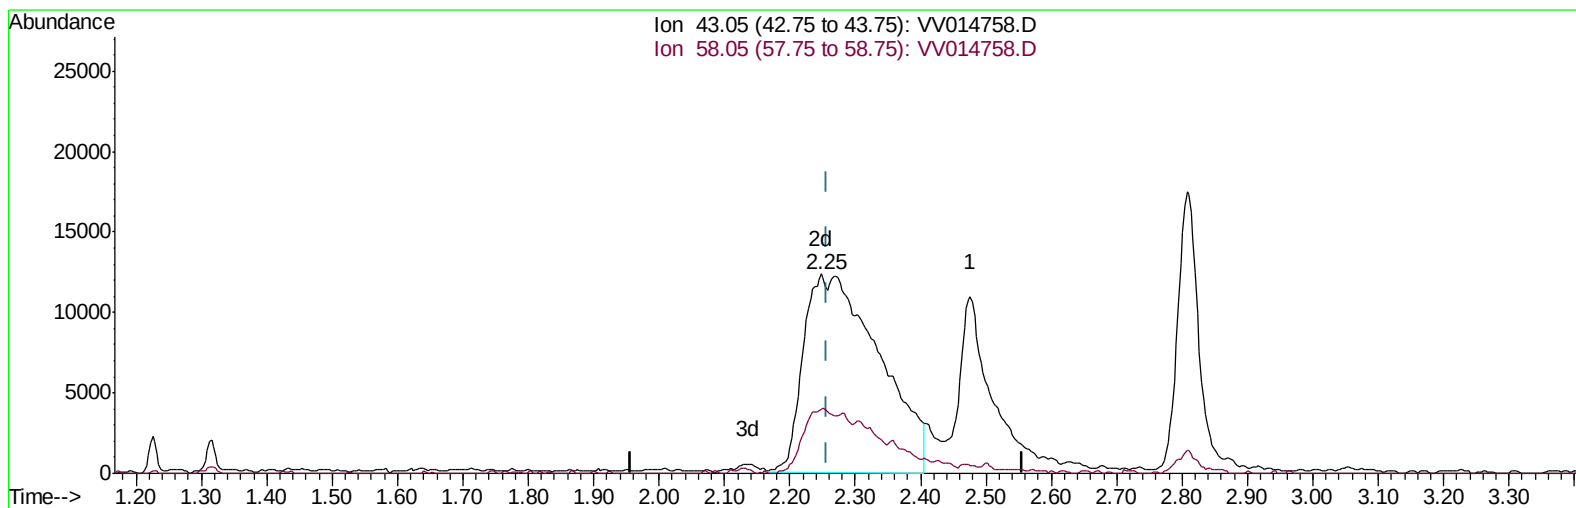

TIC: VV014758.D

(13) Acetone (T)

2.248min (-0.010) 39.22ug/L m

response 99264

Ion	Exp%	Act%
43.05	100	100
58.05	10.00	0.43
0.00	0.00	0.00
0.00	0.00	0.00