


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030520\
 Data File : VV014749.D
 Acq On : 05 Mar 2020 09:29
 Operator : SY/MD
 Sample : BFB42
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR022820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Mar 06 02:39:22 2020

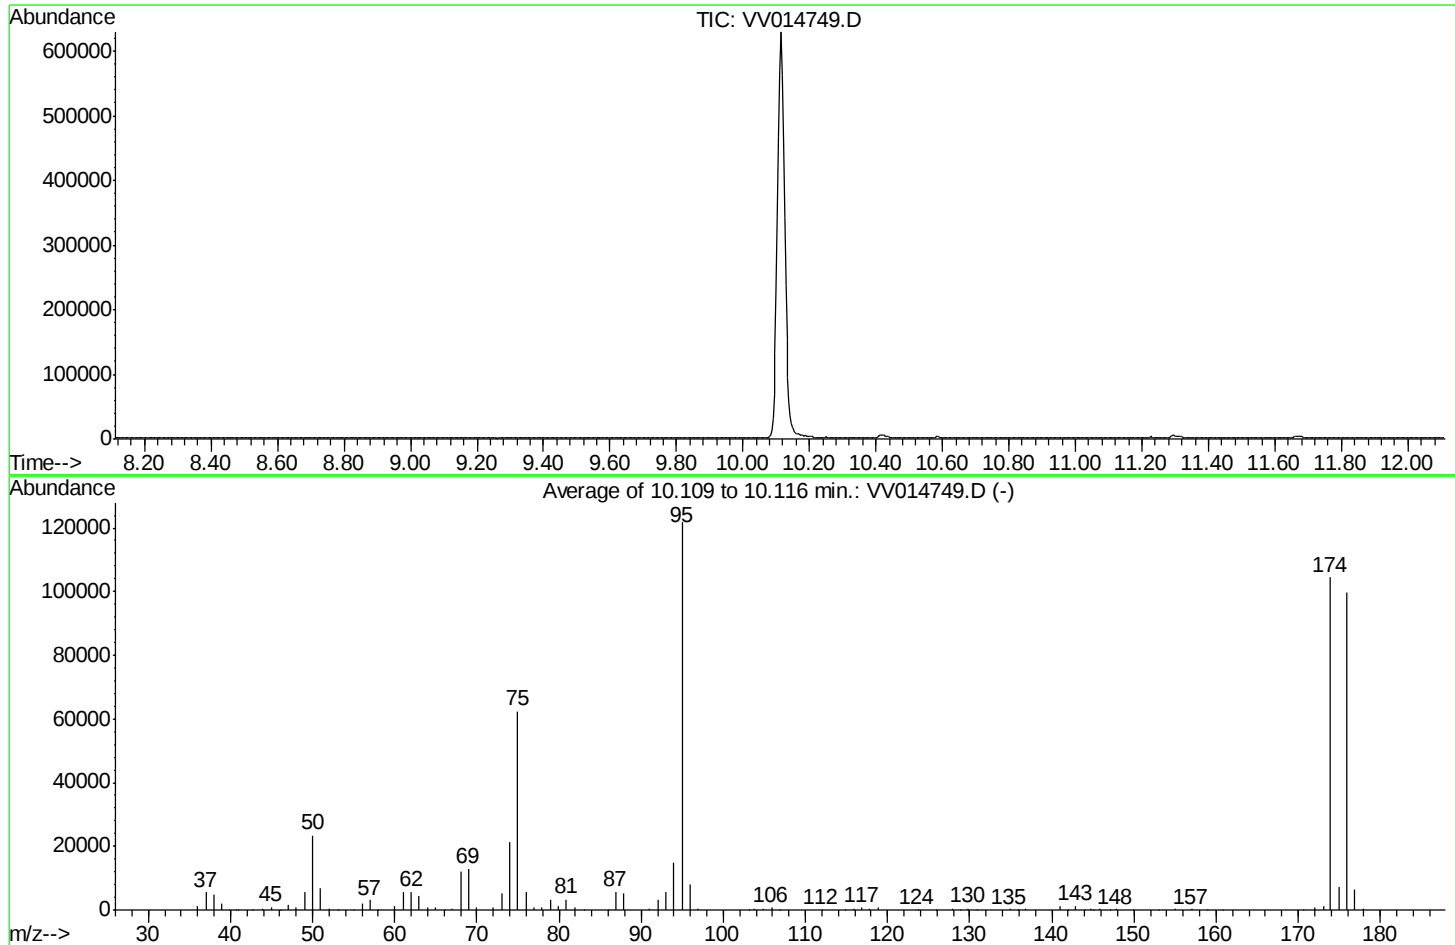

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	23394	PASS
75	95	30	80	51.2	62317	PASS
95	95	100	100	100.0	121749	PASS
96	95	5	9	6.7	8161	PASS
173	174	0.00	2	1.2	1243	PASS
174	95	50	120	85.8	104456	PASS
175	174	5	9	7.0	7335	PASS
176	174	95	101	95.4	99701	PASS
177	176	5	9	6.6	6604	PASS

m/z	Abundance
35.00	125.0
36.00	1349.0
37.00	5358.0
38.00	4873.0
39.00	2063.0
39.90	479.0
40.70	107.0
41.90	106.0
42.70	182.0
43.90	1210.0
45.00	931.0
46.10	196.0
47.00	1753.0
47.90	731.0
49.00	5071.0
50.00	22088.0
51.00	7023.0
52.00	293.0
53.00	172.0
55.10	301.0
56.00	1897.0
57.00	2928.0
57.90	197.0
59.90	1065.0
61.00	5117.0
62.00	5477.0
63.00	4310.0
64.00	650.0
65.00	560.0
66.10	189.0
67.00	367.0
68.00	11478.0
69.00	12391.0
70.00	862.0
72.00	933.0
73.00	5064.0
74.00	20312.0
75.00	58736.0
76.00	5518.0
77.00	889.0
77.90	606.0
78.90	3043.0
79.90	1012.0
80.90	2959.0
81.90	791.0
83.10	118.0
86.00	144.0
86.90	5394.0
87.90	4779.0
91.00	474.0
92.00	2975.0
93.00	5373.0
94.00	13452.0
95.00	116088.0
96.00	7705.0
97.00	260.0
103.10	103.0
103.80	513.0
104.80	220.0
105.90	688.0
112.00	100.0
114.80	189.0
116.00	491.0
116.90	709.0
117.80	474.0
118.80	558.0
123.70	113.0
127.90	400.0
128.80	141.0
129.80	471.0
130.80	156.0
134.90	257.0
136.90	213.0
140.90	1126.0
141.90	198.0
142.90	1171.0
144.00	172.0
144.80	300.0
145.80	191.0
147.00	109.0
147.80	274.0
149.80	178.0
152.90	150.0
155.00	214.0
157.00	274.0
158.90	150.0
160.80	162.0
172.00	690.0
173.00	1347.0
173.90	95752.0
174.90	6621.0
175.90	91120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

176.90	6074.0
177.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	1326.0
37.00	5725.0
38.00	5059.0
39.00	2097.0
39.90	468.0
40.70	146.0
41.00	130.0
41.90	107.0
42.70	174.0
44.00	1294.0
45.00	913.0
46.00	228.0
47.00	1718.0
47.90	804.0
49.00	5707.0
50.00	24136.0
51.00	7180.0
52.00	274.0
53.10	163.0
54.90	294.0
56.00	2101.0
57.00	3235.0
58.00	178.0
60.00	1166.0
61.00	5746.0
62.00	6025.0
63.00	4456.0
64.00	686.0
65.00	634.0
66.00	151.0
67.00	404.0
68.00	12456.0
69.00	13373.0
70.00	825.0
72.00	929.0
73.00	5575.0
74.00	22376.0
75.00	64480.0
76.00	5896.0
77.00	978.0
77.80	689.0
78.90	3381.0
79.90	1117.0
80.90	3456.0
81.90	950.0
83.10	154.0
86.00	143.0
86.90	5811.0
87.90	5502.0
91.00	541.0
92.00	3275.0
93.00	5842.0
94.00	15316.0
95.00	125984.0
96.00	8554.0
96.90	258.0
103.10	116.0
103.80	566.0
104.80	233.0
105.90	710.0
106.90	114.0
112.00	126.0
114.80	218.0
116.00	505.0
116.90	733.0
117.80	492.0
118.80	680.0
123.70	118.0
125.90	108.0
128.00	506.0
128.90	165.0
129.80	501.0
130.90	179.0
134.90	328.0
136.80	250.0
141.00	1157.0
141.90	183.0
142.90	1408.0
143.90	126.0
144.80	284.0
145.80	265.0
147.80	324.0
149.80	197.0
152.90	175.0
155.00	249.0
157.00	308.0
158.90	107.0
160.70	218.0
170.60	132.0
171.90	897.0
173.10	1255.0
173.90	108104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

174.90	7540.0
175.90	102608.0
176.90	6835.0
177.90	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.10	115.0
36.00	1128.0
37.00	5585.0
38.00	4758.0
39.00	1912.0
39.90	498.0
40.60	156.0
41.00	138.0
41.90	106.0
42.80	113.0
44.00	1368.0
45.00	941.0
46.00	220.0
47.00	1393.0
47.90	740.0
49.00	5645.0
50.00	23960.0
51.00	6762.0
52.00	229.0
53.10	147.0
54.90	279.0
56.00	1999.0
57.00	3200.0
58.00	145.0
60.00	1125.0
61.00	5760.0
62.00	5872.0
63.00	4373.0
64.00	625.0
65.00	705.0
65.90	106.0
67.00	365.0
68.00	12311.0
69.00	13260.0
70.00	776.0
72.00	788.0
73.00	5628.0
74.00	21704.0
75.00	63736.0
76.00	5758.0
77.00	939.0
77.80	693.0
78.90	3464.0
79.90	1125.0
80.90	3555.0
81.90	984.0
83.00	174.0
86.00	125.0
86.90	5717.0
87.90	5459.0
91.00	496.0
92.00	3220.0
93.00	5692.0
94.00	15442.0
95.00	123176.0
96.00	8225.0
96.90	227.0
103.00	117.0
103.80	568.0
104.80	209.0
105.90	624.0
106.80	128.0
112.00	149.0
114.80	213.0
115.90	468.0
116.90	750.0
117.80	472.0
118.80	745.0
123.70	125.0
125.90	126.0
127.90	511.0
128.90	205.0
129.90	480.0
130.90	230.0
134.90	380.0
135.80	108.0
136.80	299.0
141.00	1183.0
142.00	183.0
142.90	1483.0
144.80	199.0
145.10	200.0
145.80	292.0
147.80	314.0
149.80	179.0
153.00	172.0
154.90	264.0
157.00	263.0
159.00	102.0
160.70	236.0
170.60	141.0
171.90	949.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

173.10	1129.0
173.90	109512.0
174.90	7844.0
175.90	105376.0
176.90	6905.0
177.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.20	165.0
40.00	409.0
41.90	130.0
44.00	703.0
51.30	103.0
55.00	116.0
151.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42