


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030620\
 Data File : VV014759.D
 Acq On : 06 Mar 2020 16:00
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB97

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 06 23:28:37 2020

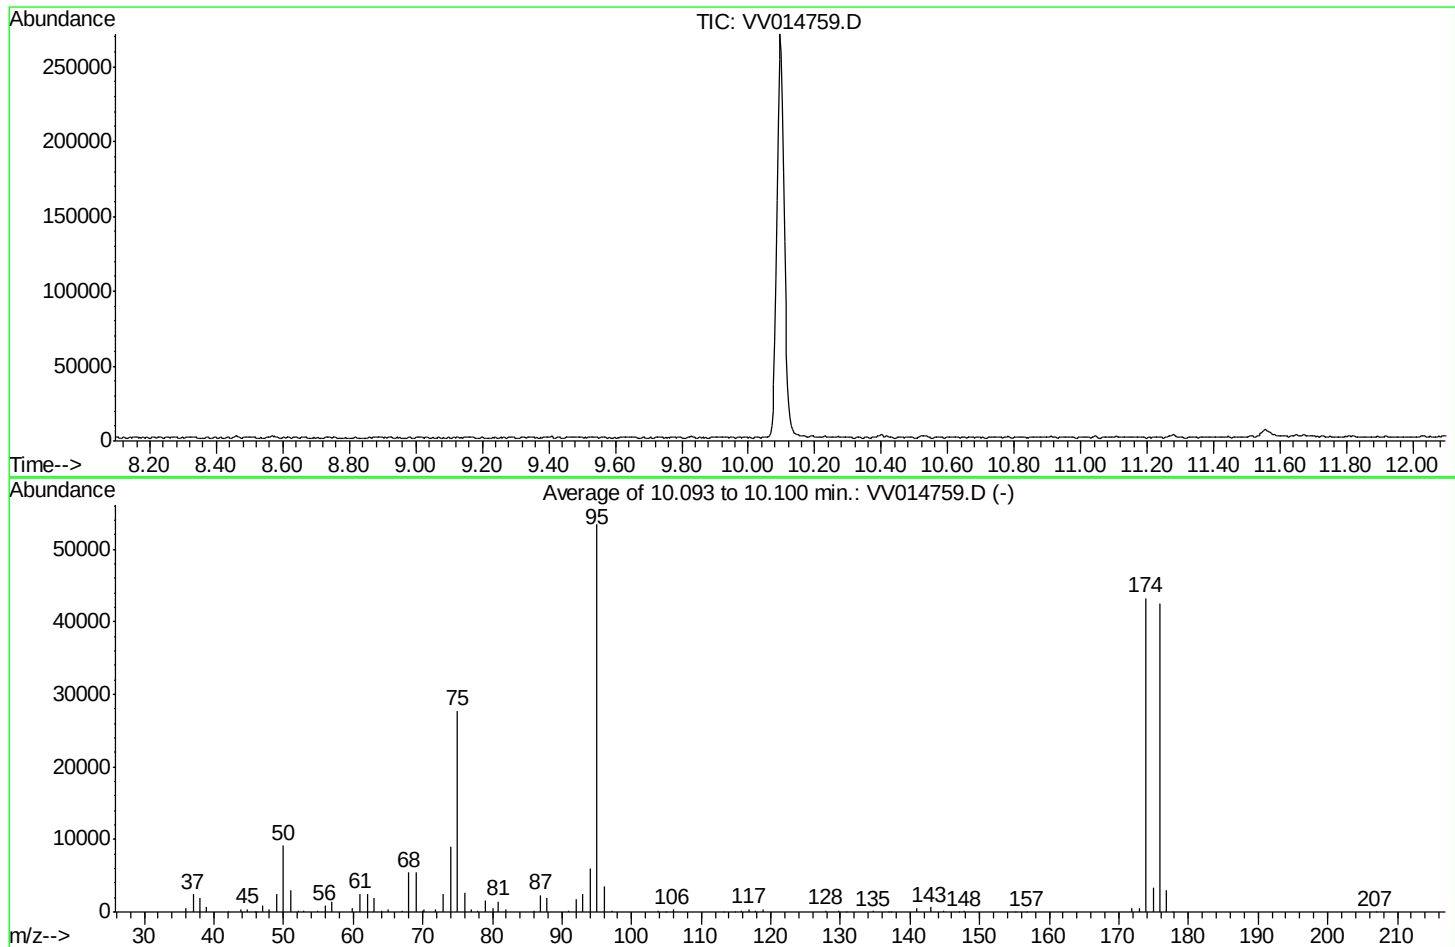

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	9143	PASS
75	95	30	80	52.0	27797	PASS
95	95	100	100	100.0	53464	PASS
96	95	5	9	6.5	3466	PASS
173	174	0.00	2	1.2	525	PASS
174	95	50	120	80.9	43274	PASS
175	174	5	9	7.9	3428	PASS
176	174	95	101	98.2	42488	PASS
177	176	5	9	6.9	2935	PASS

m/z	Abundance
35.90	549.0
37.00	2417.0
38.00	1956.0
39.00	873.0
39.90	457.0
43.00	172.0
43.90	1152.0
44.90	402.0
45.90	118.0
47.00	771.0
47.80	386.0
49.00	2623.0
50.00	9039.0
51.00	2997.0
52.10	235.0
54.80	170.0
56.00	980.0
57.00	1358.0
59.90	439.0
61.00	2430.0
62.10	2441.0
63.00	1858.0
64.00	254.0
65.00	372.0
67.00	157.0
68.00	5297.0
69.00	5322.0
69.90	446.0
71.90	282.0
73.00	2425.0
74.00	9066.0
75.00	27184.0
76.00	2707.0
76.90	307.0
77.90	242.0
79.00	1563.0
80.00	514.0
80.90	1341.0
81.90	403.0
86.00	116.0
87.00	2047.0
87.90	1941.0
90.90	274.0
92.00	1711.0
92.90	2336.0
94.00	6020.0
95.00	52592.0
96.00	3618.0
97.10	173.0
103.90	195.0
105.90	321.0
113.10	110.0
115.80	236.0
117.00	337.0
117.80	251.0
118.80	295.0
127.90	271.0
129.80	212.0
134.80	111.0
136.90	114.0
140.90	501.0
142.90	601.0
144.90	120.0
147.80	168.0
156.80	159.0
171.90	446.0
173.00	501.0
173.90	40776.0
174.90	3368.0
175.90	40600.0
176.90	2828.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.90	578.0
37.00	2512.0
38.00	1903.0
39.00	815.0
39.90	438.0
42.00	115.0
42.90	179.0
43.90	1400.0
44.80	447.0
47.00	824.0
47.80	440.0
49.00	2583.0
50.00	9404.0
51.00	3051.0
52.10	257.0
52.90	145.0
54.90	188.0
56.00	921.0
56.90	1427.0
59.90	493.0
61.00	2584.0
62.00	2499.0
63.00	1976.0
64.00	209.0
65.00	375.0
67.10	159.0
68.00	5694.0
69.00	5611.0
70.10	453.0
71.90	328.0
73.00	2589.0
74.00	9367.0
75.00	29096.0
76.00	2748.0
77.00	373.0
78.00	257.0
79.00	1612.0
80.00	618.0
80.90	1503.0
81.90	367.0
86.00	136.0
86.90	2452.0
87.90	1960.0
90.90	275.0
92.00	1794.0
93.00	2446.0
94.00	6253.0
95.00	55344.0
96.00	3611.0
97.10	167.0
103.80	192.0
105.00	102.0
106.00	299.0
113.10	116.0
114.90	119.0
115.90	238.0
117.00	409.0
117.80	281.0
118.90	363.0
128.00	267.0
129.80	202.0
130.80	118.0
134.80	120.0
140.90	520.0
142.90	628.0
144.90	100.0
147.00	110.0
147.80	181.0
156.90	108.0
171.90	475.0
173.00	553.0
173.90	44808.0
174.90	3547.0
175.90	43968.0
176.90	3078.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
35.90	513.0
37.00	2264.0
38.00	1722.0
39.00	742.0
39.90	485.0
42.00	117.0
42.90	158.0
44.00	1489.0
44.90	486.0
46.10	141.0
47.00	820.0
47.90	413.0
49.00	2195.0
50.00	8986.0
51.00	2962.0
52.10	219.0
53.00	175.0
54.90	192.0
56.00	738.0
57.00	1495.0
59.90	467.0
61.00	2493.0
62.00	2396.0
63.00	1875.0
64.00	220.0
65.00	323.0
67.10	153.0
68.00	5258.0
69.00	5242.0
70.10	417.0
71.90	323.0
73.00	2559.0
74.00	8804.0
75.00	27112.0
76.00	2336.0
77.00	423.0
78.00	297.0
78.90	1483.0
80.00	633.0
80.90	1514.0
81.90	307.0
86.10	118.0
86.90	2495.0
87.90	1788.0
90.90	246.0
92.00	1642.0
93.00	2410.0
94.00	5977.0
95.00	52456.0
96.00	3171.0
97.20	101.0
103.70	212.0
106.10	227.0
114.90	105.0
115.90	215.0
116.90	429.0
117.80	266.0
118.90	440.0
128.00	206.0
129.80	183.0
130.70	145.0
134.70	117.0
137.30	121.0
140.90	563.0
142.90	657.0
144.80	106.0
147.00	113.0
147.80	147.0
155.10	140.0
171.90	423.0
172.90	522.0
173.90	44240.0
174.90	3371.0
175.90	42896.0
176.90	2901.0
177.70	105.0
206.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

Scan 2789 (10.058 min): VV014759.D
BFB97

m/z	Abundance
38.80	181.0
39.90	631.0
40.90	239.0
42.90	169.0
43.90	1075.0
47.30	117.0
73.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97