


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV030719\
Data File : VV009521.D
Acq On : 07 Mar 2019 09:34
Operator : SY/MD
Sample : BFB71
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
Title : VOC Analysis
Last Update : Mon Mar 11 17:28:08 2019

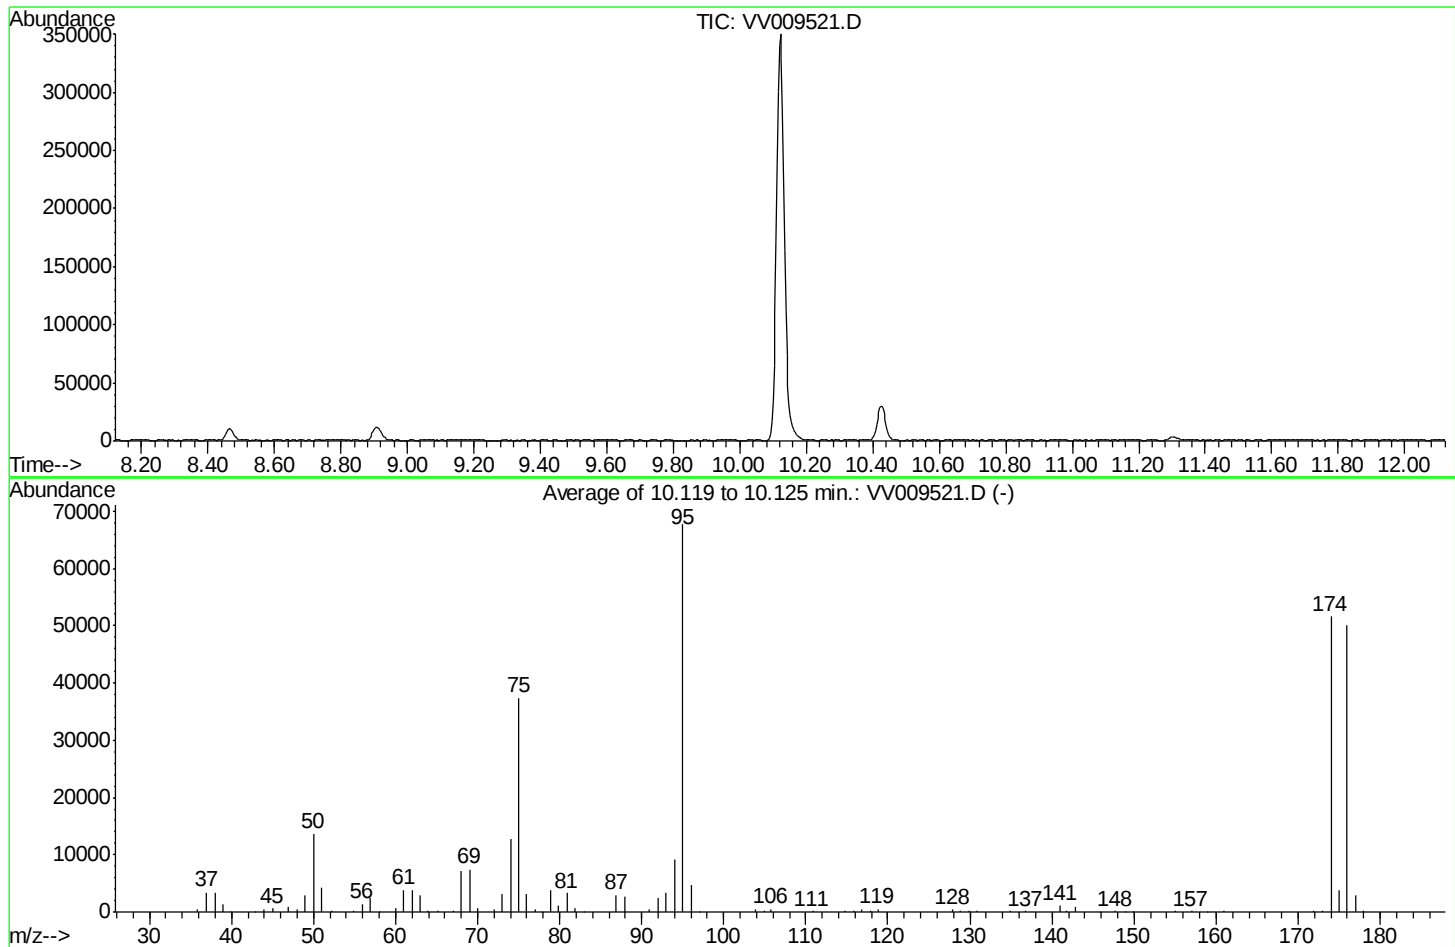

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	13660	PASS
75	95	30	80	55.2	37410	PASS
95	95	100	100	100.0	67720	PASS
96	95	5	9	6.9	4668	PASS
173	174	0.00	2	0.4	207	PASS
174	95	50	120	76.2	51584	PASS
175	174	5	9	7.4	3800	PASS
176	174	95	101	97.1	50064	PASS
177	176	5	9	5.8	2919	PASS

Scan 2795 (10.077 min): VV009521.D
BFB71

m/z	Abundance
39.80	339.0
44.00	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	565.0
37.00	3721.0
38.00	3162.0
39.00	1214.0
39.90	427.0
43.90	742.0
45.10	652.0
46.90	842.0
48.00	498.0
48.90	3024.0
50.00	13806.0
51.00	4393.0
52.10	197.0
54.90	209.0
55.90	1294.0
57.00	2504.0
58.00	120.0
59.90	756.0
61.00	4060.0
62.00	3815.0
63.00	2859.0
64.00	277.0
65.10	192.0
67.00	259.0
68.00	7010.0
69.00	7689.0
70.00	721.0
72.00	345.0
73.00	3124.0
74.00	12878.0
75.00	37584.0
76.00	3177.0
77.00	426.0
78.90	3929.0
79.90	1075.0
80.90	3353.0
81.80	866.0
83.00	137.0
86.90	2958.0
87.90	2835.0
90.90	373.0
92.00	2454.0
93.00	3398.0
94.00	9462.0
95.00	67960.0
96.00	4806.0
97.00	108.0
103.80	447.0
104.90	122.0
105.80	434.0
110.80	142.0
114.70	112.0
116.00	266.0
116.90	489.0
117.90	277.0
118.80	541.0
127.90	292.0
128.90	101.0
129.90	281.0
130.90	146.0
134.90	152.0
136.90	165.0
141.00	1104.0
141.80	147.0
142.90	1076.0
147.80	216.0
149.00	120.0
149.80	110.0
155.00	158.0
157.10	153.0
159.00	155.0
160.90	101.0
171.80	308.0
173.00	623.0
174.00	50560.0
175.00	3849.0
176.00	49056.0
177.00	2891.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	583.0
37.00	3480.0
38.00	3429.0
39.00	1272.0
39.90	462.0
42.80	119.0
43.90	720.0
45.00	607.0
47.00	860.0
48.00	449.0
48.90	3048.0
50.00	14210.0
51.00	4368.0
52.20	191.0
54.90	215.0
56.00	1445.0
56.90	2458.0
58.00	118.0
59.90	791.0
61.00	4051.0
62.00	3927.0
63.00	2925.0
64.00	256.0
65.10	166.0
67.00	207.0
68.00	7236.0
69.00	7624.0
70.00	781.0
72.00	345.0
73.00	3212.0
74.00	13033.0
75.00	38592.0
76.00	3190.0
77.00	416.0
77.80	166.0
78.90	3980.0
79.90	1067.0
80.90	3326.0
81.80	779.0
83.00	113.0
86.90	3195.0
88.00	2811.0
90.90	379.0
92.00	2621.0
93.00	3573.0
94.00	9515.0
95.00	69472.0
96.00	4830.0
97.00	120.0
103.80	413.0
104.90	134.0
105.80	496.0
110.80	142.0
114.70	131.0
115.90	232.0
116.90	515.0
117.90	244.0
118.80	582.0
127.90	362.0
128.90	113.0
129.90	334.0
130.90	135.0
134.90	154.0
136.80	187.0
141.00	1132.0
141.70	181.0
142.90	1035.0
145.90	111.0
147.70	215.0
149.00	100.0
155.00	145.0
157.00	173.0
159.00	141.0
160.90	133.0
171.80	319.0
174.00	53128.0
175.00	3930.0
176.00	51536.0
177.00	2979.0
178.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	552.0
37.00	2963.0
38.00	3259.0
39.00	1297.0
39.90	457.0
42.80	114.0
43.90	679.0
44.90	554.0
46.90	717.0
48.00	360.0
49.00	2729.0
50.00	12965.0
51.00	3893.0
52.10	151.0
54.90	216.0
56.00	1450.0
56.90	2226.0
60.00	704.0
61.00	3484.0
62.00	3721.0
63.10	2702.0
63.90	206.0
65.00	114.0
67.00	165.0
68.00	6945.0
69.00	7068.0
70.00	747.0
72.00	345.0
73.00	3121.0
74.00	12058.0
75.00	36056.0
76.00	2876.0
77.10	384.0
77.70	181.0
78.90	3609.0
79.90	982.0
80.90	3188.0
81.90	714.0
86.90	2848.0
88.00	2473.0
90.90	360.0
92.00	2372.0
93.00	3368.0
94.00	8734.0
95.00	65728.0
96.00	4368.0
97.10	122.0
103.80	333.0
104.90	132.0
105.80	484.0
110.80	116.0
114.70	123.0
115.80	241.0
116.80	523.0
117.90	236.0
118.80	528.0
128.00	383.0
128.80	160.0
129.90	319.0
130.90	127.0
134.90	155.0
136.80	187.0
141.00	1060.0
141.70	184.0
142.90	922.0
145.80	114.0
147.70	189.0
154.90	142.0
157.00	152.0
160.90	142.0
171.90	298.0
174.00	51064.0
175.00	3621.0
176.00	49600.0
177.00	2888.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71