




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/07/2024
Supervised By :Mahesh Dadoda 03/07/2024

Quant Time: Mar 07 04:31:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 07 04:30:42 2024
Response via : Initial Calibration

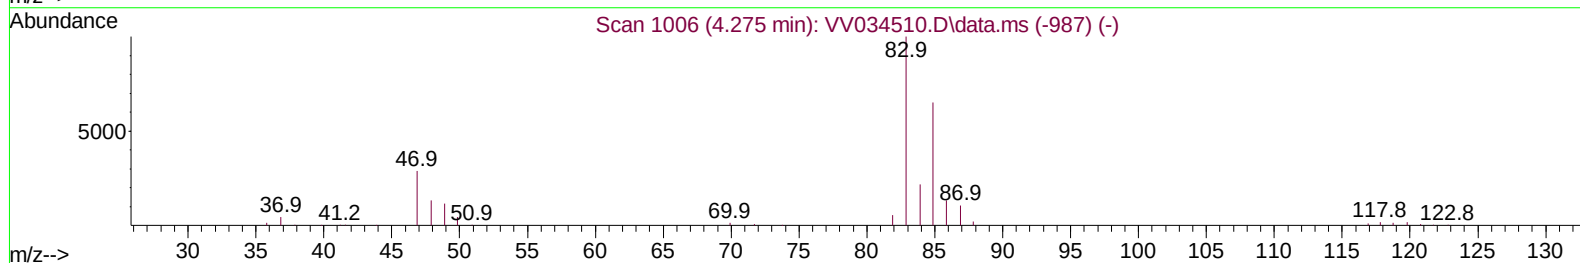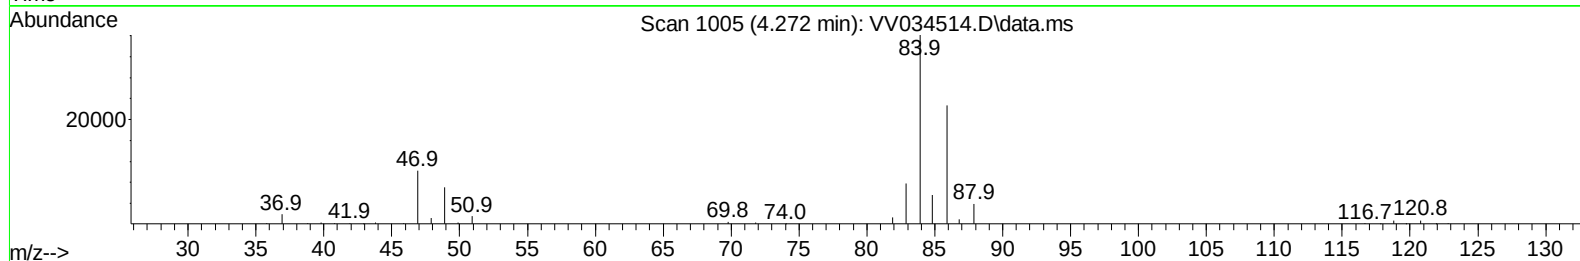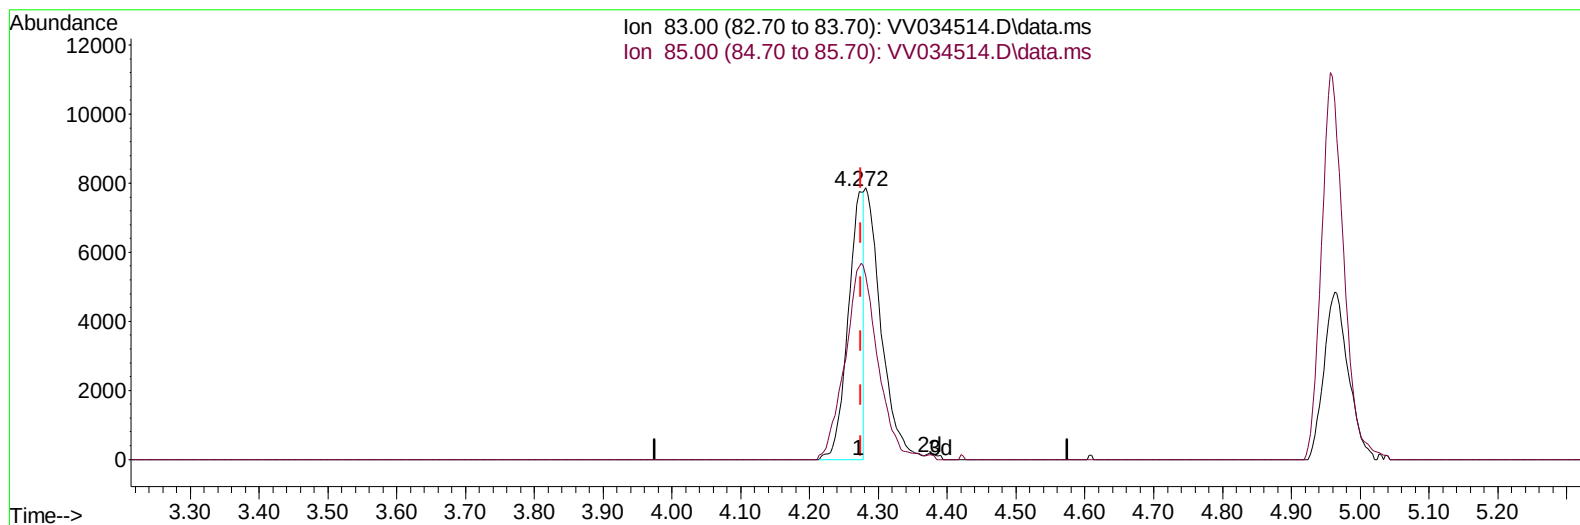

TIC: VV034514.D\data.ms

(25) Chloroform (T)

4.272min (-0.003) 2.68 ug/L

response 12237

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	65.00	72.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Manual IntegrationsAPPROVED

Quant Time: Mar 07 04:31:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 07 04:30:42 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/07/2024
Supervised By :Mahesh Dadoda 03/07/2024

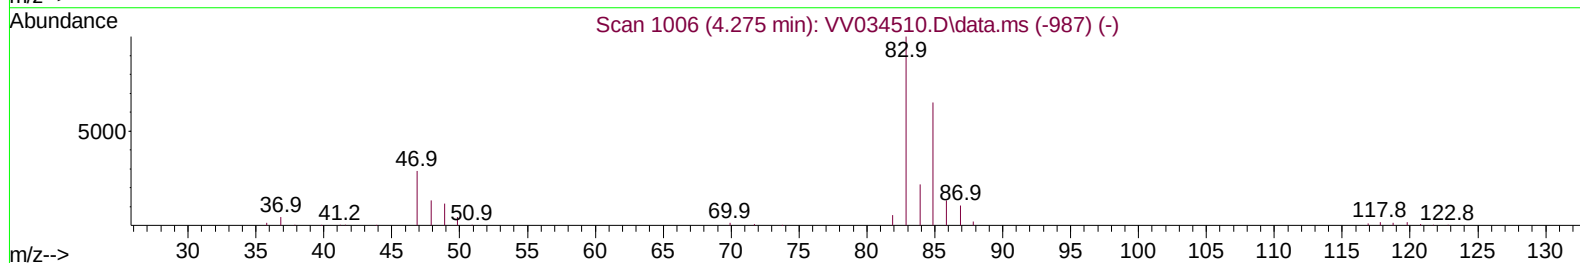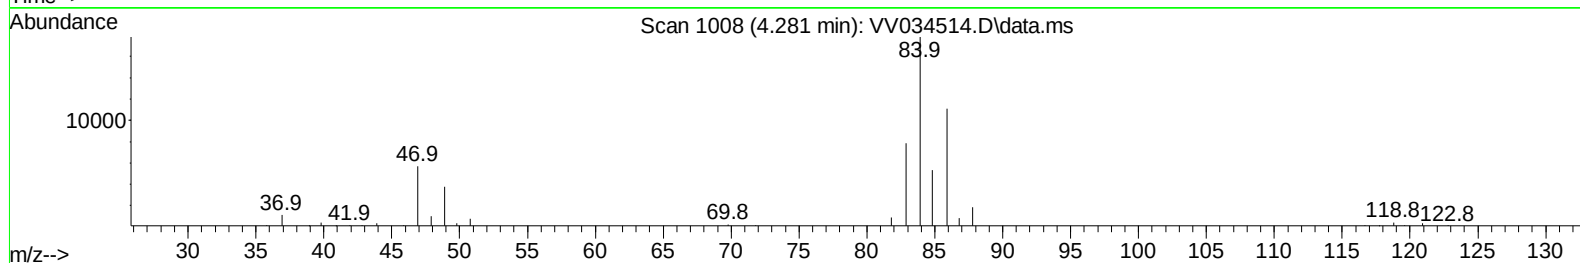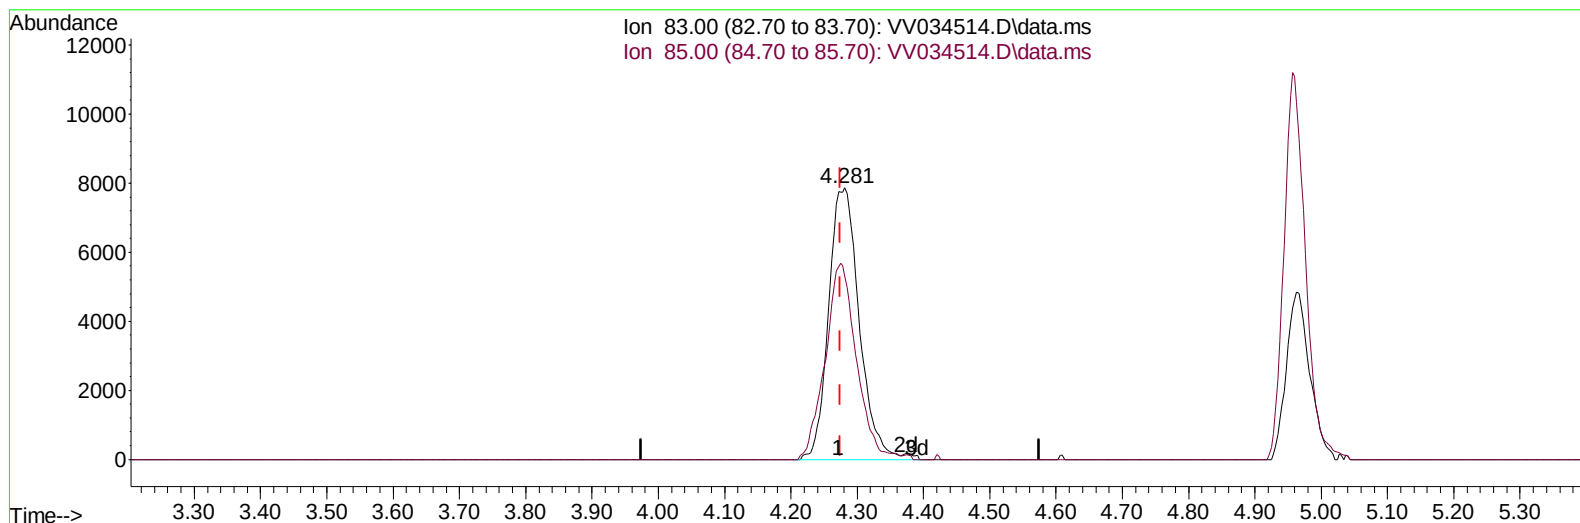

TIC: VV034514.D\data.ms

(25) Chloroform (T)

4.281min (+ 0.007) 5.55 ug/L m

response 25320

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	65.00	67.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034514.D
 Acq On : 06 Mar 2024 17:00
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/07/2024
 Supervised By :Mahesh Dadoda 03/07/2024

Quant Time: Mar 07 04:31:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 07 04:30:42 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		310062	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		285303	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		134844	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		109461	40.723	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	81.440%	
7) Chloroethane-d5	1.532	69		93225	44.519	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	89.040%	
11) 1,1-Dichloroethene-d2	2.056	65		50917	41.886	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	83.780%	
21) 2-Butanone-d5	3.793	46		199452	110.960	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	110.960%	
24) Chloroform-d	4.249	84		213444	44.912	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.820%	
26) 1,2-Dichloroethane-d4	4.941	65		148223	47.727	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	95.460%	
32) Benzene-d6	4.960	84		403686	46.883	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	93.760%	
36) 1,2-Dichloropropane-d6	5.989	67		129472	49.271	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	98.540%	
41) Toluene-d8	7.243	98		352311	45.214	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	90.420%	
43) trans-1,3-Dichloroprop...	7.555	79		56864	43.092	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	86.180%	
47) 2-Hexanone-d5	8.024	63		146514	111.656	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	111.660%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		167072	48.313	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	96.620%	
66) 1,2-Dichlorobenzene-d4	11.561	152		137412	49.855	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	99.700%	
Target Compounds							
13) Acetone	2.127	43		10358	4.793	ug/L	100
25) Chloroform	4.281	83		25320m	5.549	ug/L	
38) Bromodichloromethane	6.442	83		5095	1.562	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Manual IntegrationsAPPROVED

Quant Time: Mar 07 04:31:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 07 04:30:42 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/07/2024
Supervised By :Mahesh Dadoda 03/07/2024

