

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034512.D
 Acq On : 06 Mar 2024 16:11
 Operator : SY/MD
 Sample : P1681-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0U31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	166425	180655	14.63%	1.878%
2	1.529	145	152	169	rVB	143367	172151	13.94%	1.790%
3	2.056	307	316	327	rBV	292785	415968	33.69%	4.324%
4	2.429	428	432	433	rBV	458	291	0.02%	0.003%
5	2.883	568	573	574	rBV2	1042	799	0.06%	0.008%
6	3.134	648	651	655	rBV2	345	253	0.02%	0.003%
7	3.236	680	683	687	rVB	218	146	0.01%	0.002%
8	3.307	701	705	709	rBV2	321	208	0.02%	0.002%
9	3.375	723	726	728	rBV2	221	159	0.01%	0.002%
10	3.442	745	747	751	rBV	229	151	0.01%	0.002%
11	3.507	762	767	769	rBV2	152	156	0.01%	0.002%
12	3.658	811	814	815	rBV2	439	289	0.02%	0.003%
13	3.741	837	840	842	rVB2	344	165	0.01%	0.002%
14	3.786	845	854	895	rBV	106268	301564	24.42%	3.135%
15	4.246	983	997	1031	rBV	216278	555878	45.02%	5.779%
16	4.580	1092	1101	1107	rBV6	945	1485	0.12%	0.015%
17	4.625	1112	1115	1117	rBV2	322	167	0.01%	0.002%
18	4.642	1118	1120	1128	rVB3	339	417	0.03%	0.004%
19	4.760	1153	1157	1160	rBV3	310	209	0.02%	0.002%
20	4.780	1160	1163	1165	rBV2	243	161	0.01%	0.002%
21	4.818	1169	1175	1178	rBV2	276	350	0.03%	0.004%
22	4.953	1201	1217	1249	rBV2	472871	1234859	100.00%	12.838%
23	5.297	1319	1324	1327	rBV2	417	450	0.04%	0.005%
24	5.333	1332	1335	1336	rBV2	407	226	0.02%	0.002%
25	5.407	1355	1358	1361	rBV2	592	367	0.03%	0.004%
26	5.426	1361	1364	1365	rBV	311	160	0.01%	0.002%
27	5.490	1380	1384	1385	rVV3	481	345	0.03%	0.004%
28	5.532	1386	1397	1432	rVV	369189	758879	61.45%	7.889%
29	5.831	1480	1490	1512	rVB6	9979	23703	1.92%	0.246%
30	5.989	1519	1539	1563	rBV2	271719	562359	45.54%	5.846%
31	6.288	1627	1632	1635	rBV4	374	301	0.02%	0.003%
32	6.323	1641	1643	1648	rVB2	383	275	0.02%	0.003%
33	6.349	1649	1651	1654	rVB	472	181	0.01%	0.002%
34	6.368	1654	1657	1659	rBV2	313	207	0.02%	0.002%
35	6.458	1681	1685	1691	rVB2	538	574	0.05%	0.006%
36	6.510	1699	1701	1705	rVB2	335	206	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034512.D
Acq On : 06 Mar 2024 16:11
Operator : SY/MD
Sample : P1681-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

37	6.532	1705	1708	1712	rBV2	317	254	0.02%	0.003%
38	6.590	1717	1726	1729	rBV2	1030	1547	0.13%	0.016%
39	6.731	1767	1770	1775	rVB3	364	270	0.02%	0.003%
40	6.773	1776	1783	1787	rBV	203	245	0.02%	0.003%
41	6.815	1793	1796	1799	rBV	204	160	0.01%	0.002%
42	6.915	1814	1827	1854	rBV	137109	260696	21.11%	2.710%
43	7.137	1891	1896	1897	rBV2	878	622	0.05%	0.006%
44	7.243	1918	1929	1958	rBV	531153	934967	75.71%	9.720%
45	7.500	2007	2009	2014	rVB3	454	289	0.02%	0.003%
46	7.555	2014	2026	2053	rBV	91281	171557	13.89%	1.784%
47	7.818	2104	2108	2110	rBV	379	184	0.01%	0.002%
48	7.834	2110	2113	2116	rBV	281	165	0.01%	0.002%
49	7.857	2116	2120	2121	rBV2	467	320	0.03%	0.003%
50	7.937	2143	2145	2148	rVB	312	168	0.01%	0.002%
51	7.992	2158	2162	2163	rBV	280	176	0.01%	0.002%
52	8.024	2163	2172	2212	rBV	384643	703742	56.99%	7.316%
53	8.593	2346	2349	2351	rVB2	428	210	0.02%	0.002%
54	8.635	2358	2362	2363	rBV2	347	209	0.02%	0.002%
55	8.648	2364	2366	2369	rBV2	198	166	0.01%	0.002%
56	8.783	2398	2408	2437	rBV	552039	910833	73.76%	9.469%
57	9.030	2483	2485	2487	rVB2	456	175	0.01%	0.002%
58	9.162	2523	2526	2531	rBV	479	447	0.04%	0.005%
59	9.201	2535	2538	2539	rBV2	415	254	0.02%	0.003%
60	9.259	2552	2556	2559	rBV	219	199	0.02%	0.002%
61	9.426	2606	2608	2613	rVB2	383	287	0.02%	0.003%
62	9.487	2622	2627	2637	rBV3	930	1433	0.12%	0.015%
63	9.802	2722	2725	2729	rBV2	298	170	0.01%	0.002%
64	9.873	2743	2747	2755	rBV3	482	590	0.05%	0.006%
65	9.960	2768	2774	2776	rBV3	2448	2585	0.21%	0.027%
66	10.153	2821	2834	2859	rBV	381662	598969	48.51%	6.227%
67	10.329	2880	2889	2899	rBV6	1865	3259	0.26%	0.034%
68	10.407	2909	2913	2914	rBV2	273	175	0.01%	0.002%
69	10.426	2917	2919	2925	rVB2	276	190	0.02%	0.002%
70	10.455	2925	2928	2930	rBV2	247	150	0.01%	0.002%
71	10.471	2930	2933	2935	rBV	387	236	0.02%	0.002%
72	10.603	2970	2974	2980	rVB3	251	276	0.02%	0.003%
73	10.834	3042	3046	3047	rBV	293	165	0.01%	0.002%
74	10.866	3052	3056	3060	rVB3	1034	889	0.07%	0.009%
75	10.976	3086	3090	3093	rBV2	377	332	0.03%	0.003%
76	11.107	3128	3131	3133	rBV2	329	223	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034512.D
 Acq On : 06 Mar 2024 16:11
 Operator : SY/MD
 Sample : P1681-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0U31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.130	3135	3138	3141	rBV3	617	443	0.04%	0.005%
78	11.185	3144	3155	3180	rBV	569864	888375	71.94%	9.236%
79	11.471	3236	3244	3249	rBV6	2947	4043	0.33%	0.042%
80	11.516	3250	3258	3260	rBV6	1472	2058	0.17%	0.021%
81	11.561	3261	3272	3293	rVV	545149	873802	70.76%	9.084%
82	11.805	3345	3348	3351	rVB2	295	153	0.01%	0.002%
83	11.831	3354	3356	3360	rBV2	211	153	0.01%	0.002%
84	11.950	3391	3393	3394	rBV	429	154	0.01%	0.002%
85	12.062	3422	3428	3430	rBV4	1026	1072	0.09%	0.011%
86	12.201	3461	3471	3475	rBV5	753	1263	0.10%	0.013%
87	12.320	3501	3508	3513	rBV4	2529	3046	0.25%	0.032%
88	12.532	3571	3574	3576	rBV2	243	191	0.02%	0.002%
89	12.596	3587	3594	3597	rBV4	1410	1572	0.13%	0.016%
90	12.625	3600	3603	3607	rBV3	981	922	0.07%	0.010%
91	12.667	3613	3616	3620	rBV3	612	532	0.04%	0.006%
92	12.779	3648	3651	3652	rBV	320	171	0.01%	0.002%
93	12.950	3702	3704	3707	rBV	224	176	0.01%	0.002%
94	13.204	3780	3783	3792	rVB6	2184	2375	0.19%	0.025%
95	13.332	3820	3823	3826	rBV3	716	472	0.04%	0.005%
96	13.451	3852	3860	3869	rBV3	6911	10937	0.89%	0.114%
97	13.554	3884	3892	3899	rBV6	4565	6757	0.55%	0.070%
98	13.648	3913	3921	3927	rBV6	4880	7030	0.57%	0.073%
99	13.754	3951	3954	3956	rBV2	279	171	0.01%	0.002%
100	14.226	4098	4101	4103	rBV2	746	552	0.04%	0.006%




Sum of corrected areas: 9618918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034512.D
Acq On : 06 Mar 2024 16:11
Operator : SY/MD
Sample : P1681-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

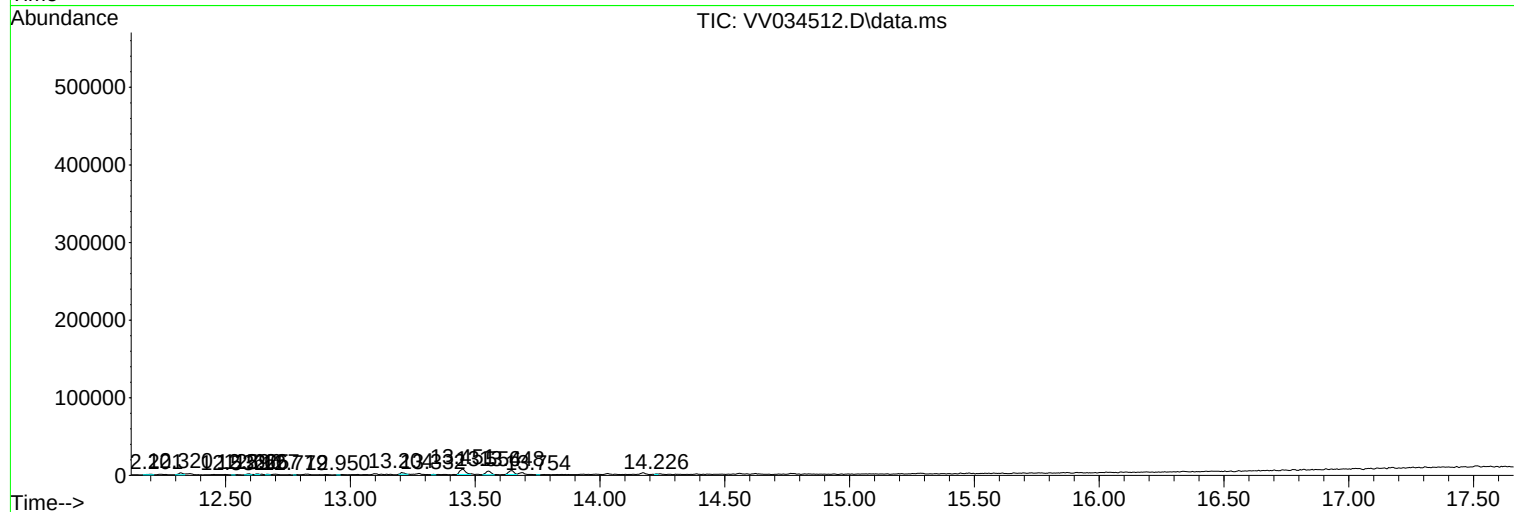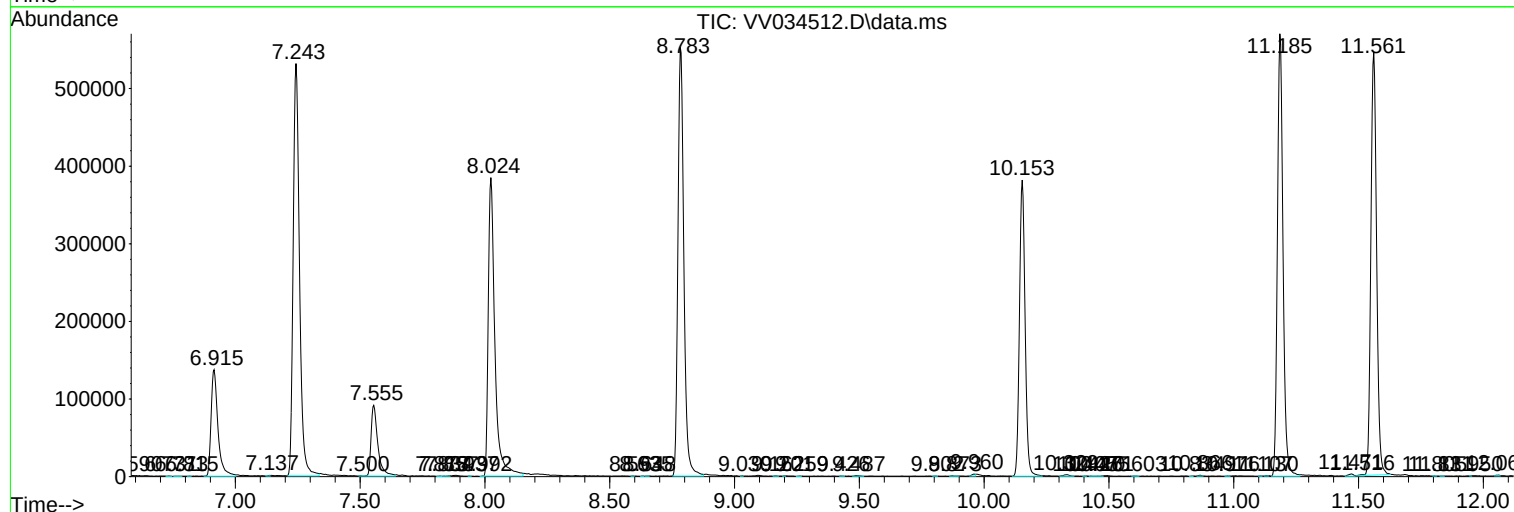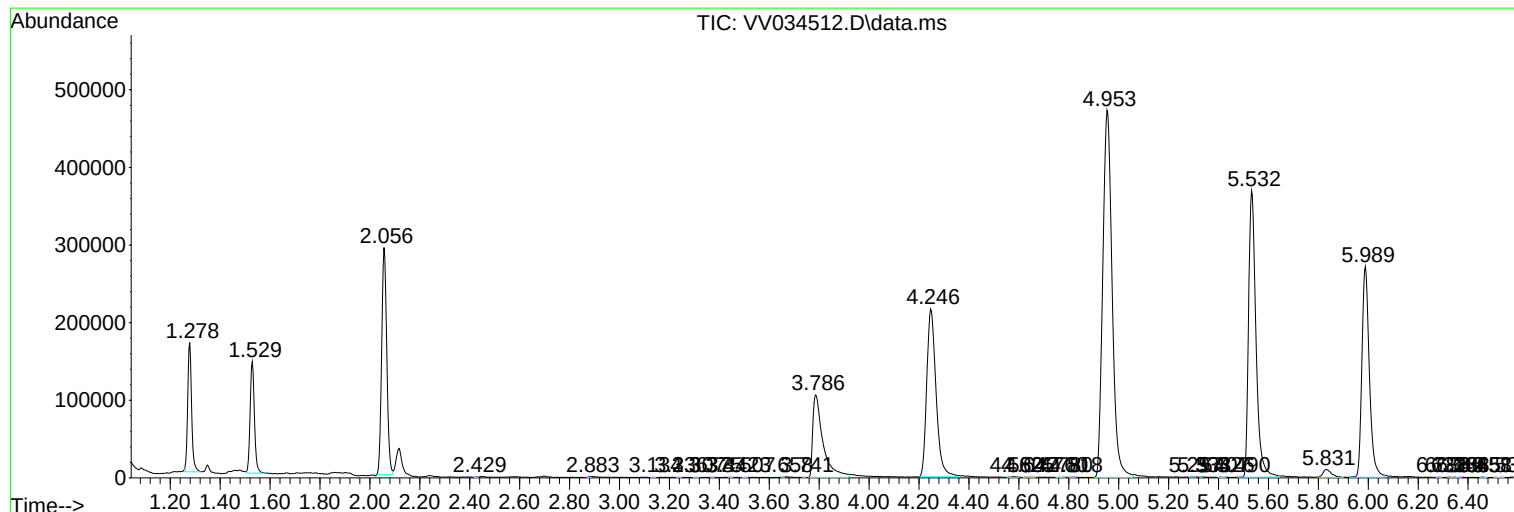

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034512.D
Acq On : 06 Mar 2024 16:11
Operator : SY/MD
Sample : P1681-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034512.D
Acq On : 06 Mar 2024 16:11
Operator : SY/MD
Sample : P1681-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0U31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
