

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034513.D
 Acq On : 06 Mar 2024 16:36
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	170428	188703	15.35%	1.978%
2	1.532	146	153	169	rVB	149102	173917	14.14%	1.823%
3	2.056	306	316	330	rBV	290530	424721	34.54%	4.452%
4	2.574	474	477	480	rBV	327	273	0.02%	0.003%
5	2.651	499	501	505	rVB2	288	155	0.01%	0.002%
6	2.719	520	522	524	rBV	237	117	0.01%	0.001%
7	2.863	565	567	569	rBV2	220	103	0.01%	0.001%
8	2.944	586	592	598	rBV3	237	398	0.03%	0.004%
9	2.995	606	608	613	rVB2	306	160	0.01%	0.002%
10	3.034	613	620	628	rBV2	210	292	0.02%	0.003%
11	3.076	629	633	637	rBV2	160	179	0.01%	0.002%
12	3.105	640	642	645	rBV	178	91	0.01%	0.001%
13	3.146	653	655	658	rVB2	243	120	0.01%	0.001%
14	3.214	674	676	680	rVB	342	172	0.01%	0.002%
15	3.297	698	702	706	rBV2	206	201	0.02%	0.002%
16	3.362	716	722	724	rBV	282	262	0.02%	0.003%
17	3.407	732	736	739	rBV2	177	146	0.01%	0.002%
18	3.477	755	758	761	rBV	183	129	0.01%	0.001%
19	3.497	761	764	766	rVV2	192	115	0.01%	0.001%
20	3.548	777	780	784	rVB	150	126	0.01%	0.001%
21	3.574	784	788	791	rBV2	187	183	0.01%	0.002%
22	3.596	793	795	800	rVV3	337	211	0.02%	0.002%
23	3.648	808	811	816	rVB2	272	189	0.02%	0.002%
24	3.764	843	847	848	rBV2	200	97	0.01%	0.001%
25	3.793	848	856	906	rBV	105931	320859	26.10%	3.363%
26	4.249	982	998	1033	rBV	206163	574788	46.75%	6.024%
27	4.545	1087	1090	1096	rVB4	654	636	0.05%	0.007%
28	4.567	1096	1097	1098	rBV	306	103	0.01%	0.001%
29	4.622	1111	1114	1117	rVB3	310	180	0.01%	0.002%
30	4.693	1133	1136	1140	rVB3	285	177	0.01%	0.002%
31	4.744	1150	1152	1155	rVB2	283	128	0.01%	0.001%
32	4.760	1155	1157	1162	rVB2	348	214	0.02%	0.002%
33	4.789	1162	1166	1169	rBV	360	343	0.03%	0.004%
34	4.831	1176	1179	1183	rVB2	431	306	0.02%	0.003%
35	4.857	1183	1187	1192	rBV3	338	374	0.03%	0.004%
36	4.957	1202	1218	1247	rBV2	468650	1229575	100.00%	12.887%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034513.D
 Acq On : 06 Mar 2024 16:36
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.365	1342	1345	1346	rBV	221	113	0.01%	0.001%
38	5.416	1356	1361	1363	rBV3	326	321	0.03%	0.003%
39	5.445	1366	1370	1371	rBV2	263	162	0.01%	0.002%
40	5.532	1386	1397	1434	rBV	354604	734233	59.71%	7.696%
41	5.828	1478	1489	1510	rBV2	25557	56137	4.57%	0.588%
42	5.989	1526	1539	1562	rBV	268583	555754	45.20%	5.825%
43	6.230	1612	1614	1619	rVB2	324	233	0.02%	0.002%
44	6.256	1620	1622	1624	rVV2	293	104	0.01%	0.001%
45	6.301	1634	1636	1639	rBV2	199	117	0.01%	0.001%
46	6.374	1656	1659	1661	rBV2	170	136	0.01%	0.001%
47	6.442	1669	1680	1691	rBV4	5890	11128	0.91%	0.117%
48	6.587	1720	1725	1726	rBV3	672	516	0.04%	0.005%
49	6.667	1745	1750	1753	rBV3	410	379	0.03%	0.004%
50	6.831	1798	1801	1808	rVB2	182	170	0.01%	0.002%
51	6.915	1816	1827	1851	rBV	138287	261986	21.31%	2.746%
52	7.243	1917	1929	1952	rBV	530254	932368	75.83%	9.772%
53	7.554	2016	2026	2050	rBV	94443	172376	14.02%	1.807%
54	7.728	2078	2080	2081	rBV	328	132	0.01%	0.001%
55	7.815	2103	2107	2110	rBV2	193	215	0.02%	0.002%
56	7.857	2115	2120	2121	rBV2	392	303	0.02%	0.003%
57	8.024	2163	2172	2210	rBV	408946	753271	61.26%	7.895%
58	8.571	2340	2342	2346	rBV2	200	139	0.01%	0.001%
59	8.606	2351	2353	2361	rVB2	381	301	0.02%	0.003%
60	8.641	2362	2364	2367	rVB2	251	128	0.01%	0.001%
61	8.786	2398	2409	2438	rBV	529316	876078	71.25%	9.182%
62	9.095	2503	2505	2509	rBV4	413	261	0.02%	0.003%
63	9.159	2522	2525	2528	rBV2	271	165	0.01%	0.002%
64	9.230	2541	2547	2548	rBV	295	240	0.02%	0.003%
65	9.265	2555	2558	2561	rBV2	166	114	0.01%	0.001%
66	9.313	2570	2573	2577	rBV2	166	104	0.01%	0.001%
67	9.477	2621	2624	2626	rBV	276	143	0.01%	0.001%
68	9.503	2626	2632	2633	rBV2	376	341	0.03%	0.004%
69	9.532	2639	2641	2646	rVB3	322	198	0.02%	0.002%
70	9.577	2652	2655	2659	rBV2	211	136	0.01%	0.001%
71	9.657	2677	2680	2683	rBV2	316	189	0.02%	0.002%
72	9.686	2686	2689	2691	rBV	296	175	0.01%	0.002%
73	9.779	2714	2718	2725	rBV2	399	435	0.04%	0.005%
74	9.828	2728	2733	2736	rVB2	284	275	0.02%	0.003%
75	10.152	2823	2834	2858	rBV	353218	561701	45.68%	5.887%
76	10.294	2874	2878	2879	rBV	233	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034513.D
 Acq On : 06 Mar 2024 16:36
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.307	2879	2882	2884	rBV2	298	197	0.02%	0.002%
78	10.323	2885	2887	2889	rBV2	317	158	0.01%	0.002%
79	10.432	2917	2921	2922	rBV	219	133	0.01%	0.001%
80	10.577	2963	2966	2969	rVB2	300	181	0.01%	0.002%
81	10.683	2996	2999	3001	rBV	155	104	0.01%	0.001%
82	10.712	3005	3008	3009	rBV	226	103	0.01%	0.001%
83	10.786	3030	3031	3035	rBV2	214	126	0.01%	0.001%
84	10.844	3046	3049	3052	rBV	204	160	0.01%	0.002%
85	10.866	3052	3056	3058	rBV	368	277	0.02%	0.003%
86	10.963	3083	3086	3089	rBV	388	278	0.02%	0.003%
87	11.037	3106	3109	3113	rBV	259	176	0.01%	0.002%
88	11.098	3126	3128	3132	rBV	256	189	0.02%	0.002%
89	11.130	3136	3138	3140	rBV3	472	167	0.01%	0.002%
90	11.185	3145	3155	3178	rBV	525377	826382	67.21%	8.661%
91	11.442	3231	3235	3238	rBV2	325	233	0.02%	0.002%
92	11.503	3251	3254	3257	rBV	173	108	0.01%	0.001%
93	11.561	3260	3272	3296	rBV	544819	865817	70.42%	9.075%
94	12.204	3460	3472	3477	rBB3	632	1154	0.09%	0.012%
95	12.429	3540	3542	3543	rBV3	343	109	0.01%	0.001%
96	12.699	3624	3626	3629	rBV	262	110	0.01%	0.001%
97	13.069	3738	3741	3743	rBV	452	276	0.02%	0.003%
98	13.451	3854	3860	3867	rBV5	1950	3081	0.25%	0.032%
99	13.689	3930	3934	3940	rBV4	775	948	0.08%	0.010%
100	13.853	3983	3985	3988	rBV	375	285	0.02%	0.003%


Sum of corrected areas: 9540902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034513.D
Acq On : 06 Mar 2024 16:36
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

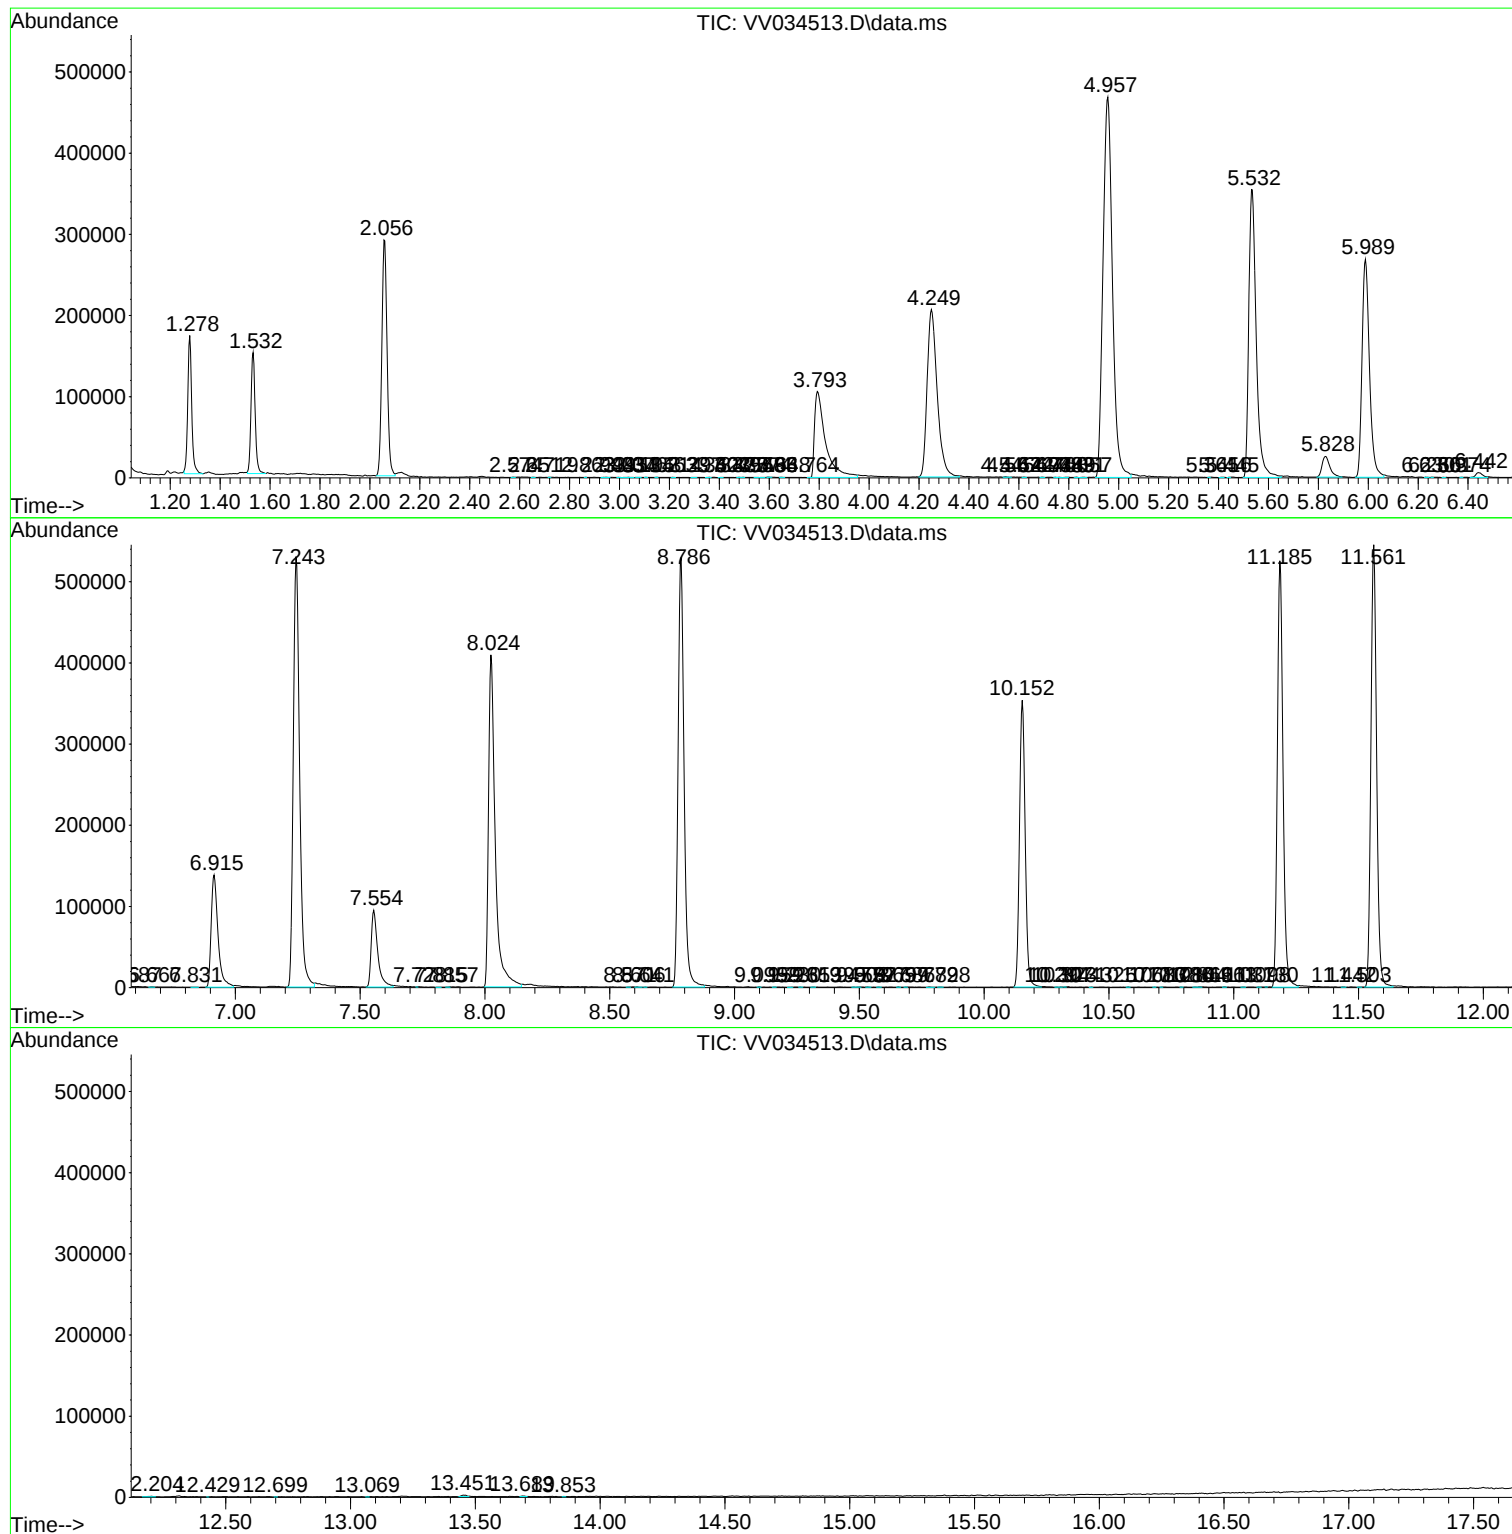

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034513.D
Acq On : 06 Mar 2024 16:36
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034513.D
Acq On : 06 Mar 2024 16:36
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------