

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V030724\
 Data File : VV034514.D
 Acq On : 06 Mar 2024 17:00
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	51	rBV	7055	7020	0.56%	0.072%
2	1.278	67	74	90	rVB	172705	187014	14.96%	1.930%
3	1.532	145	153	175	rVB	153055	179703	14.38%	1.854%
4	2.056	306	316	330	rBV	298147	433920	34.72%	4.478%
5	2.236	369	372	373	rBV	533	279	0.02%	0.003%
6	2.400	421	423	428	rVB2	460	314	0.03%	0.003%
7	2.446	434	437	444	rVB3	1080	1061	0.08%	0.011%
8	2.529	458	463	470	rBV4	759	1074	0.09%	0.011%
9	2.619	485	491	494	rBV4	497	453	0.04%	0.005%
10	2.716	515	521	525	rBV2	263	271	0.02%	0.003%
11	2.863	561	567	572	rVB2	438	628	0.05%	0.006%
12	2.892	572	576	578	rBV2	699	634	0.05%	0.007%
13	3.002	608	610	617	rVB2	387	363	0.03%	0.004%
14	3.034	617	620	623	rBV	298	219	0.02%	0.002%
15	3.076	628	633	638	rBV2	289	239	0.02%	0.002%
16	3.105	638	642	646	rBV2	259	230	0.02%	0.002%
17	3.420	735	740	742	rBV	325	273	0.02%	0.003%
18	3.671	815	818	824	rVB2	291	226	0.02%	0.002%
19	3.793	847	856	893	rBV	109178	319193	25.54%	3.294%
20	4.153	966	968	973	rBV5	348	264	0.02%	0.003%
21	4.249	981	998	1036	rBV2	206123	571715	45.75%	5.900%
22	4.478	1066	1069	1071	rBV	330	270	0.02%	0.003%
23	4.622	1112	1114	1119	rVB2	360	243	0.02%	0.003%
24	4.706	1137	1140	1143	rBV	409	256	0.02%	0.003%
25	4.728	1143	1147	1155	rBV3	257	431	0.03%	0.004%
26	4.802	1168	1170	1173	rVB2	373	196	0.02%	0.002%
27	4.828	1173	1178	1180	rBV3	295	279	0.02%	0.003%
28	4.867	1189	1190	1193	rVV	486	207	0.02%	0.002%
29	4.957	1202	1218	1250	rBV2	473244	1249754	100.00%	12.897%
30	5.265	1312	1314	1318	rVB3	384	201	0.02%	0.002%
31	5.336	1331	1336	1337	rBV3	336	239	0.02%	0.002%
32	5.388	1349	1352	1358	rVB2	370	253	0.02%	0.003%
33	5.423	1360	1363	1366	rBV3	379	225	0.02%	0.002%
34	5.532	1387	1397	1435	rVV	360466	743823	59.52%	7.676%
35	5.828	1478	1489	1510	rBV2	25856	57307	4.59%	0.591%
36	5.924	1516	1519	1522	rVB	288	207	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034514.D
 Acq On : 06 Mar 2024 17:00
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.989	1525	1539	1573	rBV	273640	573799	45.91%	5.921%
38	6.442	1670	1680	1699	rVV3	7108	14135	1.13%	0.146%
39	6.584	1720	1724	1726	rBV2	891	732	0.06%	0.008%
40	6.603	1727	1730	1732	rVB	493	325	0.03%	0.003%
41	6.793	1787	1789	1795	rVB2	356	224	0.02%	0.002%
42	6.915	1816	1827	1850	rBV	142123	270559	21.65%	2.792%
43	7.108	1884	1887	1889	rVB2	496	288	0.02%	0.003%
44	7.146	1889	1899	1903	rBV5	1264	1905	0.15%	0.020%
45	7.243	1918	1929	1955	rBV	536520	947400	75.81%	9.777%
46	7.400	1976	1978	1981	rVB2	608	244	0.02%	0.003%
47	7.555	2017	2026	2052	rBV	95503	174652	13.97%	1.802%
48	7.748	2082	2086	2090	rBV2	379	452	0.04%	0.005%
49	7.847	2114	2117	2120	rVB2	442	292	0.02%	0.003%
50	7.873	2120	2125	2128	rBV2	279	338	0.03%	0.003%
51	7.931	2141	2143	2148	rVB2	370	285	0.02%	0.003%
52	8.024	2163	2172	2210	rBV	417658	765458	61.25%	7.899%
53	8.387	2281	2285	2291	rVB4	636	683	0.05%	0.007%
54	8.564	2335	2340	2344	rVB4	333	307	0.02%	0.003%
55	8.625	2356	2359	2364	rVB2	345	271	0.02%	0.003%
56	8.786	2398	2409	2437	rBV	540559	887688	71.03%	9.160%
57	8.937	2453	2456	2458	rBV2	415	291	0.02%	0.003%
58	9.050	2488	2491	2496	rVB3	475	421	0.03%	0.004%
59	9.095	2503	2505	2508	rVB	517	252	0.02%	0.003%
60	9.374	2588	2592	2597	rVB	233	216	0.02%	0.002%
61	9.815	2724	2729	2731	rBV2	295	264	0.02%	0.003%
62	10.153	2822	2834	2857	rBV	361648	572899	45.84%	5.912%
63	10.281	2870	2874	2880	rVB2	342	317	0.03%	0.003%
64	10.333	2885	2890	2894	rVB2	545	600	0.05%	0.006%
65	10.770	3021	3026	3028	rBV2	213	212	0.02%	0.002%
66	10.786	3028	3031	3034	rVV2	316	267	0.02%	0.003%
67	10.924	3071	3074	3076	rBV2	340	222	0.02%	0.002%
68	10.956	3081	3084	3088	rBV	384	364	0.03%	0.004%
69	11.030	3104	3107	3110	rBV	416	199	0.02%	0.002%
70	11.185	3141	3155	3181	rBV	535365	837781	67.04%	8.645%
71	11.313	3192	3195	3197	rBV2	480	265	0.02%	0.003%
72	11.365	3209	3211	3215	rVV3	335	218	0.02%	0.002%
73	11.561	3260	3272	3289	rBV	554293	866538	69.34%	8.942%
74	12.040	3416	3421	3425	rBV3	346	339	0.03%	0.003%
75	12.198	3460	3470	3472	rBV2	720	1069	0.09%	0.011%
76	12.307	3501	3504	3507	rVV2	342	207	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
 Data File : VV034514.D
 Acq On : 06 Mar 2024 17:00
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.358	3517	3520	3523	rBV2	380	217	0.02%	0.002%
78	12.561	3580	3583	3587	rBV2	387	224	0.02%	0.002%
79	12.593	3589	3593	3596	rBV2	437	309	0.02%	0.003%
80	12.796	3653	3656	3659	rVV2	279	256	0.02%	0.003%
81	13.069	3739	3741	3745	rBV2	283	236	0.02%	0.002%
82	13.210	3782	3785	3786	rBV	392	207	0.02%	0.002%
83	13.242	3791	3795	3797	rBV	282	209	0.02%	0.002%
84	13.271	3801	3804	3806	rBV2	312	214	0.02%	0.002%
85	13.358	3827	3831	3835	rVB2	673	598	0.05%	0.006%
86	13.384	3835	3839	3842	rBV3	638	563	0.05%	0.006%
87	13.461	3857	3863	3865	rBV3	675	804	0.06%	0.008%
88	13.551	3888	3891	3896	rBV2	356	351	0.03%	0.004%
89	13.612	3907	3910	3913	rBV3	417	285	0.02%	0.003%
90	13.654	3919	3923	3930	rBV3	332	452	0.04%	0.005%
91	13.696	3930	3936	3938	rBV3	557	570	0.05%	0.006%
92	13.866	3986	3989	3991	rBV2	410	325	0.03%	0.003%
93	13.969	4019	4021	4024	rBV2	379	268	0.02%	0.003%
94	14.185	4086	4088	4093	rVB3	556	299	0.02%	0.003%
95	14.304	4121	4125	4129	rBV3	462	404	0.03%	0.004%
96	14.336	4131	4135	4138	rBV2	547	415	0.03%	0.004%
97	14.406	4152	4157	4160	rBV3	490	554	0.04%	0.006%
98	14.464	4173	4175	4178	rBV	347	201	0.02%	0.002%
99	14.538	4196	4198	4202	rVB2	469	241	0.02%	0.002%
100	14.866	4297	4300	4301	rBV3	494	297	0.02%	0.003%




Sum of corrected areas: 9690461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

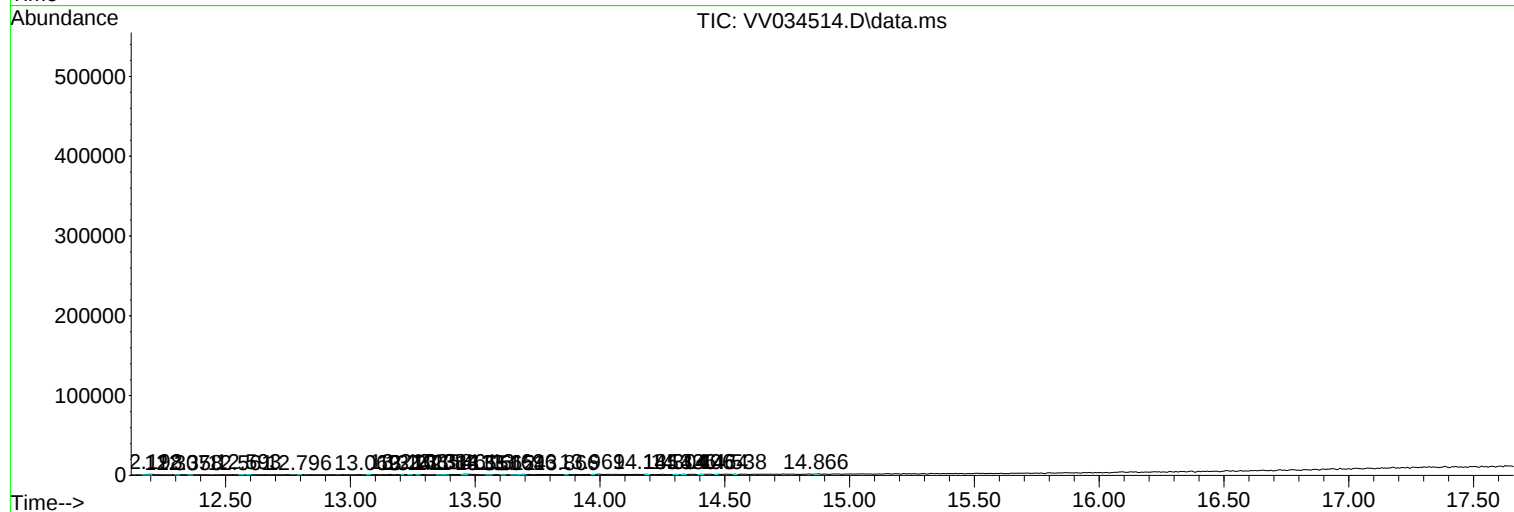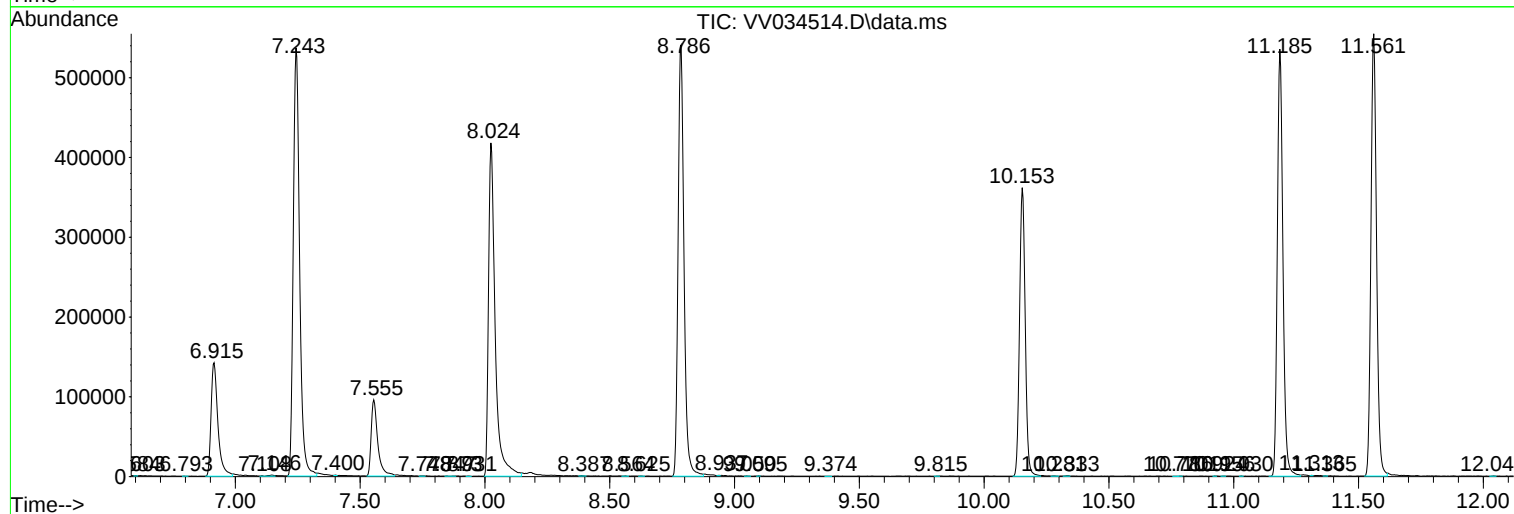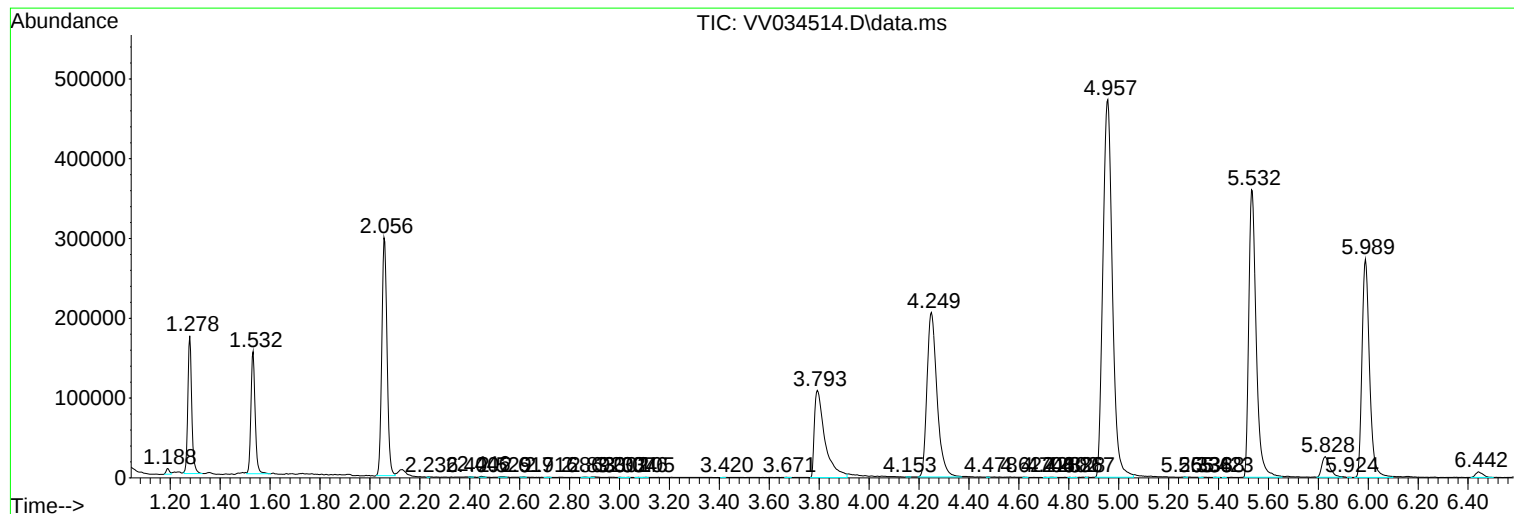

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034514.D
Acq On : 06 Mar 2024 17:00
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------