


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030724\
Data File : VV034509.D
Acq On : 06 Mar 2024 14:51
Operator : SY/MD
Sample : BFB264
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB264

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Thu Mar 07 04:30:42 2024

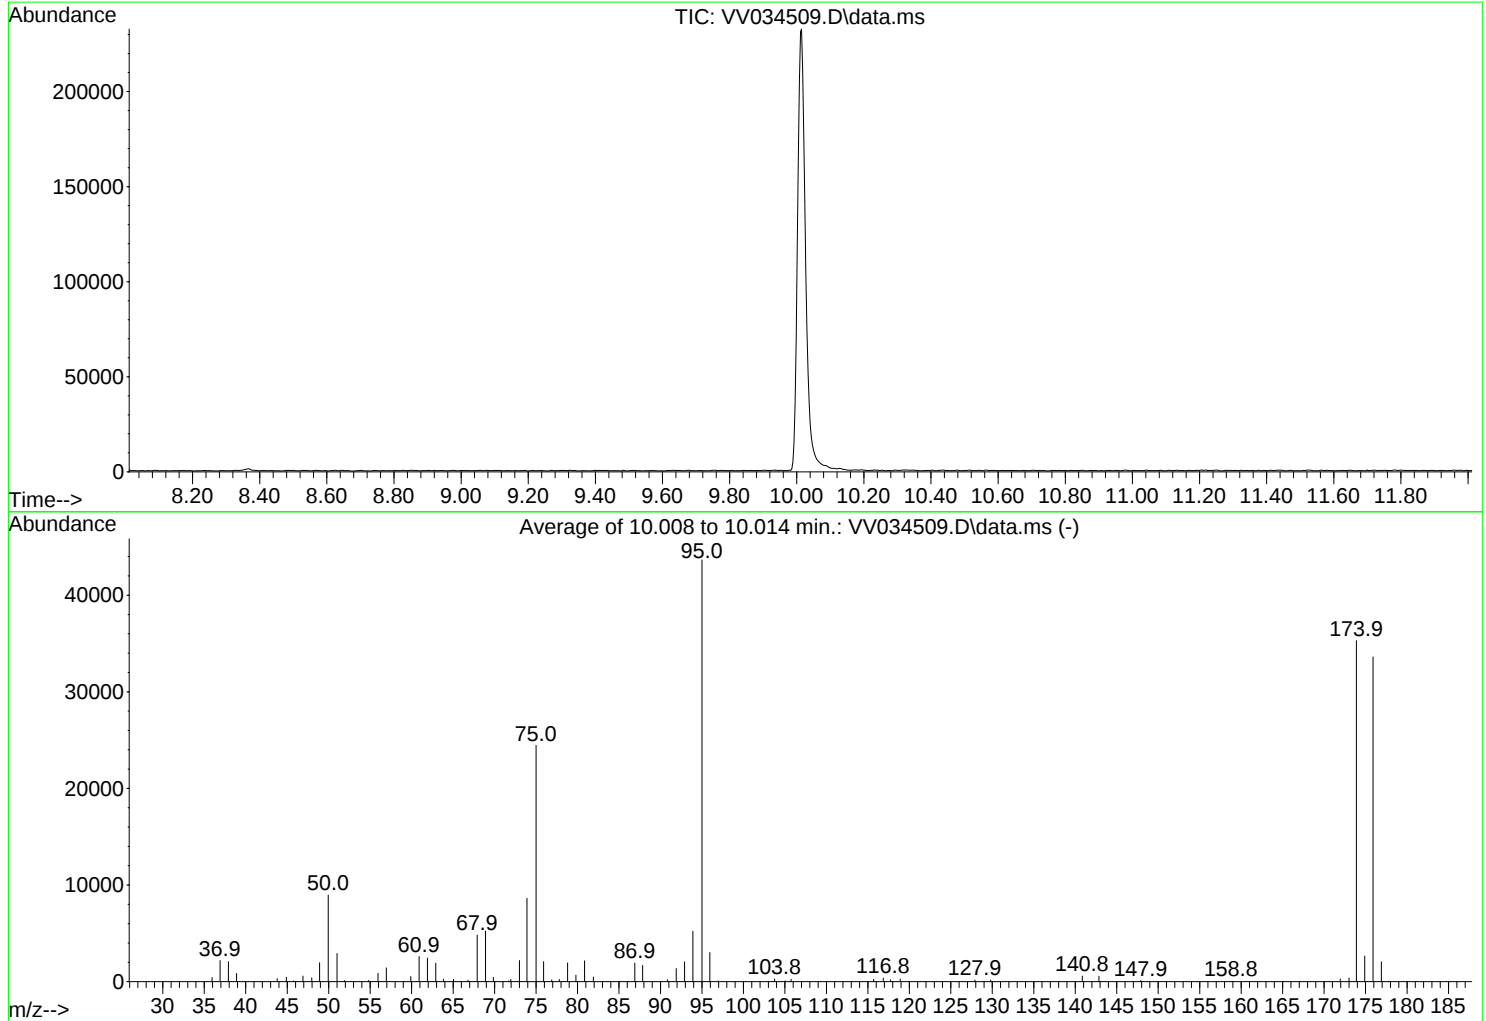

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	8966	PASS
75	95	30	80	56.0	24461	PASS
95	95	100	100	100.0	43661	PASS
96	95	5	9	6.9	3016	PASS
173	174	0.00	2	1.1	378	PASS
174	95	50	120	80.8	35299	PASS
175	174	5	9	7.5	2651	PASS
176	174	95	105	95.2	33613	PASS
177	176	5	10	6.1	2050	PASS

m/z	Abundance
39.80	342.0
43.80	434.0
76.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
36.00	408.0
36.90	1964.0
37.90	1940.0
38.90	816.0
39.90	358.0
43.80	804.0
44.90	402.0
46.90	514.0
47.90	353.0
48.90	1785.0
49.90	8339.0
51.00	2778.0
51.90	102.0
54.80	111.0
55.90	741.0
57.00	1313.0
59.90	451.0
60.90	2466.0
61.90	2362.0
62.90	1723.0
63.80	213.0
65.00	235.0
66.80	115.0
67.90	4537.0
68.90	4862.0
69.80	470.0
71.70	234.0
72.00	222.0
73.00	2039.0
73.90	8084.0
75.00	22896.0
75.90	2061.0
77.00	283.0
77.80	179.0
78.80	1932.0
79.80	562.0
80.80	2104.0
81.90	389.0
86.90	1812.0
87.90	1659.0
90.90	172.0
91.90	1371.0
92.90	1961.0
93.90	4734.0
95.00	40464.0
96.00	2918.0
103.80	259.0
105.10	110.0
105.80	244.0
115.70	223.0
116.90	344.0
117.70	154.0
118.90	258.0
127.90	134.0
128.80	112.0
129.80	155.0
140.90	455.0
142.80	554.0
158.80	105.0
171.90	290.0
173.90	31992.0
174.90	2527.0
175.90	30184.0
176.90	1936.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	447.0
36.90	2289.0
37.90	2155.0
38.90	838.0
39.90	369.0
43.80	774.0
44.90	483.0
45.80	132.0
46.90	624.0
47.90	432.0
48.90	2018.0
49.90	9254.0
51.00	2974.0
51.90	116.0
54.80	121.0
55.90	905.0
56.90	1474.0
59.90	575.0
60.90	2744.0
61.90	2482.0
62.90	2010.0
63.90	249.0
65.10	266.0
66.80	172.0
67.90	4928.0
68.90	5444.0
69.90	457.0
71.90	255.0
73.00	2283.0
73.90	8947.0
75.00	25440.0
75.90	2157.0
77.00	318.0
77.80	252.0
78.80	1982.0
79.80	711.0
80.90	2237.0
81.90	487.0
86.90	1983.0
87.90	1739.0
90.80	202.0
91.90	1369.0
92.90	2124.0
93.90	5324.0
95.00	45272.0
96.00	3134.0
97.00	123.0
103.80	282.0
105.00	119.0
105.70	256.0
115.70	275.0
116.90	391.0
117.70	209.0
118.90	288.0
127.90	184.0
129.80	170.0
140.80	598.0
142.90	579.0
147.90	160.0
172.00	287.0
173.00	577.0
173.90	36440.0
174.90	2679.0
175.90	34824.0
176.90	2112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	438.0
36.90	2303.0
37.90	2119.0
38.90	861.0
40.00	375.0
43.80	685.0
44.90	506.0
45.80	141.0
46.90	606.0
48.00	401.0
48.90	2047.0
50.00	9306.0
51.00	2972.0
51.90	126.0
54.80	113.0
56.00	959.0
56.90	1494.0
59.90	572.0
60.90	2574.0
61.90	2472.0
62.90	2022.0
63.90	285.0
65.10	269.0
66.80	177.0
67.90	5014.0
68.90	5419.0
69.90	419.0
71.90	240.0
73.00	2263.0
73.90	8835.0
75.00	25048.0
75.90	2003.0
76.90	281.0
77.80	254.0
78.80	1884.0
79.80	756.0
80.90	2100.0
81.90	564.0
86.90	1960.0
87.80	1642.0
90.80	231.0
91.90	1315.0
92.90	2100.0
93.90	5617.0
95.00	45248.0
95.90	2996.0
96.90	150.0
103.70	295.0
105.70	271.0
115.70	272.0
116.80	364.0
117.80	250.0
118.90	301.0
127.90	204.0
129.80	188.0
140.80	673.0
142.90	562.0
147.90	171.0
154.80	100.0
171.90	293.0
173.00	558.0
173.90	37464.0
174.90	2746.0
175.90	35832.0
176.90	2102.0
177.80	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264