

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030823\
 Data File : VV030144.D
 Acq On : 08 Mar 2023 11:53
 Operator : SY/MD
 Sample : VV0308WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK308

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	61	rBV2	4769	4659	1.18%	0.133%
2	1.281	69	75	86	rVB	50390	51887	13.15%	1.483%
3	1.535	147	154	166	rVB	57178	66114	16.75%	1.890%
4	2.063	307	318	335	rBV	101214	148687	37.67%	4.250%
5	2.455	430	440	454	rVB	11580	18780	4.76%	0.537%
6	3.838	857	870	923	rBV2	28082	146783	37.19%	4.195%
7	4.262	985	1002	1032	rBV	75879	197011	49.92%	5.631%
8	4.969	1205	1222	1244	rBV2	155383	394681	100.00%	11.280%
9	5.545	1387	1401	1426	rBV	143726	295675	74.91%	8.451%
10	5.998	1528	1542	1573	rBV	97834	205061	51.96%	5.861%
11	6.924	1819	1830	1847	rBV	38046	72051	18.26%	2.059%
12	7.252	1919	1932	1955	rBV	168648	302920	76.75%	8.658%
13	7.564	2017	2029	2048	rBV	23920	43119	10.93%	1.232%
14	8.037	2165	2176	2208	rBV	182498	376666	95.44%	10.765%
15	8.792	2399	2411	2438	rBV	215595	367407	93.09%	10.501%
16	10.162	2827	2837	2853	rBV	84092	132328	33.53%	3.782%
17	11.194	3143	3158	3185	rBV	227877	354821	89.90%	10.141%
18	11.570	3263	3275	3294	rBV	194477	308769	78.23%	8.825%
19	12.207	3458	3473	3485	rBV2	4315	7115	1.80%	0.203%
20	13.995	4014	4029	4039	rBV2	2251	4364	1.11%	0.125%




Sum of corrected areas: 3498898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030823\
Data File : VV030144.D
Acq On : 08 Mar 2023 11:53
Operator : SY/MD
Sample : VV0308WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

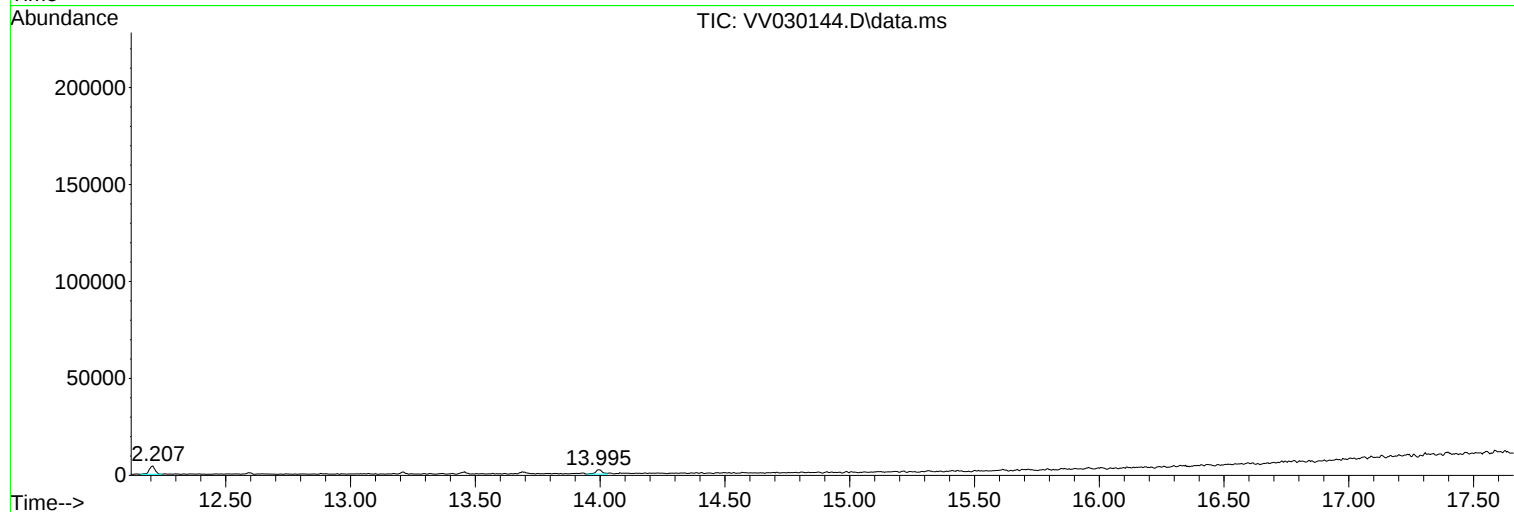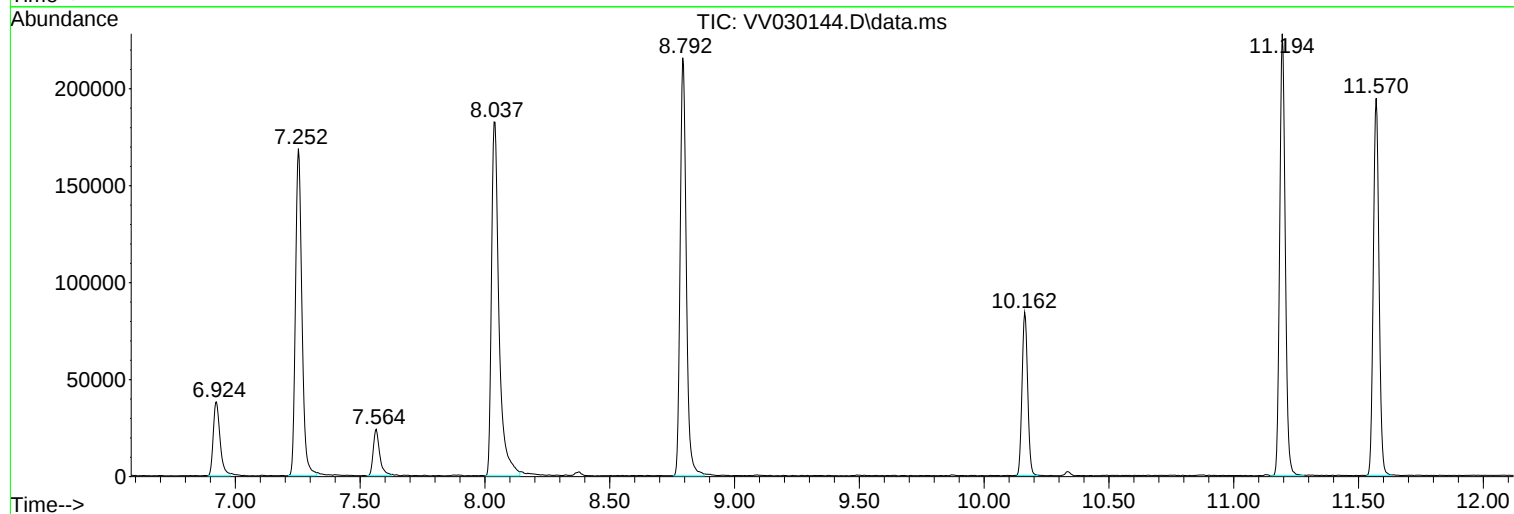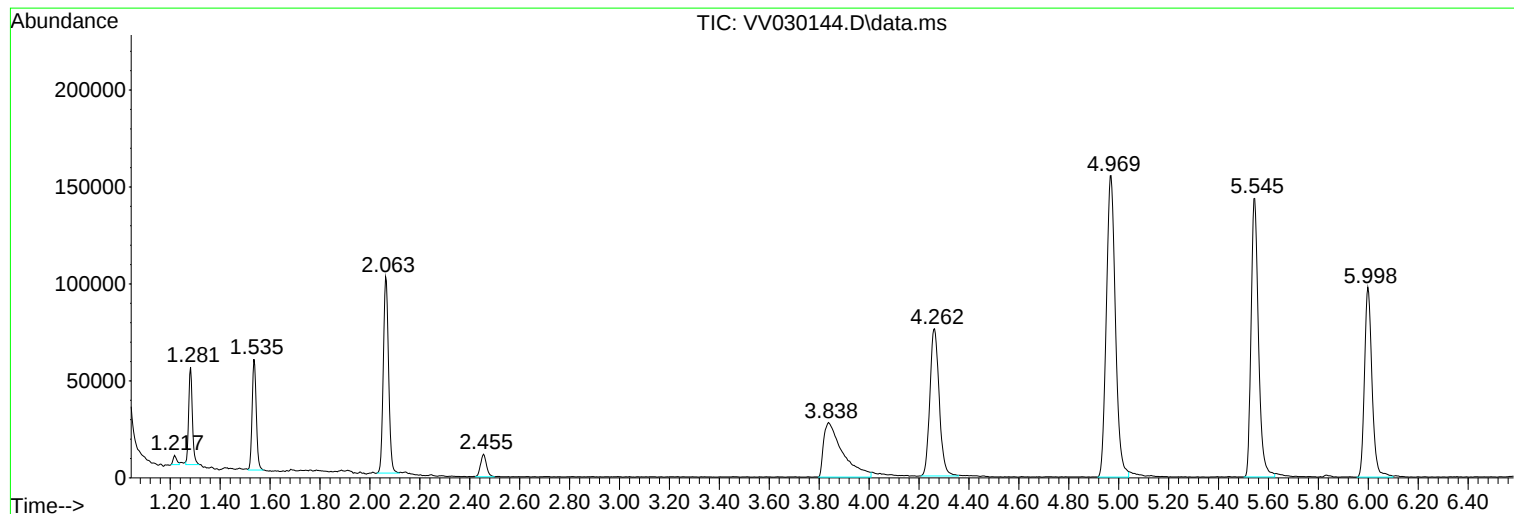

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030823\
Data File : VV030144.D
Acq On : 08 Mar 2023 11:53
Operator : SY/MD
Sample : VV0308WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030823\
Data File : VV030144.D
Acq On : 08 Mar 2023 11:53
Operator : SY/MD
Sample : VV0308WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc