


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030823\
Data File : VV030142.D
Acq On : 08 Mar 2023 09:13
Operator : SY/MD
Sample : BFB228
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB228

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 03 22:25:34 2023

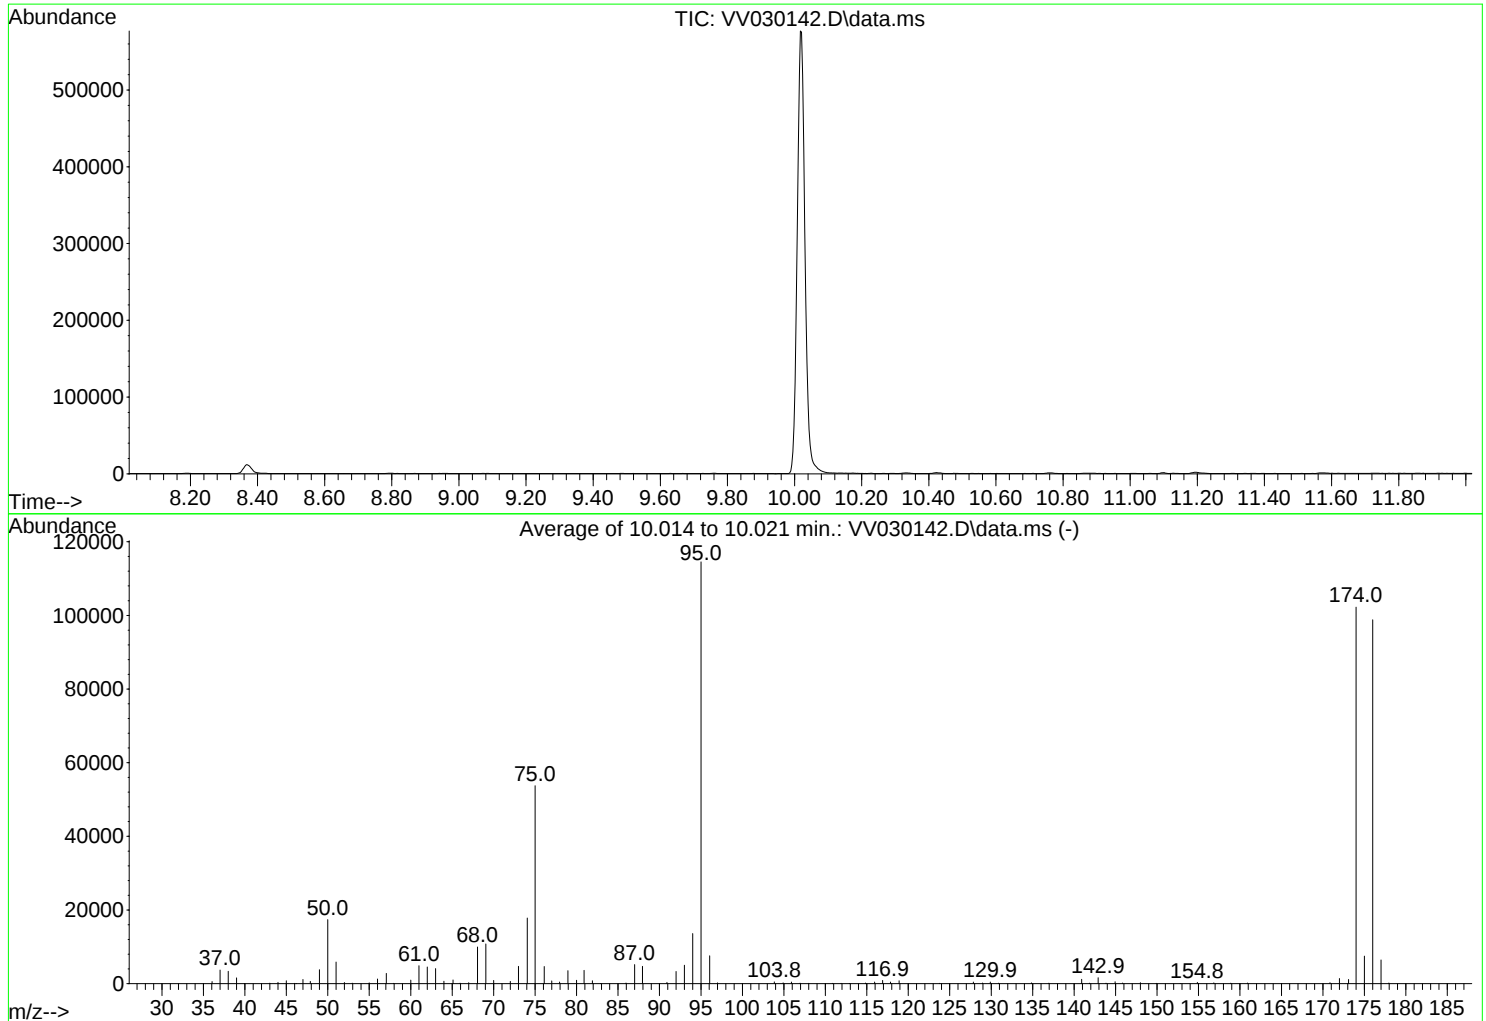

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	17400	PASS
75	95	30	80	46.9	53736	PASS
95	95	100	100	100.0	114547	PASS
96	95	5	9	6.6	7559	PASS
173	174	0.00	2	1.1	1129	PASS
174	95	50	120	89.3	102243	PASS
175	174	5	9	7.3	7497	PASS
176	174	95	105	96.6	98789	PASS
177	176	5	10	6.5	6440	PASS

m/z	Abundance
39.90	202.0
44.00	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.10	533.0
37.00	3726.0
38.00	3095.0
39.00	1516.0
40.00	252.0
43.00	105.0
44.00	584.0
45.00	790.0
46.00	145.0
47.00	1035.0
47.90	591.0
49.00	3537.0
50.00	16440.0
51.00	5676.0
52.00	258.0
53.00	122.0
55.00	205.0
56.00	1228.0
57.00	2642.0
57.90	112.0
60.00	968.0
61.00	4403.0
62.00	4296.0
63.00	3806.0
64.00	609.0
65.10	969.0
66.00	117.0
67.00	245.0
68.00	9723.0
69.00	10214.0
70.00	835.0
72.00	596.0
73.00	4459.0
74.00	16880.0
75.00	51048.0
76.10	4505.0
77.00	683.0
78.00	415.0
79.00	3429.0
80.00	832.0
80.90	3521.0
81.90	732.0
85.90	176.0
87.00	4810.0
87.90	4594.0
90.90	305.0
92.00	3102.0
93.00	4700.0
94.00	12877.0
95.00	107712.0
96.00	7292.0
97.00	262.0
103.90	428.0
104.90	202.0
105.90	368.0
106.90	126.0
108.00	116.0
110.90	134.0
114.80	133.0
116.00	384.0
116.90	867.0
117.80	368.0
118.90	737.0
127.80	383.0
129.00	160.0
129.90	398.0
130.90	118.0
134.90	192.0
136.90	148.0
140.90	1075.0
141.80	152.0
142.90	1546.0
143.80	117.0
145.00	526.0
145.80	143.0
148.00	283.0
152.80	100.0
154.80	345.0
156.80	230.0
158.90	120.0
160.90	168.0
170.90	269.0
172.00	1238.0
173.10	1084.0
174.00	93552.0
175.00	7008.0
176.00	89840.0
177.00	6057.0
178.00	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	541.0
37.00	3766.0
38.00	3457.0
39.00	1594.0
40.00	238.0
43.00	133.0
44.00	626.0
45.00	826.0
46.00	105.0
46.20	107.0
47.00	1160.0
47.90	632.0
49.00	3990.0
50.00	18016.0
51.00	6116.0
52.00	295.0
52.90	153.0
55.00	227.0
56.00	1308.0
57.00	2916.0
57.90	108.0
60.00	1023.0
61.00	5063.0
62.00	4719.0
63.00	4305.0
64.00	663.0
65.10	1057.0
65.90	117.0
67.00	271.0
68.10	10216.0
69.10	11153.0
70.00	917.0
72.00	638.0
73.00	4868.0
74.00	18320.0
75.00	55680.0
76.10	4795.0
77.00	744.0
78.00	437.0
79.00	3653.0
80.00	934.0
80.90	3675.0
81.90	806.0
86.00	169.0
87.00	5379.0
87.90	4831.0
90.90	350.0
92.00	3444.0
93.00	5156.0
94.00	14059.0
95.00	118464.0
96.00	7793.0
97.00	248.0
103.90	469.0
104.90	216.0
105.90	435.0
107.00	136.0
108.00	114.0
110.80	123.0
111.90	128.0
114.90	177.0
116.00	422.0
116.90	899.0
117.80	449.0
118.90	814.0
123.80	104.0
127.90	446.0
129.00	175.0
129.90	460.0
130.90	163.0
134.80	216.0
137.00	147.0
140.90	1223.0
141.90	144.0
142.90	1685.0
143.80	138.0
145.00	525.0
145.80	161.0
148.00	299.0
149.90	119.0
152.80	102.0
154.80	335.0
156.90	222.0
158.90	150.0
160.90	183.0
170.80	287.0
172.00	1451.0
173.10	1126.0
174.00	105752.0
175.00	7700.0
176.00	102120.0
177.00	6595.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

178.00

161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	569.0
37.00	3538.0
38.00	3450.0
39.00	1536.0
40.00	213.0
43.00	128.0
44.00	653.0
45.00	797.0
47.00	1227.0
47.90	649.0
49.00	3883.0
50.00	17744.0
51.00	5763.0
52.00	299.0
52.90	164.0
55.00	284.0
56.00	1298.0
57.10	2808.0
58.00	104.0
60.00	946.0
61.00	5180.0
62.00	4613.0
63.00	4210.0
64.00	646.0
65.10	974.0
66.00	116.0
67.00	279.0
68.00	9937.0
69.10	11014.0
70.00	865.0
72.00	614.0
73.00	4809.0
74.10	18200.0
75.00	54480.0
76.10	4613.0
77.00	733.0
77.90	419.0
78.90	3518.0
80.00	921.0
80.90	3608.0
81.90	807.0
82.90	108.0
86.00	157.0
87.00	5361.0
88.00	4711.0
90.90	369.0
92.00	3431.0
93.00	5115.0
94.00	13814.0
95.00	117464.0
96.10	7591.0
97.00	197.0
103.80	487.0
104.90	211.0
105.90	506.0
107.00	123.0
111.90	117.0
112.90	110.0
114.90	193.0
115.80	447.0
116.90	845.0
117.90	457.0
118.90	749.0
123.80	113.0
127.90	469.0
128.90	219.0
129.90	446.0
130.90	185.0
134.80	236.0
137.00	145.0
140.90	1211.0
141.90	142.0
142.90	1647.0
143.90	133.0
144.90	487.0
145.90	174.0
148.00	265.0
149.90	141.0
154.90	319.0
156.90	217.0
158.90	158.0
160.90	154.0
170.80	264.0
172.00	1471.0
173.10	1177.0
174.00	107424.0
175.00	7782.0
176.00	104408.0
177.00	6668.0
177.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228