

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034519.D
 Acq On : 08 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0308WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 08 23:18:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 08 23:17:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	315261	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	288443	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	138955	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	109781	40.169	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.340%		
7) Chloroethane-d5	1.526	69	96845	45.485	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.960%		
11) 1,1-Dichloroethene-d2	2.057	65	50139	40.566	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.140%		
21) 2-Butanone-d5	3.780	46	197576	108.104	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	108.100%		
24) Chloroform-d	4.246	84	221555	45.850	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.700%		
26) 1,2-Dichloroethane-d4	4.937	65	152807	48.391	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.780%		
32) Benzene-d6	4.957	84	415456	47.725	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.440%		
36) 1,2-Dichloropropane-d6	5.986	67	130742	49.212	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.420%		
41) Toluene-d8	7.243	98	363060	46.086	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.180%		
43) trans-1,3-Dichloroprop...	7.555	79	59612	44.683	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.360%		
47) 2-Hexanone-d5	8.021	63	136900	103.194	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	103.190%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	172777	49.419	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.840%		
66) 1,2-Dichlorobenzene-d4	11.558	152	140066	49.314	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.620%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.185	75	16804	6.335	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034519.D
Acq On : 08 Mar 2024 10:02
Operator : SY/MD
Sample : VV0308WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 08 23:18:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration

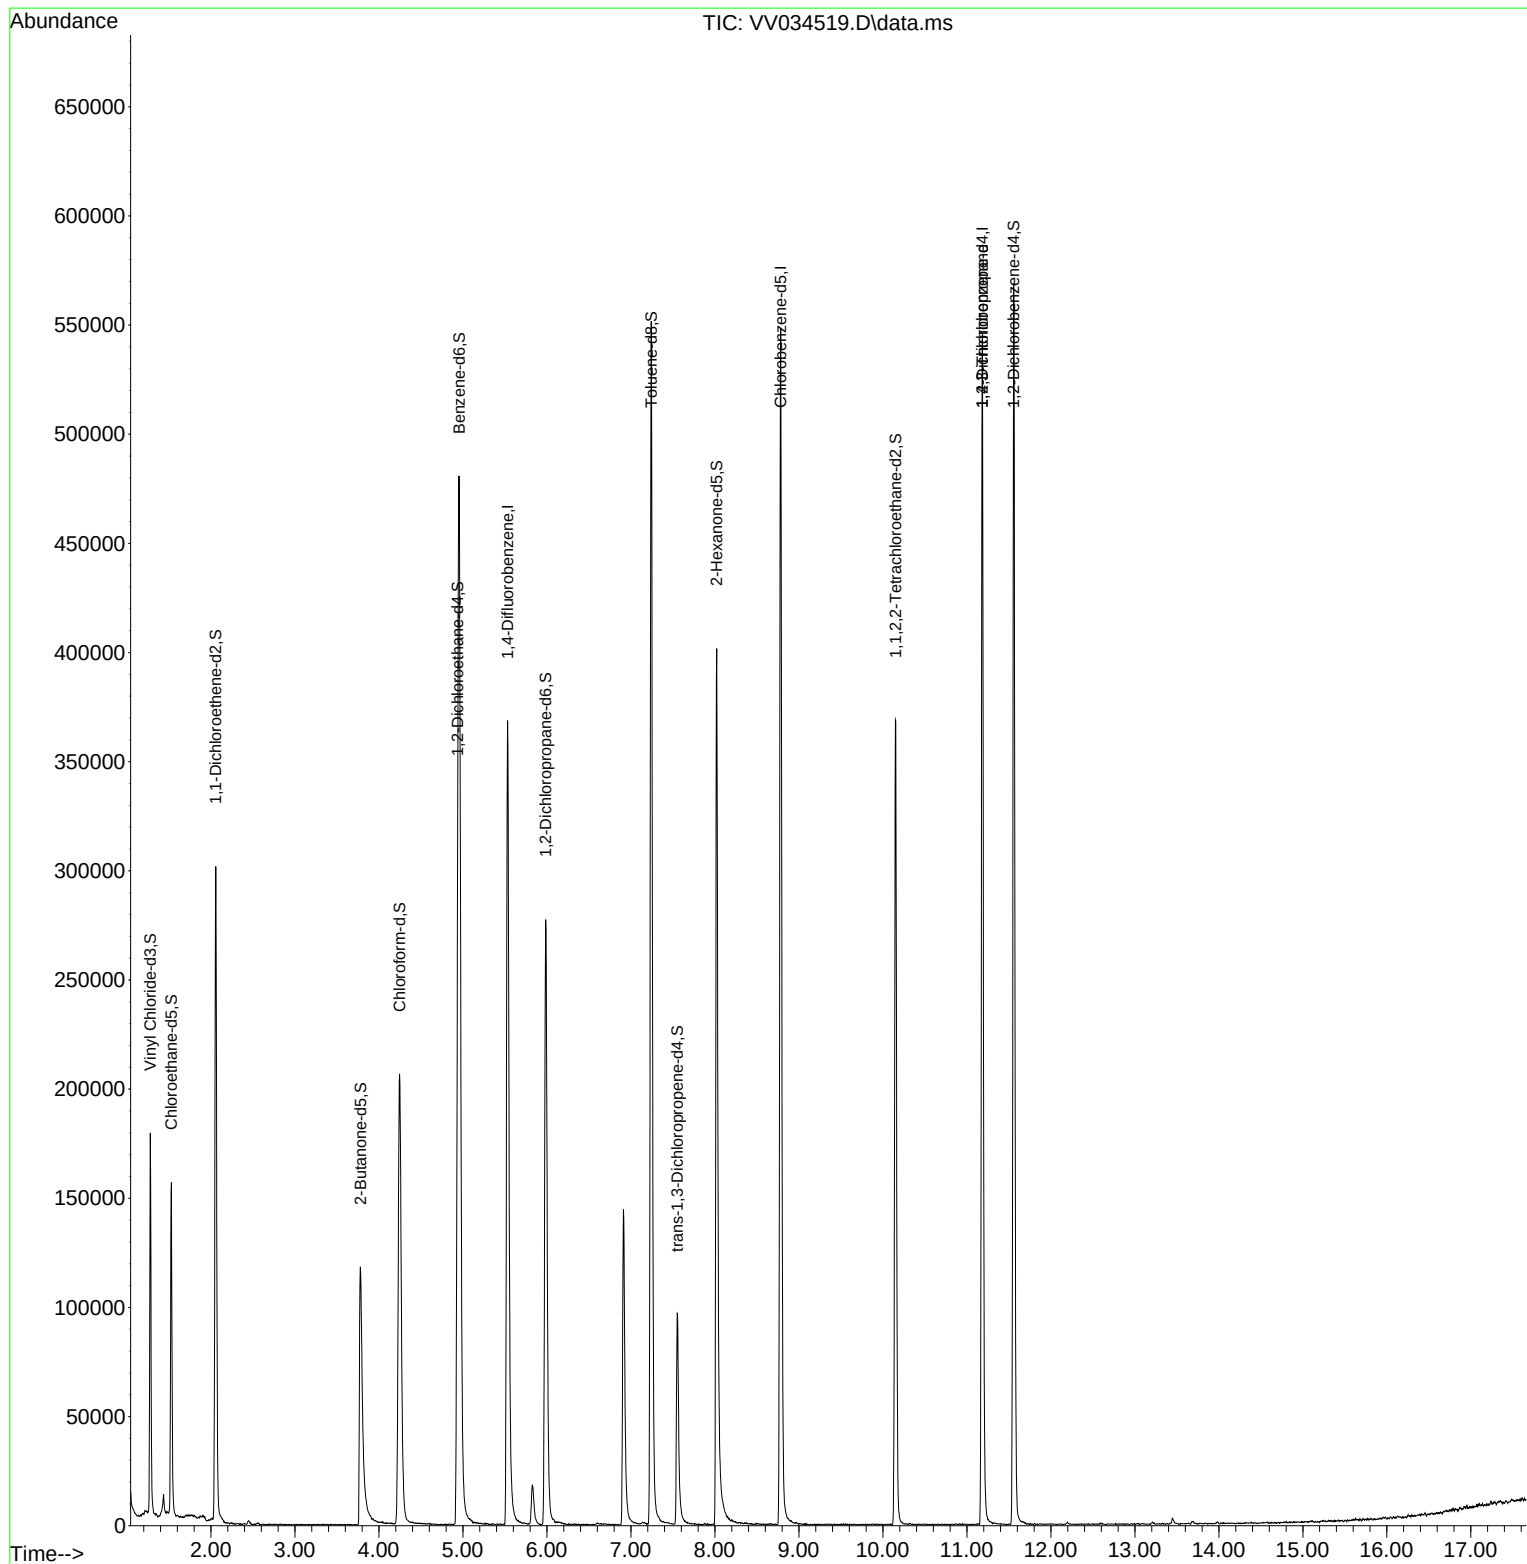

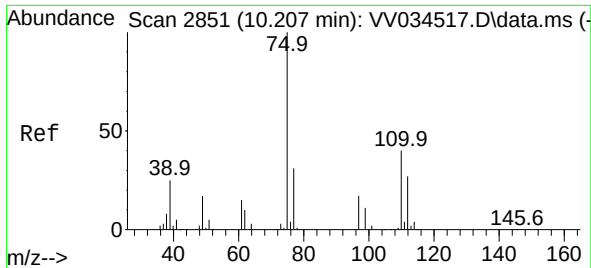

#61
 1,2,3-Trichloropropane
 Concen: 6.335 ug/L
 RT: 11.185 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV034519.D
 Acq: 08 Mar 2024 10:02

Instrument :
 MSVOA_V
 ClientSampleId :

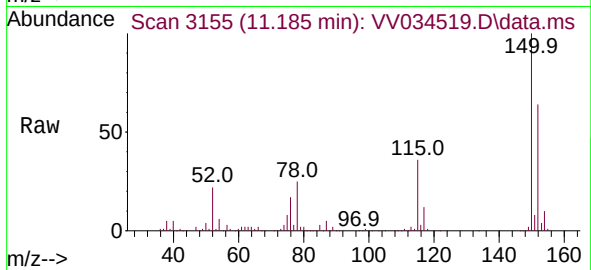

Tgt Ion: 75 Resp: 16804
 Ion Ratio Lower Upper
 75 100
 77 35.2 25.9 38.9
 110 2.6 33.1 49.7#

