

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034525.D
 Acq On : 08 Mar 2024 12:27
 Operator : SY/MD
 Sample : P1637-02 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 08 23:20:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 08 23:17:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	314428	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	290518	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	137775	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	103986	38.149	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.300%		
7) Chloroethane-d5	1.526	69	91699	43.182	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.360%		
11) 1,1-Dichloroethene-d2	2.057	65	49192	39.905	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.820%		
21) 2-Butanone-d5	3.780	46	187396	102.805	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.810%		
24) Chloroform-d	4.246	84	213742	44.350	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.700%		
26) 1,2-Dichloroethane-d4	4.937	65	144960	46.028	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.060%		
32) Benzene-d6	4.957	84	397554	45.342	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.680%		
36) 1,2-Dichloropropane-d6	5.986	67	127816	47.767	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.540%		
41) Toluene-d8	7.243	98	350645	44.192	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.380%		
43) trans-1,3-Dichloroprop...	7.551	79	55535	41.330	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.660%		
47) 2-Hexanone-d5	8.021	63	135416	101.346	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.350%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	171825	48.796	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.600%		
66) 1,2-Dichlorobenzene-d4	11.558	152	133244	47.314	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.620%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	3883	1.015	ug/L #	63
61) 1,2,3-Trichloropropane	11.182	75	17103	6.503	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034525.D
Acq On : 08 Mar 2024 12:27
Operator : SY/MD
Sample : P1637-02 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 08 23:20:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration

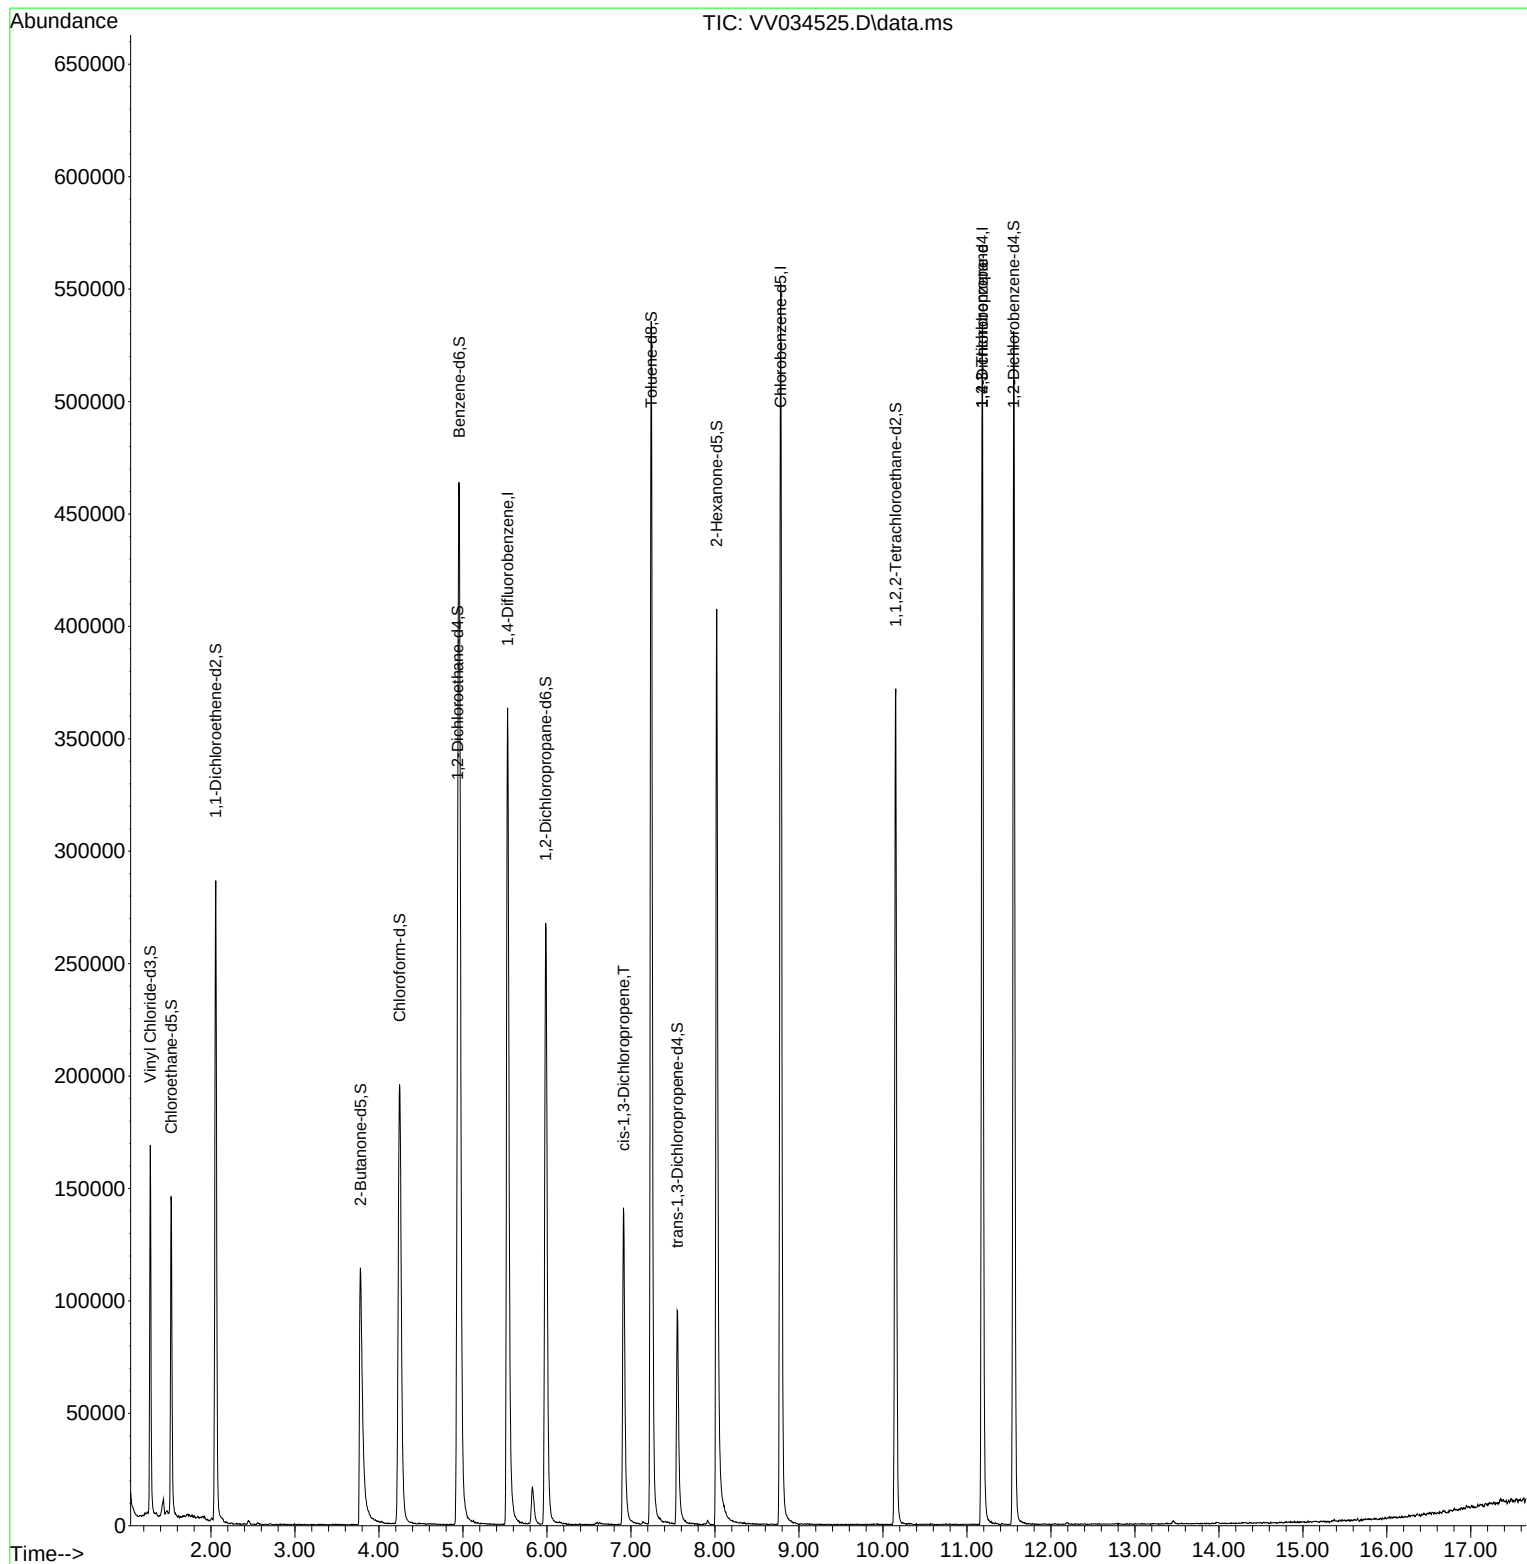

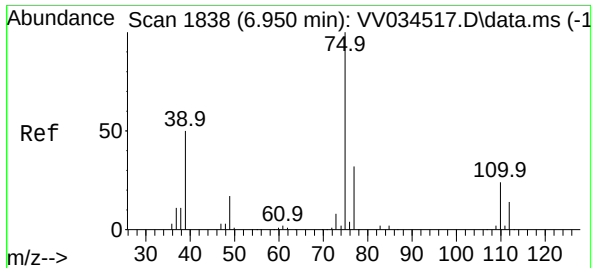

#39

cis-1,3-Dichloropropene

Concen: 1.015 ug/L

RT: 6.915 min Scan# 11

Delta R.T. -0.035 min

Lab File: VV034525.D

Acq: 08 Mar 2024 12:27

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 3883

Ion Ratio Lower Upper

75 100

77 49.8 20.9 38.9#

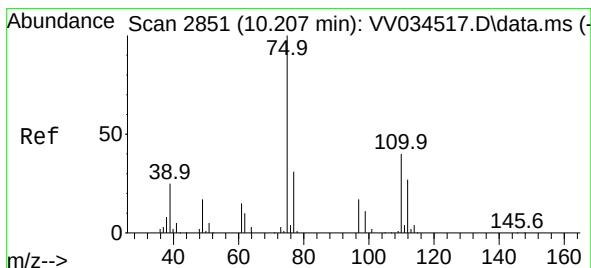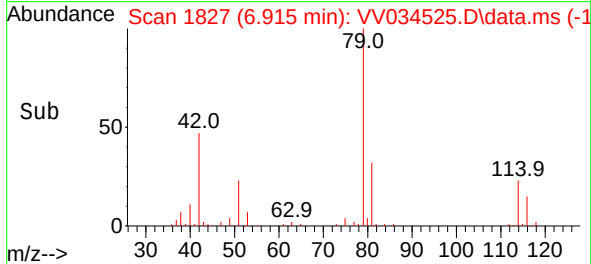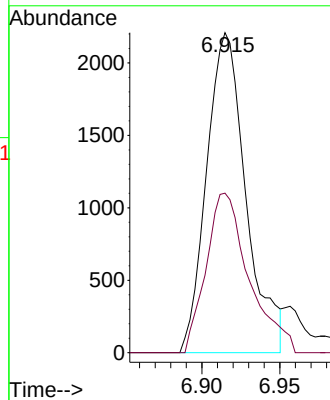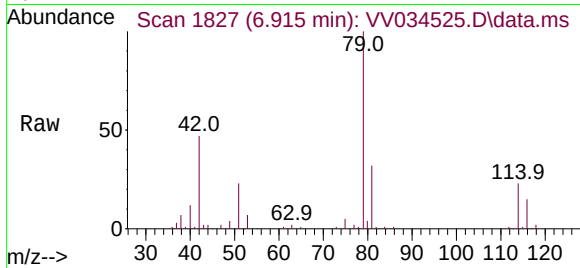

#61

1,2,3-Trichloropropane

Concen: 6.503 ug/L

RT: 11.182 min Scan# 3154

Delta R.T. 0.974 min

Lab File: VV034525.D

Acq: 08 Mar 2024 12:27

Tgt Ion: 75 Resp: 17103

Ion Ratio Lower Upper

75 100

77 34.8 25.9 38.9

110 2.9 33.1 49.7#

