

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034527.D
 Acq On : 08 Mar 2024 13:27
 Operator : SY/MD
 Sample : P1679-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 08 23:20:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 08 23:17:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	316871	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	285338	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	135785	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	101174	36.832	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	73.660%	
7) Chloroethane-d5	1.526	69	90473	42.276	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	84.560%	
11) 1,1-Dichloroethene-d2	2.056	65	47193	37.988	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.980%	
21) 2-Butanone-d5	3.780	46	189618	103.222	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.220%	
24) Chloroform-d	4.246	84	214010	44.063	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.120%	
26) 1,2-Dichloroethane-d4	4.937	65	146746	46.236	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.480%	
32) Benzene-d6	4.957	84	398710	46.299	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	5.986	67	128786	49.004	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.000%	
41) Toluene-d8	7.243	98	339066	43.509	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.020%	
43) trans-1,3-Dichloroprop...	7.551	79	55312	41.911	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	83.820%	
47) 2-Hexanone-d5	8.021	63	138475	105.517	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	105.520%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	170693	49.354	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.700%	
66) 1,2-Dichlorobenzene-d4	11.561	152	132467	47.727	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.460%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.185	75	16608	6.407	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034527.D
Acq On : 08 Mar 2024 13:27
Operator : SY/MD
Sample : P1679-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 08 23:20:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration

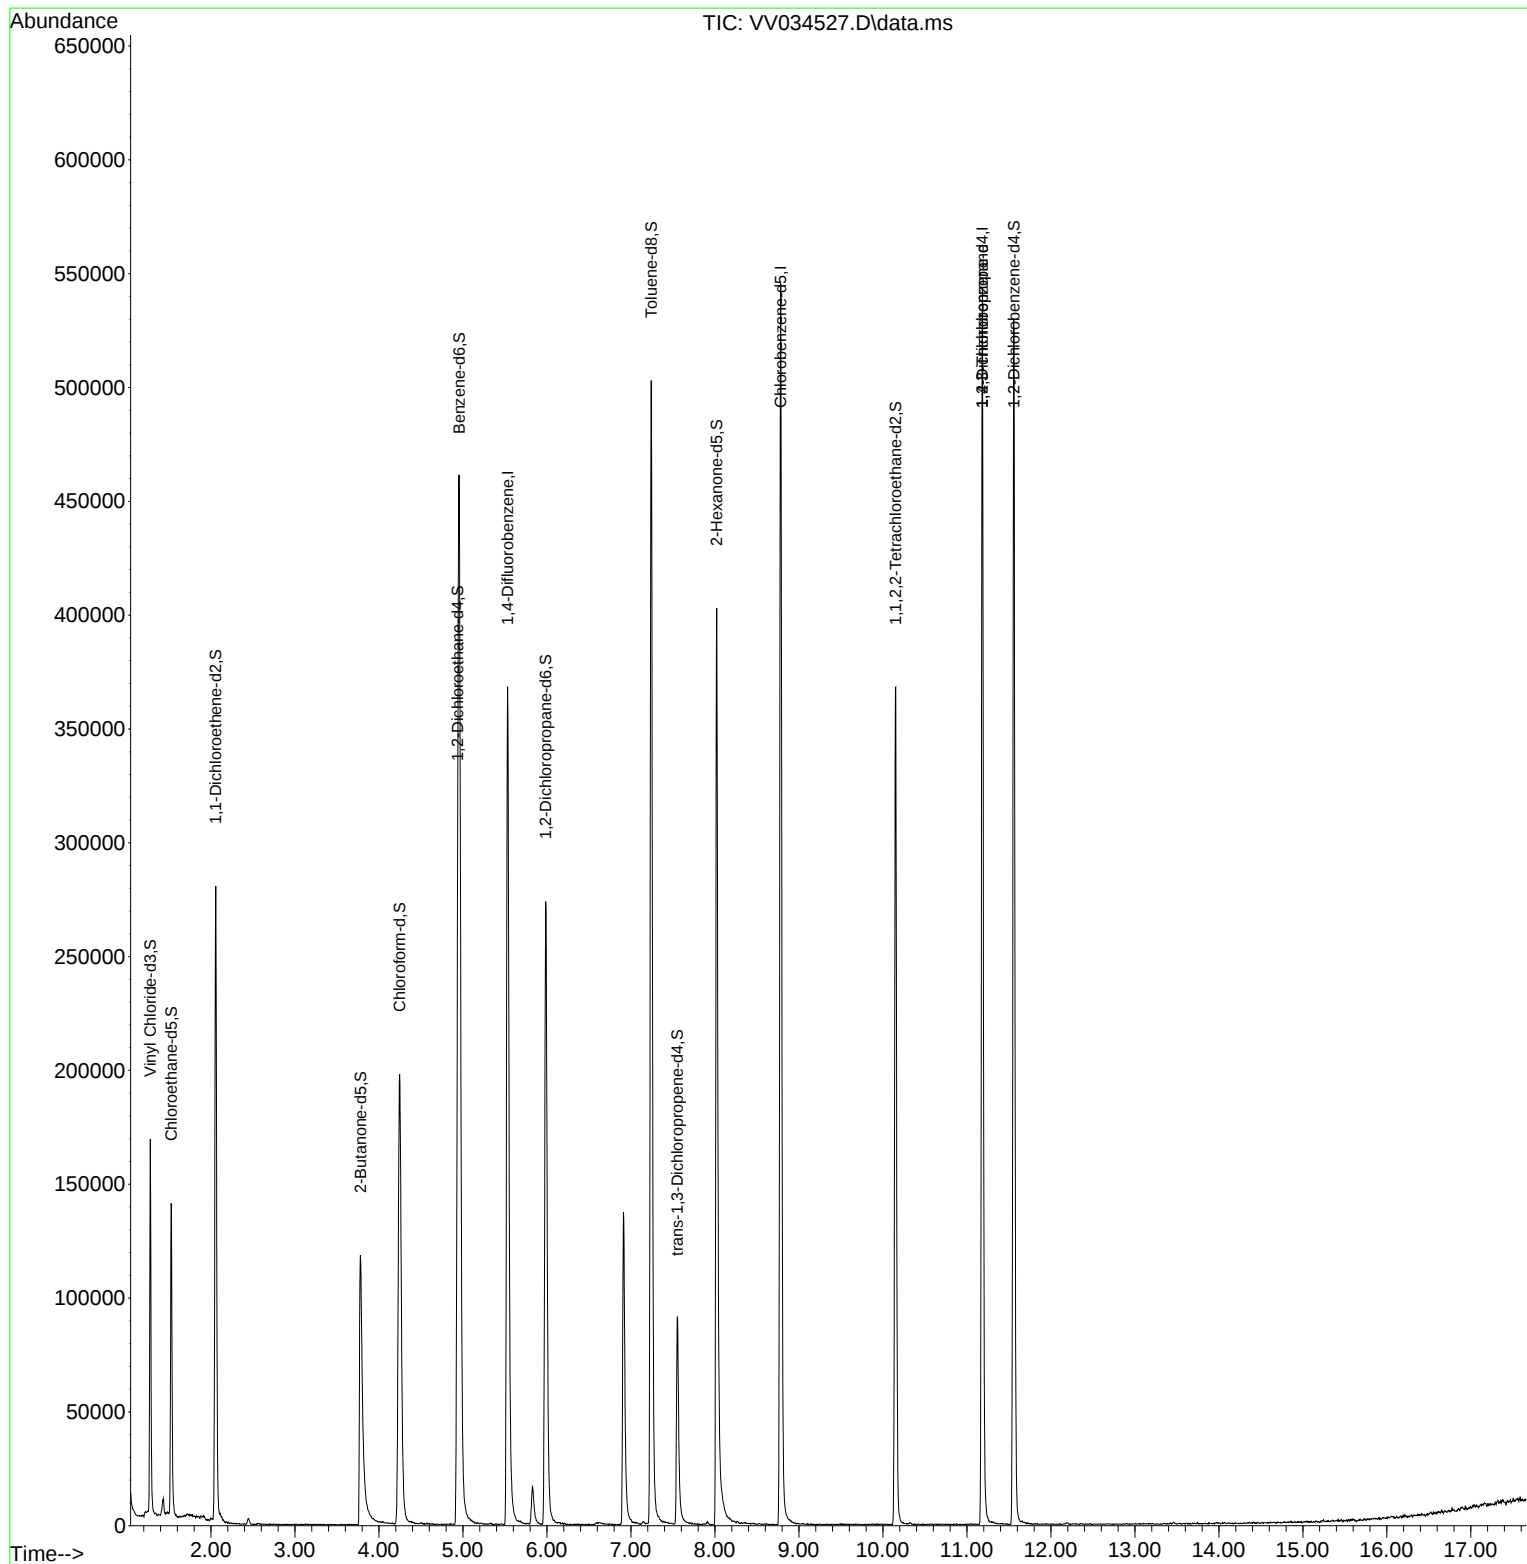

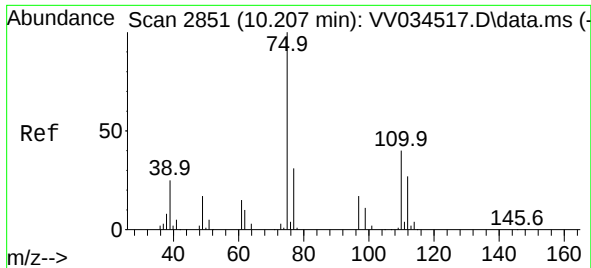

#61
 1,2,3-Trichloropropane
 Concen: 6.407 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.977 min
 Lab File: VV034527.D
 Acq: 08 Mar 2024 13:27

Instrument :
 MSVOA_V
 ClientSampleId :

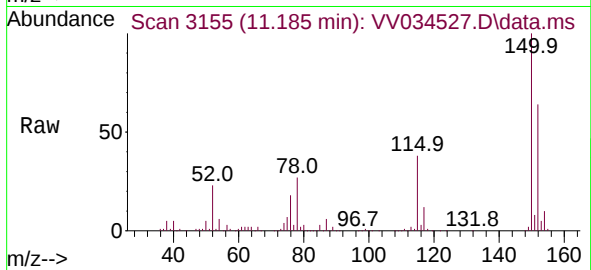

Tgt Ion: 75 Resp: 16608
 Ion Ratio Lower Upper
 75 100
 77 34.4 25.9 38.9
 110 3.1 33.1 49.7#

