

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034529.D
 Acq On : 08 Mar 2024 14:16
 Operator : SY/MD
 Sample : P1637-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 08 23:21:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 08 23:17:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	291620	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	276257	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	129572	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	95649	37.835	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.680%		
7) Chloroethane-d5	1.526	69	85528	43.426	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.860%		
11) 1,1-Dichloroethene-d2	2.056	65	45091	39.439	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.880%		
21) 2-Butanone-d5	3.780	46	187221	110.742	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	110.740%		
24) Chloroform-d	4.246	84	206525	46.204	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.400%		
26) 1,2-Dichloroethane-d4	4.941	65	142521	48.793	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.580%		
32) Benzene-d6	4.957	84	379792	45.552	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.100%		
36) 1,2-Dichloropropane-d6	5.986	67	124824	49.057	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.120%		
41) Toluene-d8	7.243	98	332171	44.025	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.040%		
43) trans-1,3-Dichloroprop...	7.551	79	54063	42.311	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.620%		
47) 2-Hexanone-d5	8.021	63	139510	109.800	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	109.800%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	170656	50.966	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.940%		
66) 1,2-Dichlorobenzene-d4	11.561	152	130685	49.343	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.680%		
Target Compounds			Qvalue			
61) 1,2,3-Trichloropropane	11.185	75	15750	6.368	ug/L #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034529.D
Acq On : 08 Mar 2024 14:16
Operator : SY/MD
Sample : P1637-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 08 23:21:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration

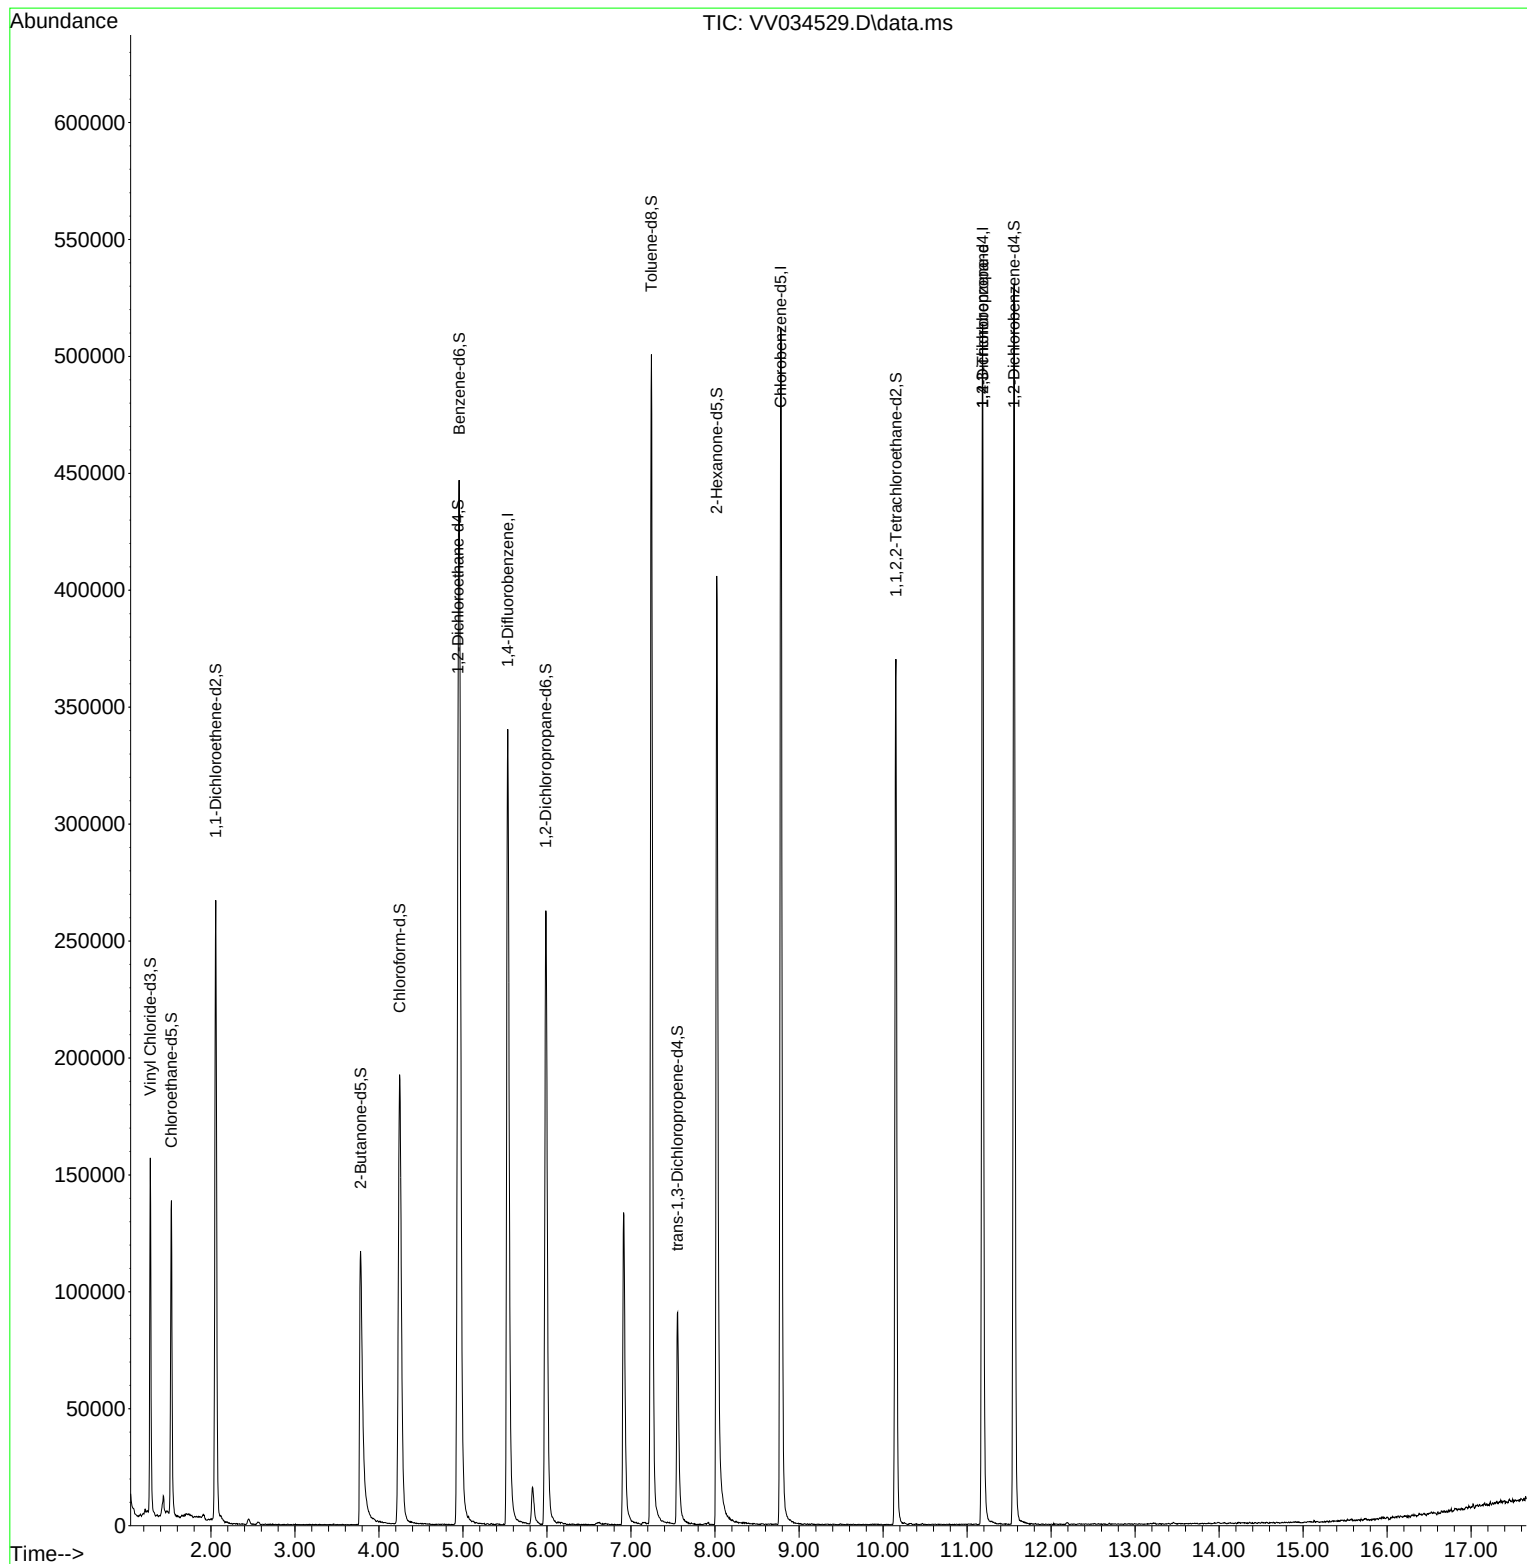

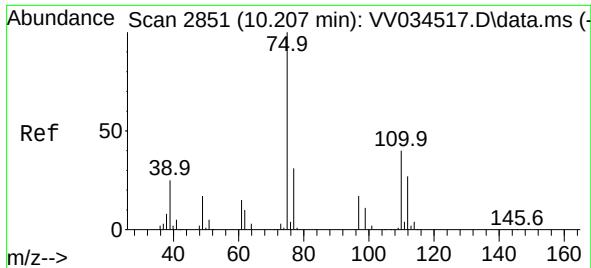

#61
 1,2,3-Trichloropropane
 Concen: 6.368 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.977 min
 Lab File: VV034529.D
 Acq: 08 Mar 2024 14:16

Instrument :
 MSVOA_V
 ClientSampleId :

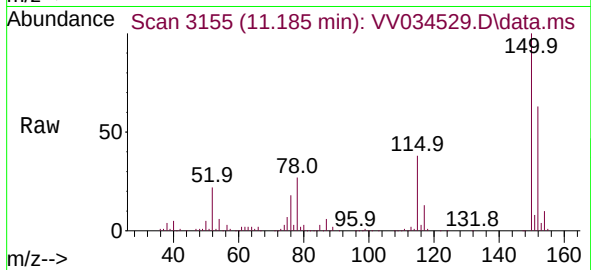

Tgt Ion:	75	Resp:	15750
Ion Ratio	Lower	Upper	
75	100		
77	36.5	25.9	38.9
110	1.2	33.1	49.7#

