

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030824\
 Data File : VW034521.D
 Acq On : 08 Mar 2024 10:50
 Operator : SY/MD
 Sample : P1637-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNO1

Quant Time: Mar 08 23:19:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 08 23:17:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	315312	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	294855	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	148506	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	107510	39.332	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.660%
7) Chloroethane-d5	1.529	69	93827	44.060	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.120%
11) 1,1-Dichloroethene-d2	2.056	65	49784	40.272	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.540%
21) 2-Butanone-d5	3.780	46	185890	101.693	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.690%
24) Chloroform-d	4.246	84	233056	48.222	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.440%
26) 1,2-Dichloroethane-d4	4.940	65	151411	47.942	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.880%
32) Benzene-d6	4.956	84	413112	46.423	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.840%
36) 1,2-Dichloropropane-d6	5.985	67	130565	48.077	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.160%
41) Toluene-d8	7.243	98	371095	46.082	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.160%
43) trans-1,3-Dichloroprop...	7.551	79	63179	46.327	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.660%
47) 2-Hexanone-d5	8.021	63	144837	106.802	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.800%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	174057	48.703	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.400%
66) 1,2-Dichlorobenzene-d4	11.557	152	144135	47.483	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.960%
Target Compounds						
					Qvalue	
6) Bromomethane	1.481	94	48714	25.737	ug/L	99
9) Trichlorofluoromethane	1.712	101	322862	68.342	ug/L	100
12) 1,1-Dichloroethene	2.069	96	106541	45.124	ug/L	95
13) Acetone	2.108	43	292120	132.934	ug/L	99
16) Methylene chloride	2.445	84	85328	34.071	ug/L	96
18) Methyl tert-butyl Ether	2.703	73	316598	38.578	ug/L	100
19) 1,1-Dichloroethane	3.108	63	394321	88.084	ug/L	100
25) Chloroform	4.275	83	381209	82.158	ug/L	99
27) 1,2-Dichloroethane	5.037	62	391845	103.942	ug/L	100
31) Carbon tetrachloride	4.735	117	117234	31.317	ug/L	100
33) Benzene	5.011	78	220639	24.108	ug/L	100
34) Trichloroethene	5.837	95	29920	11.501	ug/L	98
38) Bromodichloromethane	6.436	83	38632	11.462	ug/L	97
39) cis-1,3-Dichloropropene	6.953	75	144947	37.336	ug/L	97
40) 4-Methyl-2-pentanone	7.153	43	351765	99.558	ug/L	99
44) trans-1,3-Dichloropropene	7.577	75	375220	100.492	ug/L	100
45) 1,1,2-Trichloroethane	7.770	97	67969	29.399	ug/L	99
46) Tetrachloroethene	7.902	164	120181	62.116	ug/L	98
48) 2-Hexanone	8.072	43	278609	98.956	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034521.D
Acq On : 08 Mar 2024 10:50
Operator : SY/MD
Sample : P1637-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNO1

Quant Time: Mar 08 23:19:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Dibromochloromethane	8.175	129	253388	103.858	ug/L	98
50) 1,2-Dibromoethane	8.278	107	145318	59.233	ug/L	100
51) Chlorobenzene	8.815	112	108563	17.337	ug/L	99
52) Ethylbenzene	8.943	91	826292	76.132	ug/L	100
53) m,p-Xylene	9.072	106	323732	78.602	ug/L	99
54) o-Xylene	9.477	106	250978	62.231	ug/L	98
55) Styrene	9.493	104	425153	62.262	ug/L	100
61) 1,2,3-Trichloropropane	10.207	75	129263	45.599	ug/L	99
62) 1,3,5-Trimethylbenzene	10.474	105	125261	14.138	ug/L	100
63) 1,2,4-Trimethylbenzene	10.850	105	378939	43.245	ug/L	98
65) 1,4-Dichlorobenzene	11.207	146	473851	96.087	ug/L	98
67) 1,2-Dichlorobenzene	11.577	146	360350	74.053	ug/L	99
68) 1,2-Dibromo-3-chloropr...	12.365	75	48566	57.512	ug/L	99
70) 1,2,4-trichlorobenzene	13.197	180	116915	35.666	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034521.D
Acq On : 08 Mar 2024 10:50
Operator : SY/MD
Sample : P1637-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNO1

Quant Time: Mar 08 23:19:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 08 23:17:44 2024
Response via : Initial Calibration




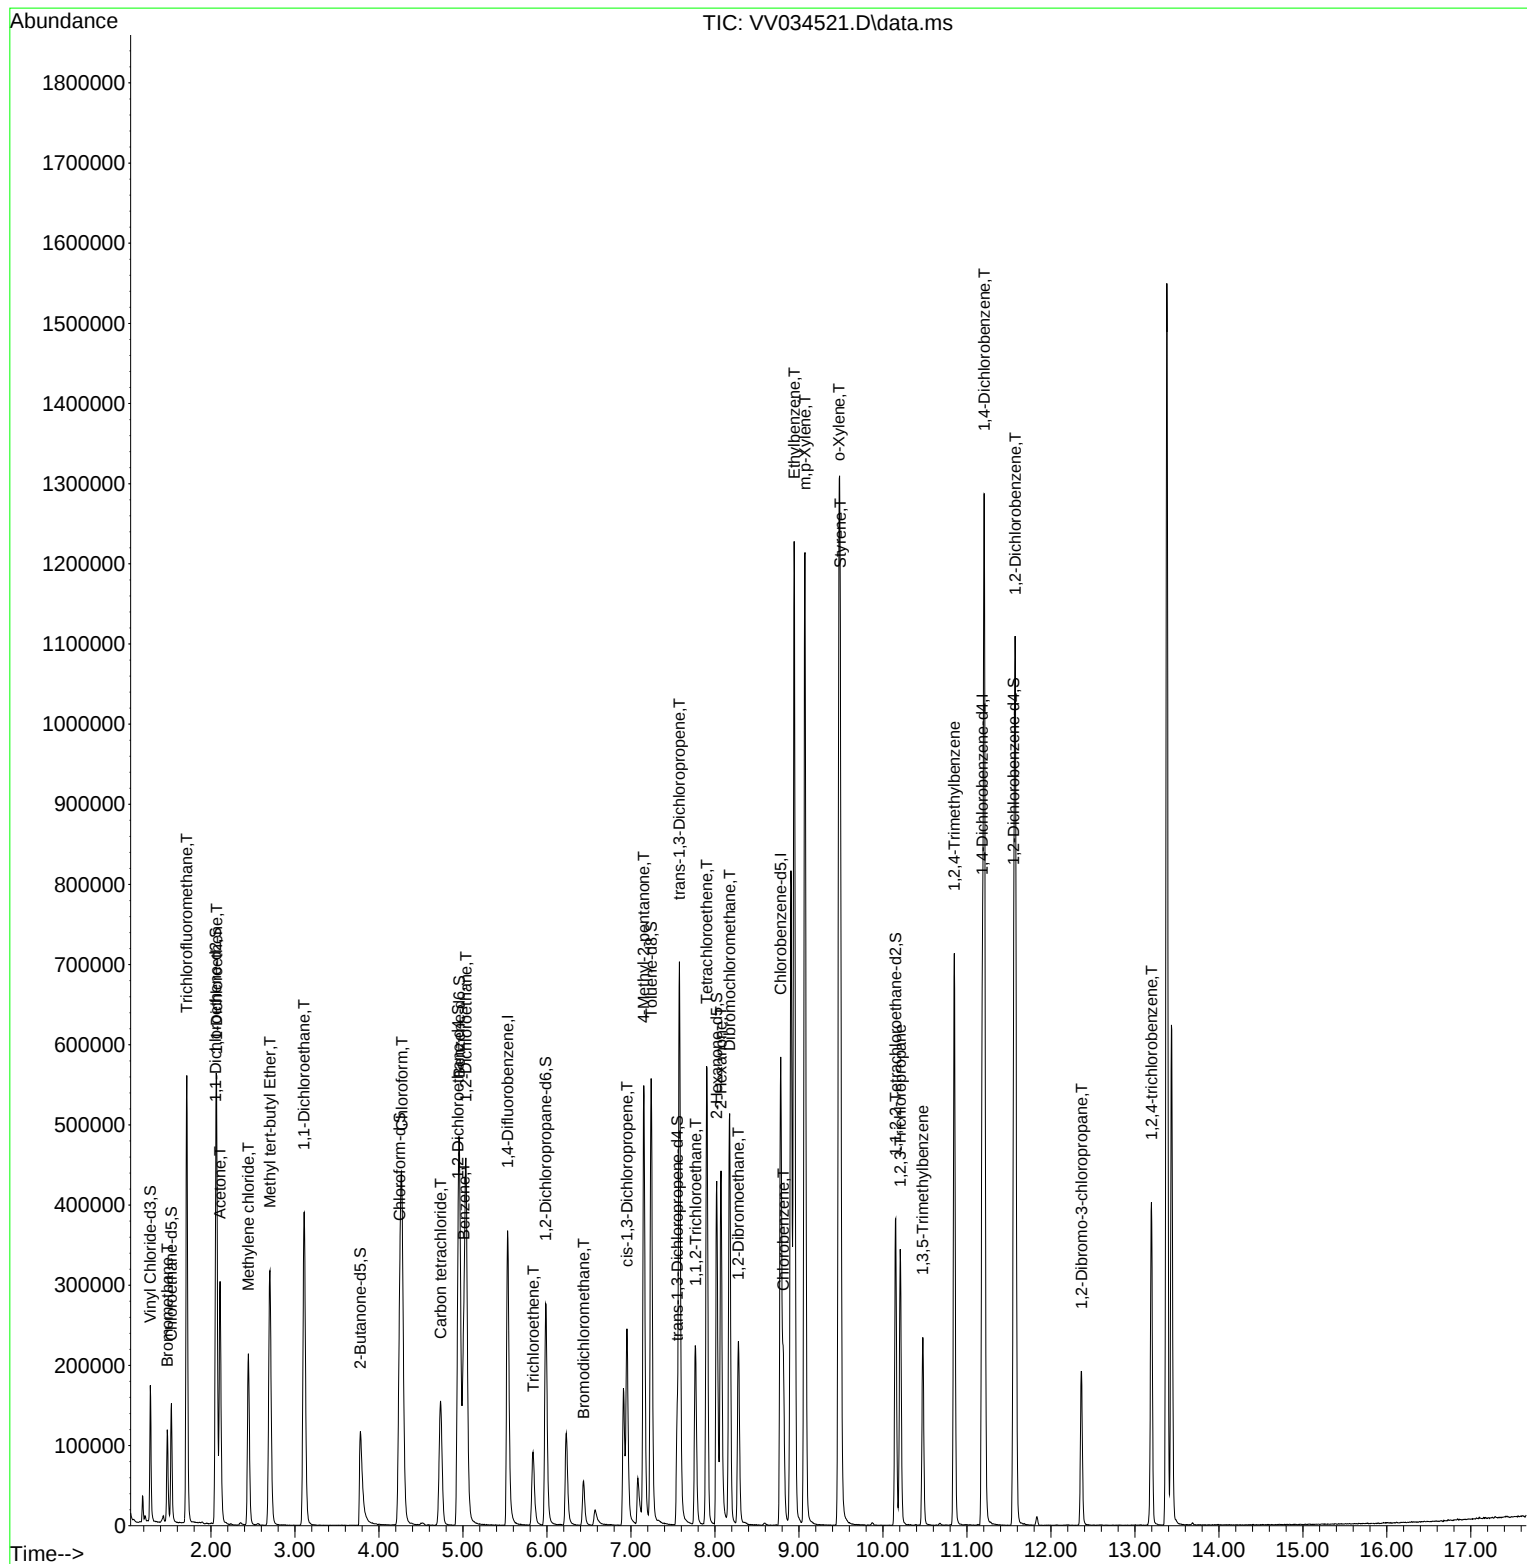


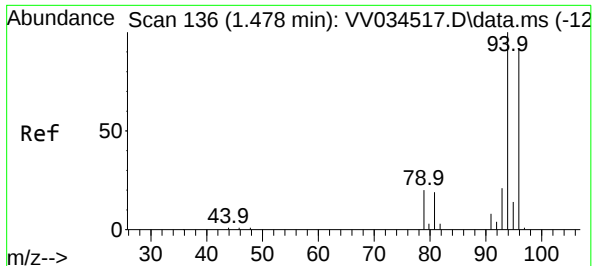

#6
Bromomethane
Concen: 25.737 ug/L
RT: 1.481 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 94 Resp: 48714
Ion Ratio Lower Upper
94 100
96 93.6 66.0 122.6

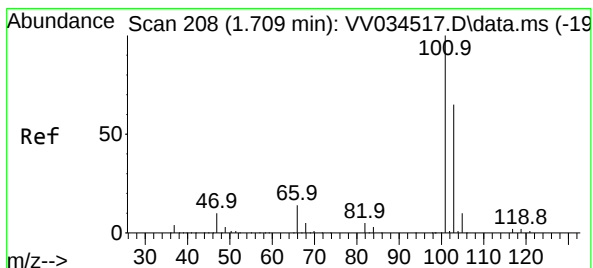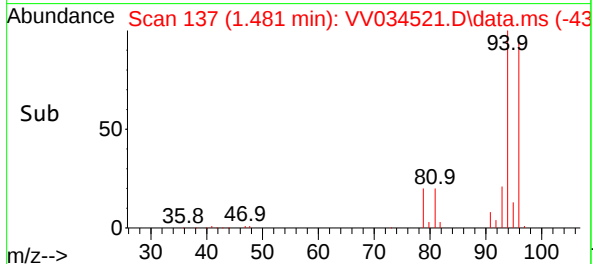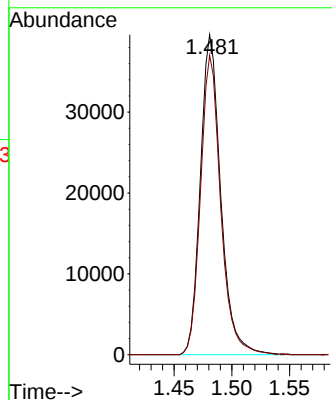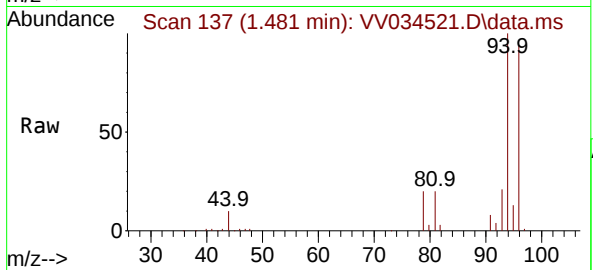

#9
Trichlorofluoromethane
Concen: 68.342 ug/L
RT: 1.712 min Scan# 209
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion:101 Resp: 322862
Ion Ratio Lower Upper
101 100
103 64.5 51.8 77.8


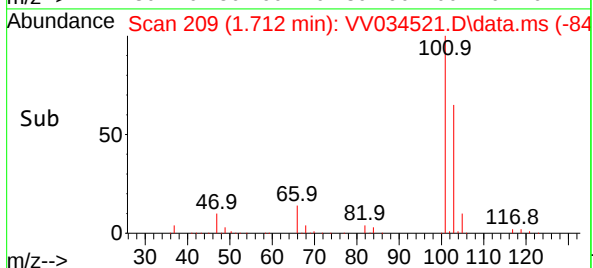
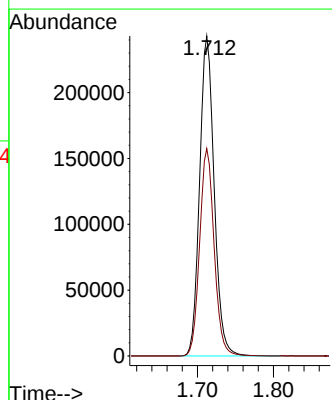
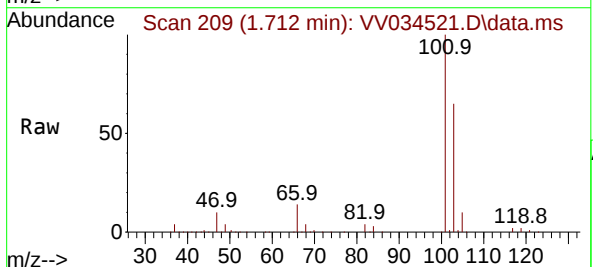




#12
1,1-Dichloroethene
Concen: 45.124 ug/L
RT: 2.069 min Scan# 319
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 96 Resp: 106541
Ion Ratio Lower Upper
96 100
61 182.3 128.9 239.3
63 127.8 98.0 182.0

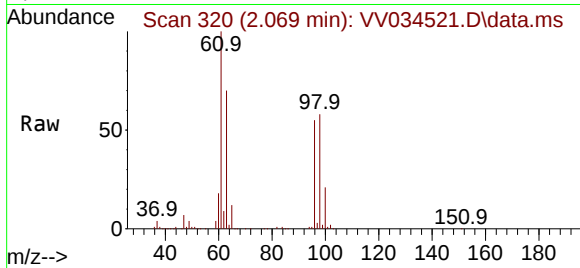

#13
Acetone
Concen: 132.934 ug/L
RT: 2.108 min Scan# 332
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 43 Resp: 292120
Ion Ratio Lower Upper
43 100
58 28.3 0.0 57.2



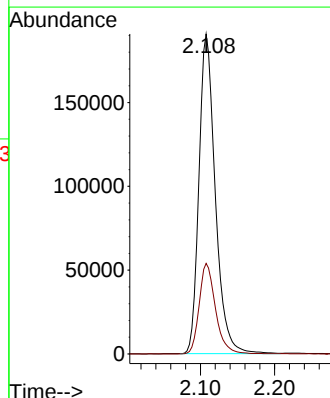
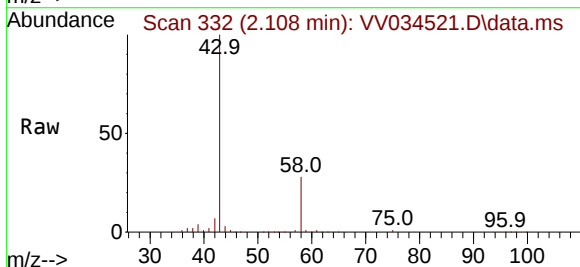




#16
Methylene chloride
Concen: 34.071 ug/L
RT: 2.445 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 84 Resp: 85328
Ion Ratio Lower Upper
84 100
86 62.9 45.6 84.6
49 126.8 92.3 171.3



#18
Methyl tert-butyl Ether
Concen: 38.578 ug/L
RT: 2.703 min Scan# 517
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 73 Resp: 316598
Ion Ratio Lower Upper
73 100
43 21.6 17.1 25.7
57 22.2 17.6 26.4


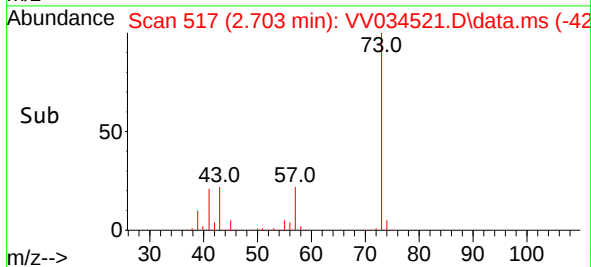

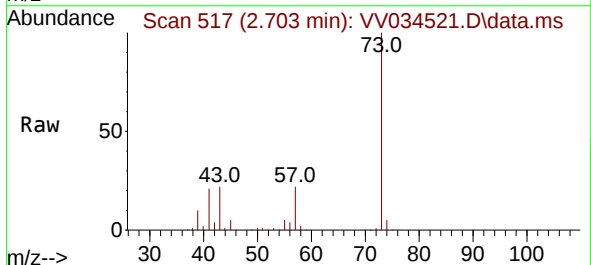




#19
1,1-Dichloroethane
Concen: 88.084 ug/L
RT: 3.108 min Scan# 64
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 63 Resp: 394321
Ion Ratio Lower Upper
63 100
65 31.3 22.1 41.1
83 14.0 9.9 18.3

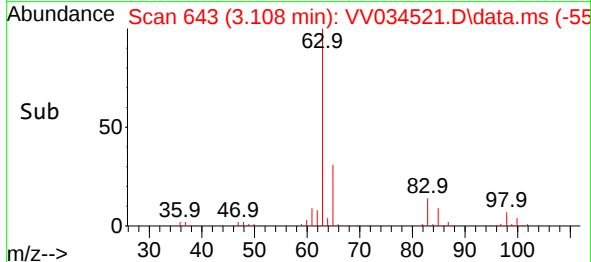

#25
Chloroform
Concen: 82.158 ug/L
RT: 4.275 min Scan# 1006
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 83 Resp: 381209
Ion Ratio Lower Upper
83 100
85 65.8 45.5 84.5


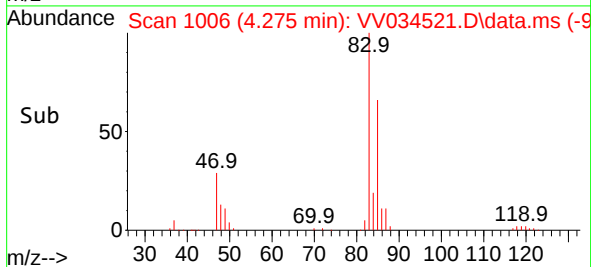

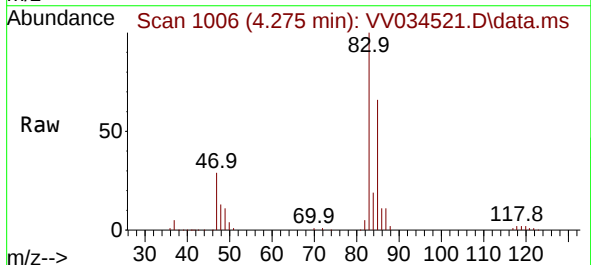


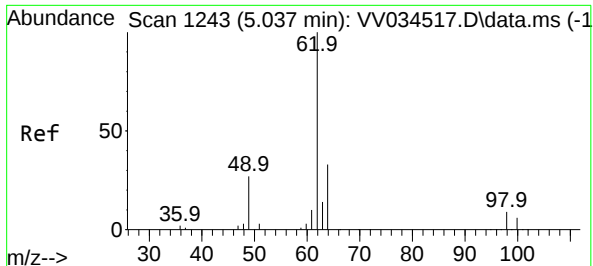

#27
1,2-Dichloroethane
Concen: 103.942 ug/L
RT: 5.037 min Scan# 1149
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 62 Resp: 391845
Ion Ratio Lower Upper
62 100
98 8.4 6.6 10.0

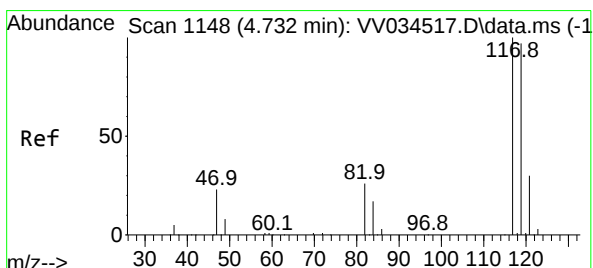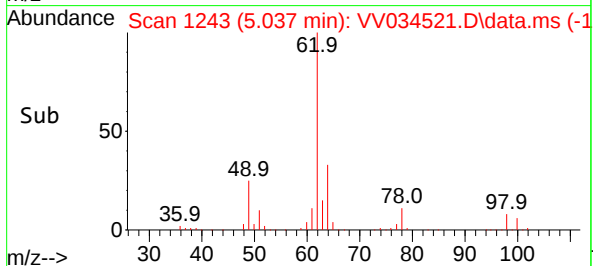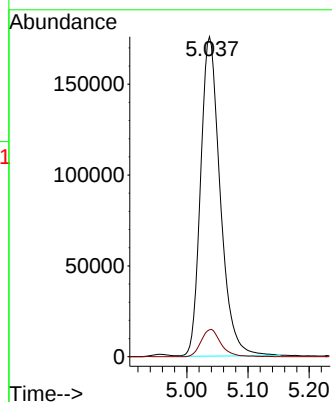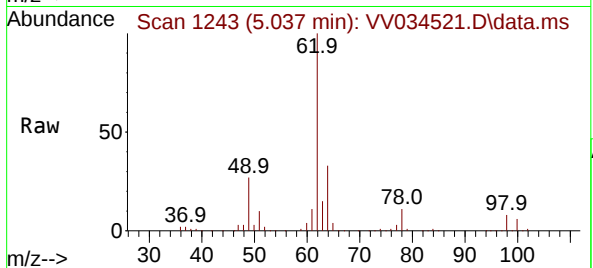

#31
Carbon tetrachloride
Concen: 31.317 ug/L
RT: 4.735 min Scan# 1149
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 117 Resp: 117234
Ion Ratio Lower Upper
117 100
119 96.9 77.5 116.3

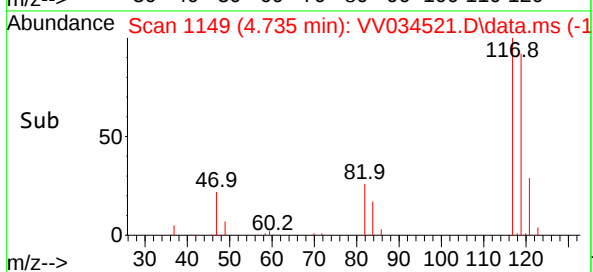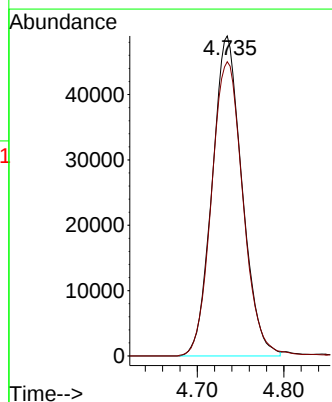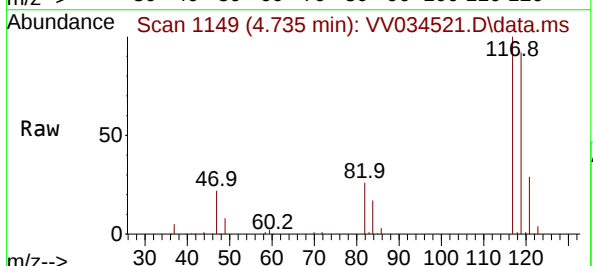

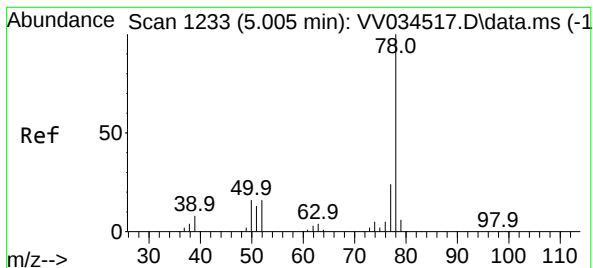

#33

Benzene

Concen: 24.108 ug/L

RT: 5.011 min Scan# 1

Delta R.T. 0.006 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50





Instrument :

MSVOA_V

ClientSampleId :

DCNO1

Tgt Ion: 78 Resp: 220639

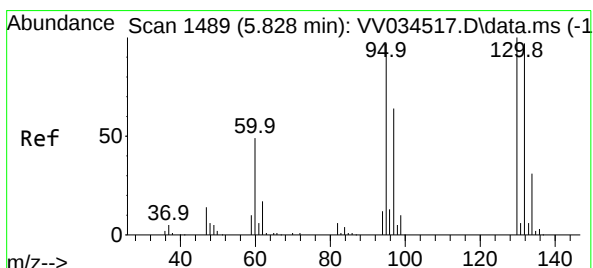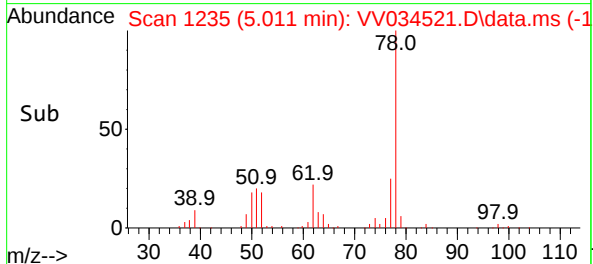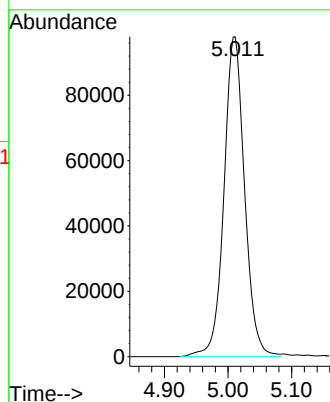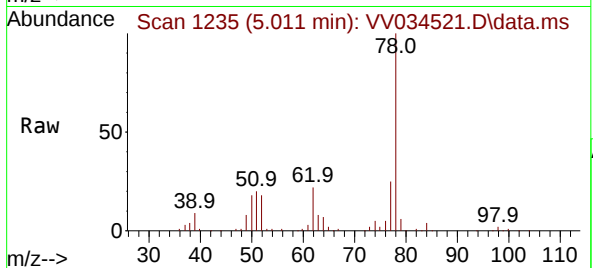

#34

Trichloroethene

Concen: 11.501 ug/L

RT: 5.837 min Scan# 1492

Delta R.T. 0.009 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Tgt Ion: 95 Resp: 29920




Ion Ratio Lower Upper


95 100

97 65.7 44.7 83.1

132 94.1 65.3 121.3

130 101.4 69.1 128.3


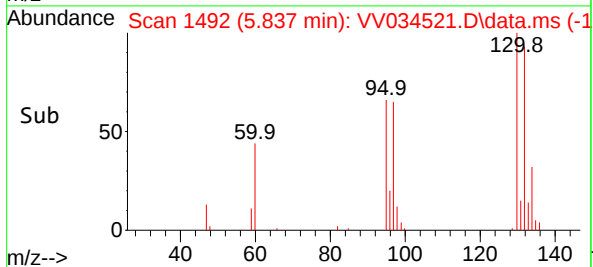

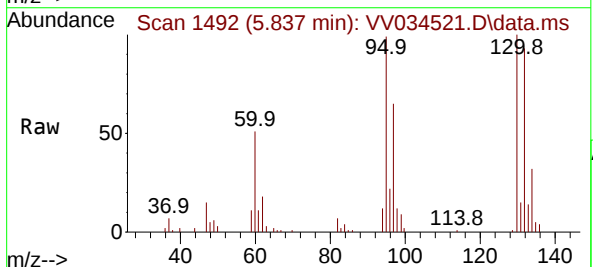




#38
Bromodichloromethane
Concen: 11.462 ug/L
RT: 6.436 min Scan# 1
Delta R.T. 0.006 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 83 Resp: 38632
Ion Ratio Lower Upper
83 100
85 65.8 44.6 82.8
127 9.5 6.9 10.3

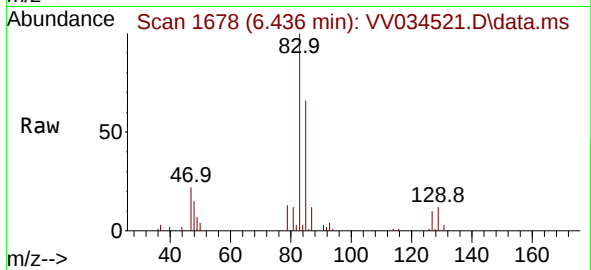

#39
cis-1,3-Dichloropropene
Concen: 37.336 ug/L
RT: 6.953 min Scan# 1839
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 75 Resp: 144947
Ion Ratio Lower Upper
75 100
77 31.4 20.9 38.9

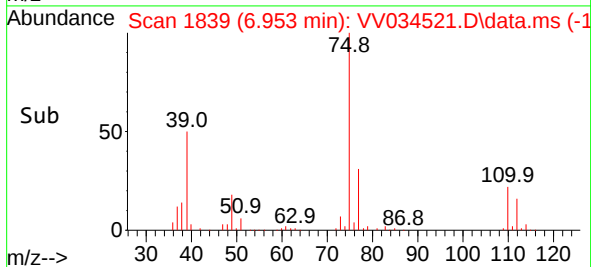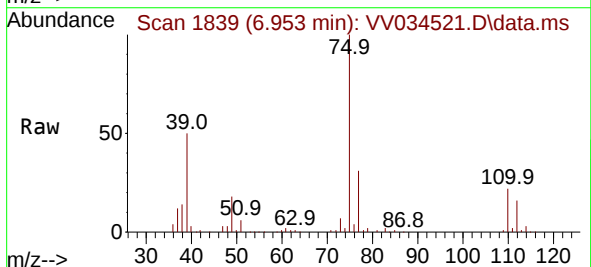

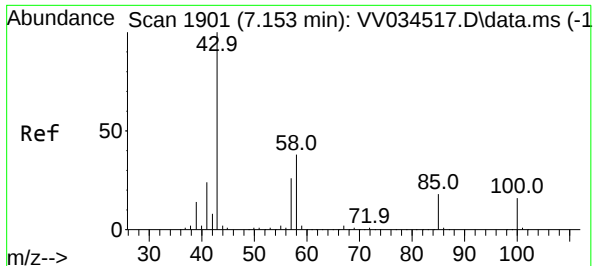

#40

4-Methyl-2-pentanone

Concen: 99.558 ug/L

RT: 7.153 min Scan# 1901

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :

DCNO1





Tgt Ion: 43 Resp: 351765

Ion Ratio Lower Upper

43 100

58 39.1 30.6 46.0

100 16.1 12.5 18.7

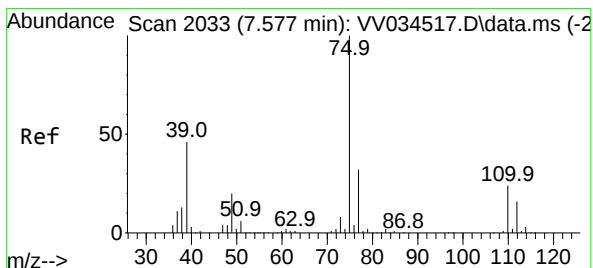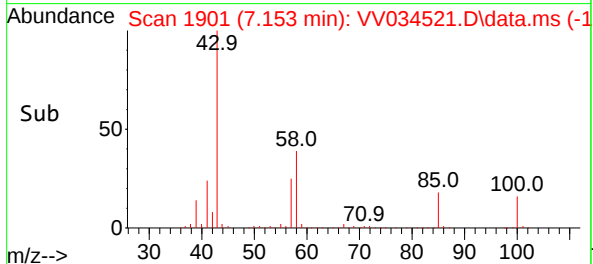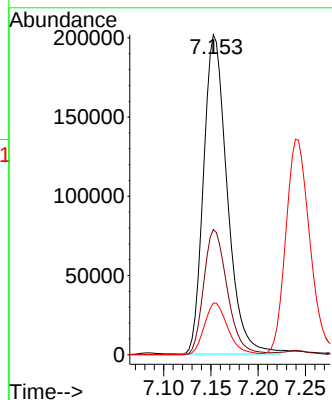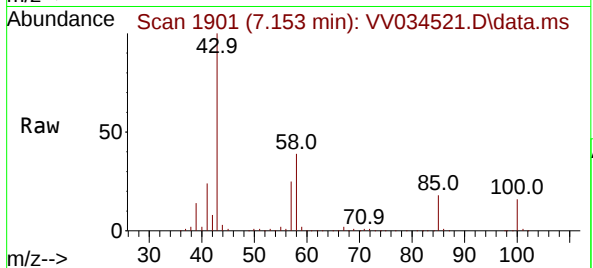

#44

trans-1,3-Dichloropropene

Concen: 100.492 ug/L

RT: 7.577 min Scan# 2033

Delta R.T. -0.000 min

Lab File: VV034521.D




Acq: 08 Mar 2024 10:50


Tgt Ion: 75 Resp: 375220

Ion Ratio Lower Upper

75 100

77 31.0 21.8 40.4

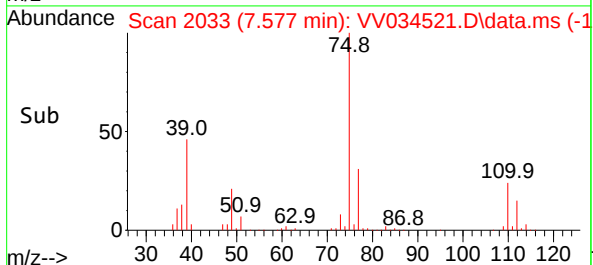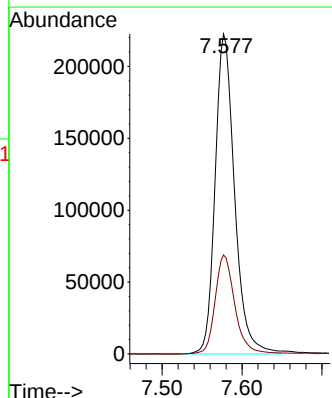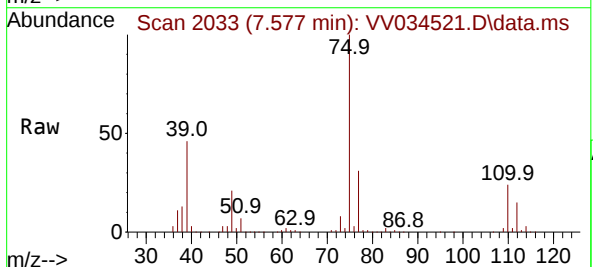



#45

1,1,2-Trichloroethane

Concen: 29.399 ug/L

RT: 7.770 min Scan# 2091

Delta R.T. 0.006 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :

DCNO1

Tgt Ion: 97 Resp: 67969





Ion Ratio Lower Upper

97 100

99 61.2 43.8 81.4

83 83.6 59.4 110.2

85 54.1 38.4 71.4

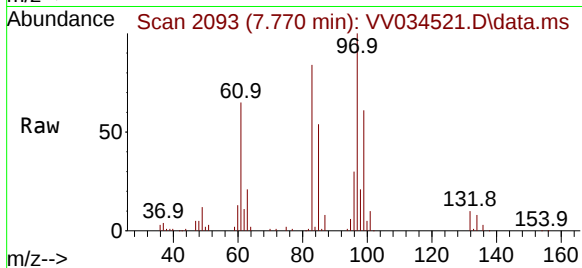

#46

Tetrachloroethene

Concen: 62.116 ug/L

RT: 7.902 min Scan# 2134

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Tgt Ion:164 Resp: 120181




Ion Ratio Lower Upper


164 100

129 96.1 65.7 121.9

131 90.4 62.2 115.6

166 131.0 89.7 166.7



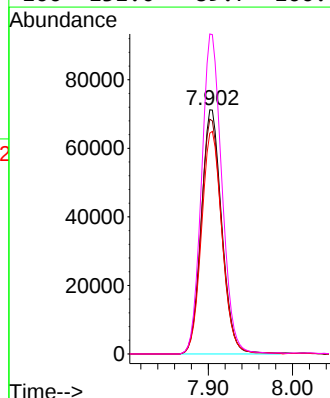
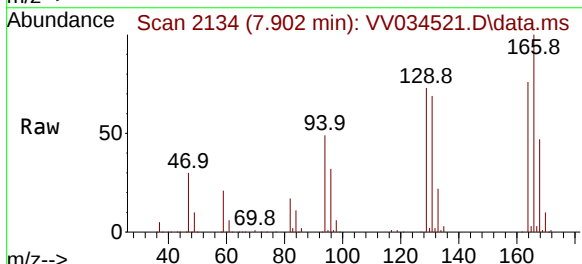




#48
2-Hexanone
Concen: 98.956 ug/L
RT: 8.072 min Scan# 2186
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 43 Resp: 278609
Ion Ratio Lower Upper
43 100
58 53.3 42.0 63.0
57 18.5 15.2 22.8
100 12.6 10.0 15.0

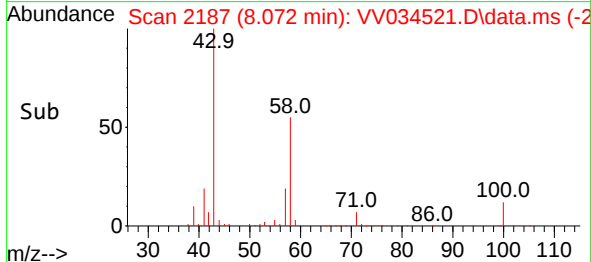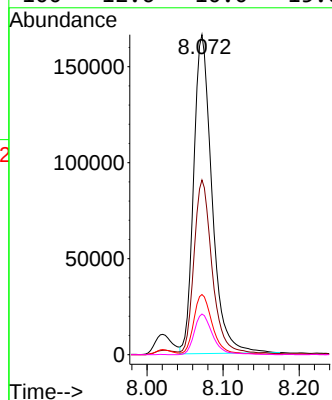

#49
Dibromochloromethane
Concen: 103.858 ug/L
RT: 8.175 min Scan# 2219
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion:129 Resp: 253388
Ion Ratio Lower Upper
129 100
127 77.9 53.3 98.9

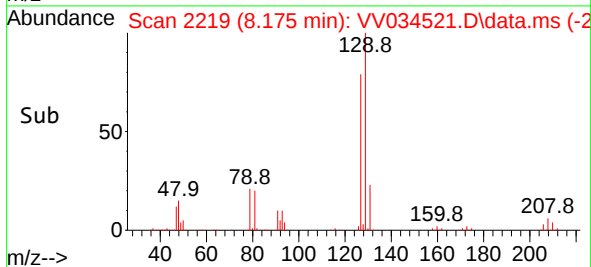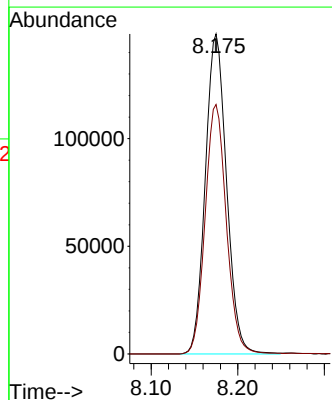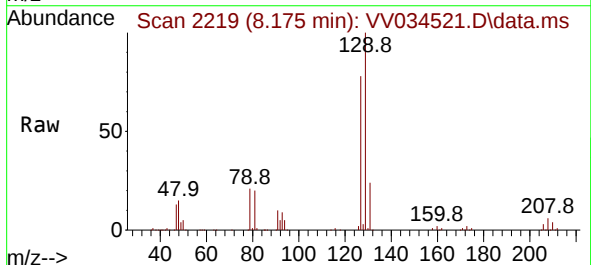



#50

1,2-Dibromoethane

Concen: 59.233 ug/L

RT: 8.278 min Scan# 21

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :

DCNO1





Tgt Ion:107 Resp: 145318

Ion Ratio Lower Upper

107 100

109 95.4 66.5 123.5

188 4.1 3.4 5.2



#51

Chlorobenzene

Concen: 17.337 ug/L

RT: 8.815 min Scan# 2418

Delta R.T. 0.003 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50




Tgt Ion:112 Resp: 108563


Ion Ratio Lower Upper

112 100

114 31.3 22.3 41.5

77 58.8 47.7 71.5


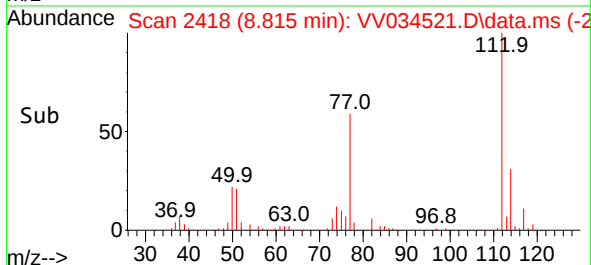
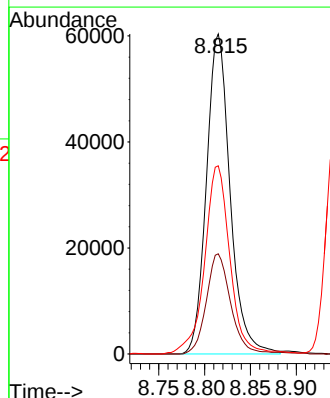
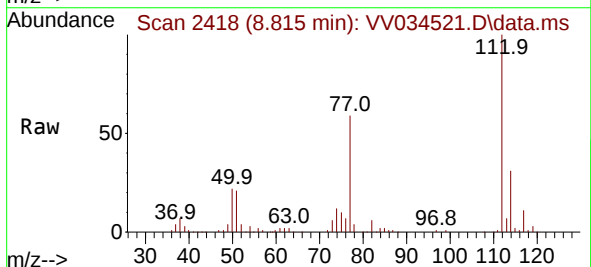




#52
Ethylbenzene
Concen: 76.132 ug/L
RT: 8.943 min Scan# 2458
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 91 Resp: 826292
Ion Ratio Lower Upper
91 100
106 30.5 21.3 39.5

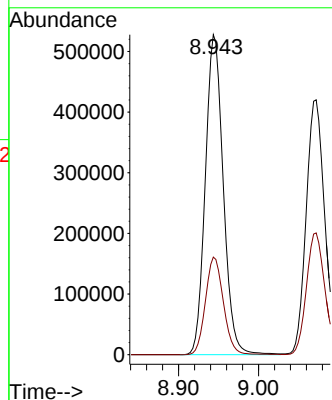

#53
m,p-Xylene
Concen: 78.602 ug/L
RT: 9.072 min Scan# 2498
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 106 Resp: 323732
Ion Ratio Lower Upper
106 100
91 209.3 145.3 269.9



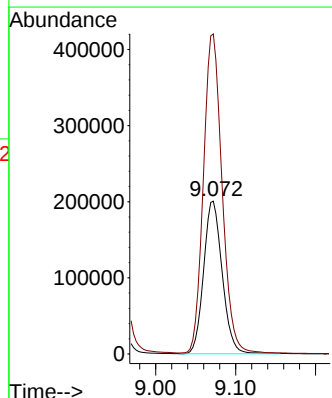





#54
o-Xylene
Concen: 62.231 ug/L
RT: 9.477 min Scan# 2623
Delta R.T. 0.003 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion:106 Resp: 250978
Ion Ratio Lower Upper
106 100
91 220.4 152.2 282.7



#55
Styrene
Concen: 62.262 ug/L
RT: 9.493 min Scan# 2629
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion:104 Resp: 425153
Ion Ratio Lower Upper
104 100
78 47.1 33.0 61.4


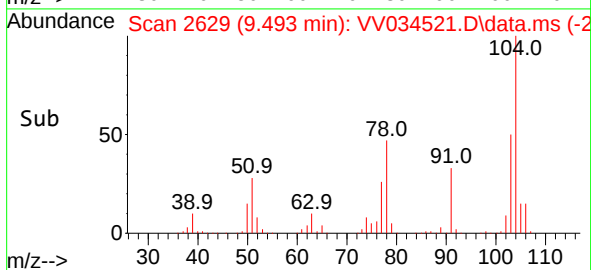

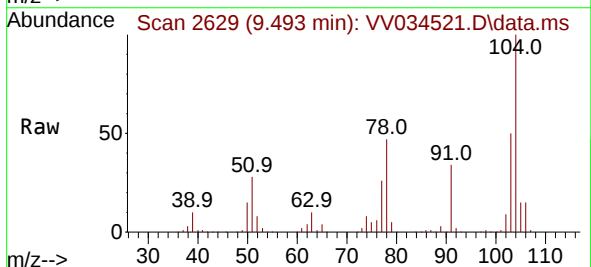




#61
1,2,3-Trichloropropane
Concen: 45.599 ug/L
RT: 10.207 min Scan# 2851
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50




Instrument :
MSVOA_V
ClientSampleId :
DCNO1


Tgt Ion: 75 Resp: 129263
Ion Ratio Lower Upper
75 100
77 32.7 25.9 38.9
110 40.6 33.1 49.7

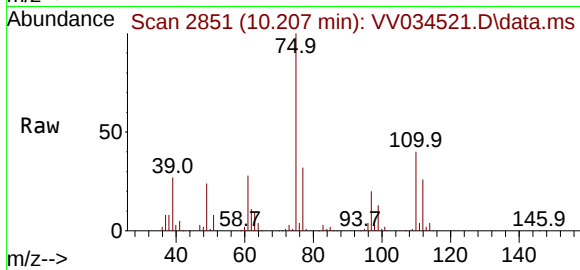

#62
1,3,5-Trimethylbenzene
Concen: 14.138 ug/L
RT: 10.474 min Scan# 2934
Delta R.T. -0.000 min
Lab File: VV034521.D
Acq: 08 Mar 2024 10:50

Tgt Ion: 105 Resp: 125261
Ion Ratio Lower Upper
105 100
120 47.7 38.2 57.2

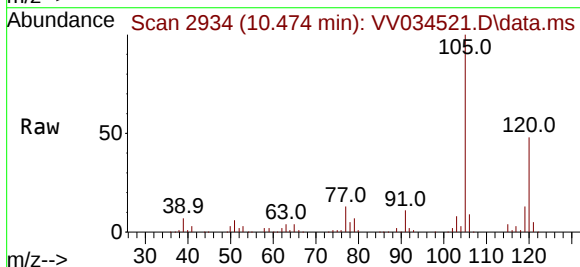



#63

1,2,4-Trimethylbenzene

Concen: 43.245 ug/L

RT: 10.850 min Scan# 3051

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :





DCNO1

Tgt Ion:105 Resp: 378939

Ion Ratio Lower Upper

105 100

120 44.2 36.2 54.4

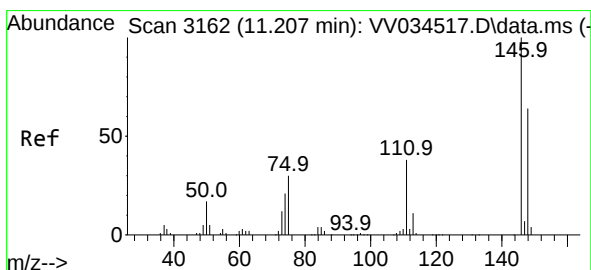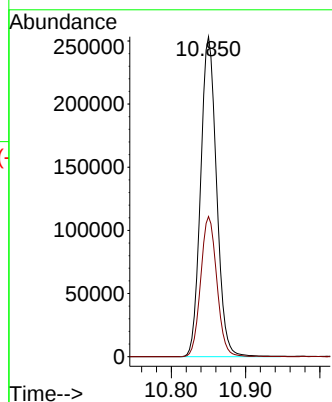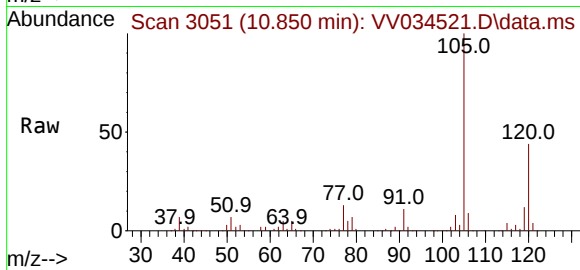

#65

1,4-Dichlorobenzene

Concen: 96.087 ug/L

RT: 11.207 min Scan# 3162

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50




Tgt Ion:146 Resp: 473851


Ion Ratio Lower Upper

146 100

111 38.6 26.5 49.1

148 64.9 44.0 81.8

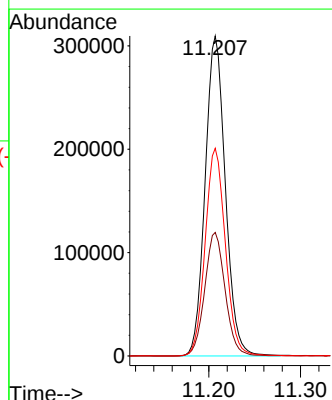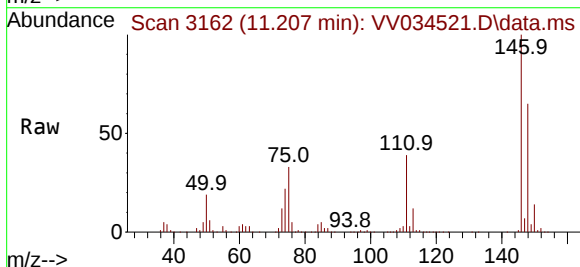



#67

1,2-Dichlorobenzene

Concen: 74.053 ug/L

RT: 11.577 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :

DCNO1





Tgt Ion:146 Resp: 360350

Ion Ratio Lower Upper

146 100

111 41.2 33.8 50.8

148 63.8 51.3 76.9

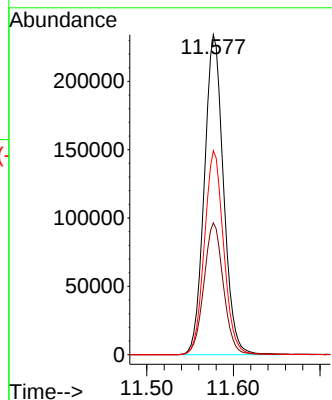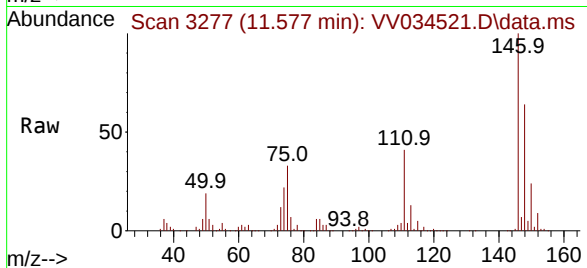

#68

1,2-Dibromo-3-chloropropane

Concen: 57.512 ug/L

RT: 12.365 min Scan# 3522

Delta R.T. 0.003 min

Lab File: VV034521.D

Acq: 08 Mar 2024 10:50




Tgt Ion: 75 Resp: 48566


Ion Ratio Lower Upper

75 100

155 78.4 63.3 94.9

157 100.9 81.4 122.0

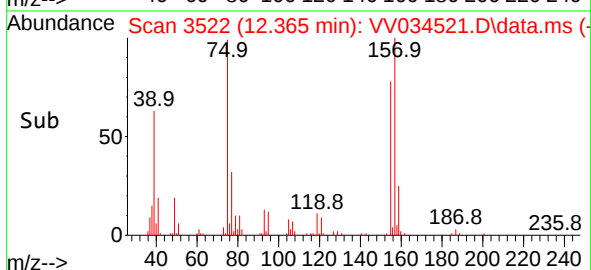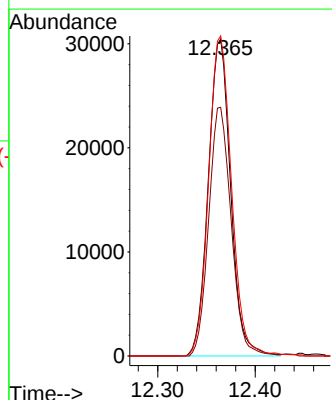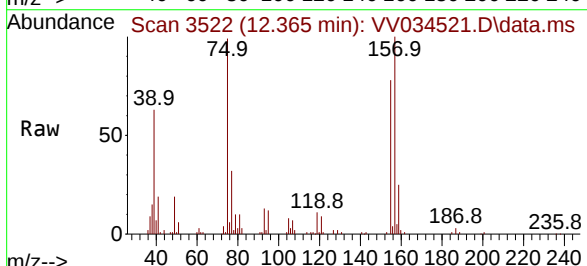



#70

1,2,4-trichlorobenzene

Concen: 35.666 ug/L

RT: 13.197 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV034521.D


Acq: 08 Mar 2024 10:50

Instrument :

MSVOA_V

ClientSampleId :

DCNO1

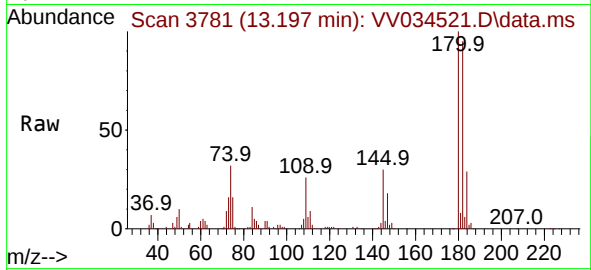

Tgt Ion:180 Resp: 116915

Ion Ratio Lower Upper

180 100

182 95.4 74.8 112.2

145 30.7 24.2 36.4

