

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034518.D
 Acq On : 08 Mar 2024 09:38
 Operator : SY/MD
 Sample : VV0308MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	179684	189565	14.66%	1.911%
2	1.529	144	152	171	rVB	152529	186479	14.42%	1.880%
3	2.056	306	316	350	rVB	303055	458306	35.45%	4.620%
4	2.182	350	355	360	rBV3	1052	980	0.08%	0.010%
5	2.224	366	368	369	rBV2	630	291	0.02%	0.003%
6	2.355	405	409	412	rBV2	298	198	0.02%	0.002%
7	2.400	421	423	427	rVB2	330	216	0.02%	0.002%
8	2.449	429	438	445	rVV3	2019	2954	0.23%	0.030%
9	2.799	544	547	553	rVB2	236	203	0.02%	0.002%
10	2.899	572	578	582	rBV	313	302	0.02%	0.003%
11	2.976	599	602	606	rBV2	360	258	0.02%	0.003%
12	3.272	691	694	697	rVB2	259	173	0.01%	0.002%
13	3.298	697	702	707	rBV2	201	263	0.02%	0.003%
14	3.375	722	726	731	rVV2	174	200	0.02%	0.002%
15	3.455	746	751	756	rBV	179	224	0.02%	0.002%
16	3.780	843	852	884	rBV	115110	301727	23.34%	3.041%
17	4.246	981	997	1029	rBV	205756	527580	40.81%	5.318%
18	4.458	1059	1063	1065	rBV3	546	381	0.03%	0.004%
19	4.577	1095	1100	1107	rVB4	549	672	0.05%	0.007%
20	4.619	1110	1113	1116	rBV2	368	293	0.02%	0.003%
21	4.690	1130	1135	1143	rVB3	275	379	0.03%	0.004%
22	4.744	1147	1152	1156	rBV2	440	426	0.03%	0.004%
23	4.883	1189	1195	1197	rBV2	151	169	0.01%	0.002%
24	4.953	1201	1217	1250	rBV2	488791	1292783	100.00%	13.031%
25	5.346	1335	1339	1341	rVB	380	262	0.02%	0.003%
26	5.394	1348	1354	1358	rBV3	308	367	0.03%	0.004%
27	5.413	1358	1360	1363	rBV2	238	175	0.01%	0.002%
28	5.532	1386	1397	1432	rBV	372843	771094	59.65%	7.773%
29	5.828	1478	1489	1510	rBV3	18666	40446	3.13%	0.408%
30	5.986	1525	1538	1565	rBV	284542	590946	45.71%	5.957%
31	6.140	1582	1586	1588	rBV4	431	355	0.03%	0.004%
32	6.413	1668	1671	1677	rVB2	227	209	0.02%	0.002%
33	6.465	1685	1687	1691	rVB2	293	168	0.01%	0.002%
34	6.593	1724	1727	1729	rBV3	507	317	0.02%	0.003%
35	6.912	1816	1826	1854	rBV	144525	276329	21.37%	2.785%
36	7.133	1890	1895	1896	rBV3	660	494	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034518.D
 Acq On : 08 Mar 2024 09:38
 Operator : SY/MD
 Sample : VV0308MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.243	1917	1929	1970	rBV	560068	988588	76.47%	9.965%
38	7.458	1994	1996	2004	rVB3	573	483	0.04%	0.005%
39	7.551	2016	2025	2056	rBV	99116	184224	14.25%	1.857%
40	7.873	2119	2125	2126	rBV2	420	364	0.03%	0.004%
41	8.021	2161	2171	2209	rBV	404421	731281	56.57%	7.371%
42	8.342	2269	2271	2273	rVB	528	184	0.01%	0.002%
43	8.400	2285	2289	2291	rBV2	485	305	0.02%	0.003%
44	8.436	2297	2300	2304	rBV2	340	302	0.02%	0.003%
45	8.625	2355	2359	2360	rBV	251	181	0.01%	0.002%
46	8.635	2360	2362	2365	rVV2	344	231	0.02%	0.002%
47	8.674	2370	2374	2376	rVV	290	235	0.02%	0.002%
48	8.783	2397	2408	2433	rBV	566544	915752	70.84%	9.231%
49	8.960	2460	2463	2465	rVB2	375	207	0.02%	0.002%
50	8.973	2465	2467	2472	rVB3	1027	667	0.05%	0.007%
51	8.998	2472	2475	2477	rBV2	414	262	0.02%	0.003%
52	9.104	2506	2508	2512	rVB4	709	447	0.03%	0.005%
53	9.169	2525	2528	2535	rVB3	251	249	0.02%	0.003%
54	9.368	2585	2590	2592	rBV2	222	223	0.02%	0.002%
55	9.500	2629	2631	2637	rVB2	343	246	0.02%	0.002%
56	9.526	2637	2639	2643	rBV	397	269	0.02%	0.003%
57	9.735	2700	2704	2707	rVB2	246	213	0.02%	0.002%
58	9.789	2718	2721	2727	rVB2	253	271	0.02%	0.003%
59	9.866	2742	2745	2746	rBV2	377	191	0.01%	0.002%
60	9.992	2778	2784	2788	rBV2	335	382	0.03%	0.004%
61	10.101	2812	2818	2820	rBV2	265	292	0.02%	0.003%
62	10.149	2821	2833	2859	rBV	380982	608347	47.06%	6.132%
63	10.320	2880	2886	2890	rBV3	527	537	0.04%	0.005%
64	10.455	2920	2928	2931	rVB2	254	316	0.02%	0.003%
65	10.487	2931	2938	2940	rBV2	404	455	0.04%	0.005%
66	10.609	2972	2976	2982	rBV2	227	236	0.02%	0.002%
67	10.860	3050	3054	3060	rBV4	389	526	0.04%	0.005%
68	11.053	3110	3114	3118	rVB2	312	229	0.02%	0.002%
69	11.133	3133	3139	3144	rBV4	919	1228	0.09%	0.012%
70	11.185	3144	3155	3186	rVV	562255	887607	68.66%	8.947%
71	11.333	3199	3201	3204	rVB3	598	254	0.02%	0.003%
72	11.448	3234	3237	3241	rVB3	461	314	0.02%	0.003%
73	11.474	3241	3245	3248	rBV	313	252	0.02%	0.003%
74	11.558	3258	3271	3292	rBV	586158	921605	71.29%	9.290%
75	11.731	3320	3325	3326	rVB2	363	204	0.02%	0.002%
76	11.947	3390	3392	3396	rVB	268	183	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034518.D
 Acq On : 08 Mar 2024 09:38
 Operator : SY/MD
 Sample : VV0308MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	12.124	3444	3447	3452	rVV3	353	271	0.02%	0.003%
78	12.271	3488	3493	3498	rBV2	367	431	0.03%	0.004%
79	12.474	3552	3556	3558	rBV	332	246	0.02%	0.002%
80	12.538	3573	3576	3579	rBV2	274	189	0.01%	0.002%
81	12.593	3586	3593	3599	rBV3	907	1234	0.10%	0.012%
82	12.673	3614	3618	3620	rBV2	396	306	0.02%	0.003%
83	12.760	3642	3645	3649	rBV2	244	201	0.02%	0.002%
84	13.059	3736	3738	3747	rVB2	549	400	0.03%	0.004%
85	13.204	3778	3783	3784	rBV2	2227	1665	0.13%	0.017%
86	13.291	3807	3810	3813	rVB	310	176	0.01%	0.002%
87	13.445	3848	3858	3871	rBV	7559	12604	0.97%	0.127%
88	13.554	3890	3892	3894	rBB2	342	169	0.01%	0.002%
89	13.622	3911	3913	3919	rVB3	356	270	0.02%	0.003%
90	13.686	3926	3933	3946	rBV8	3095	4825	0.37%	0.049%
91	14.011	4032	4034	4037	rBV3	354	272	0.02%	0.003%
92	14.130	4069	4071	4073	rBV2	296	169	0.01%	0.002%
93	14.165	4078	4082	4087	rVB3	425	426	0.03%	0.004%
94	14.201	4087	4093	4095	rBV2	618	526	0.04%	0.005%
95	14.300	4122	4124	4126	rBV2	337	180	0.01%	0.002%
96	14.490	4180	4183	4186	rBV2	431	360	0.03%	0.004%
97	14.570	4206	4208	4213	rBV3	351	225	0.02%	0.002%
98	14.821	4283	4286	4289	rBV3	366	299	0.02%	0.003%
99	14.950	4324	4326	4329	rVB2	516	243	0.02%	0.002%
100	15.037	4350	4353	4356	rBV5	471	361	0.03%	0.004%




Sum of corrected areas: 9920574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034518.D
Acq On : 08 Mar 2024 09:38
Operator : SY/MD
Sample : VV0308MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

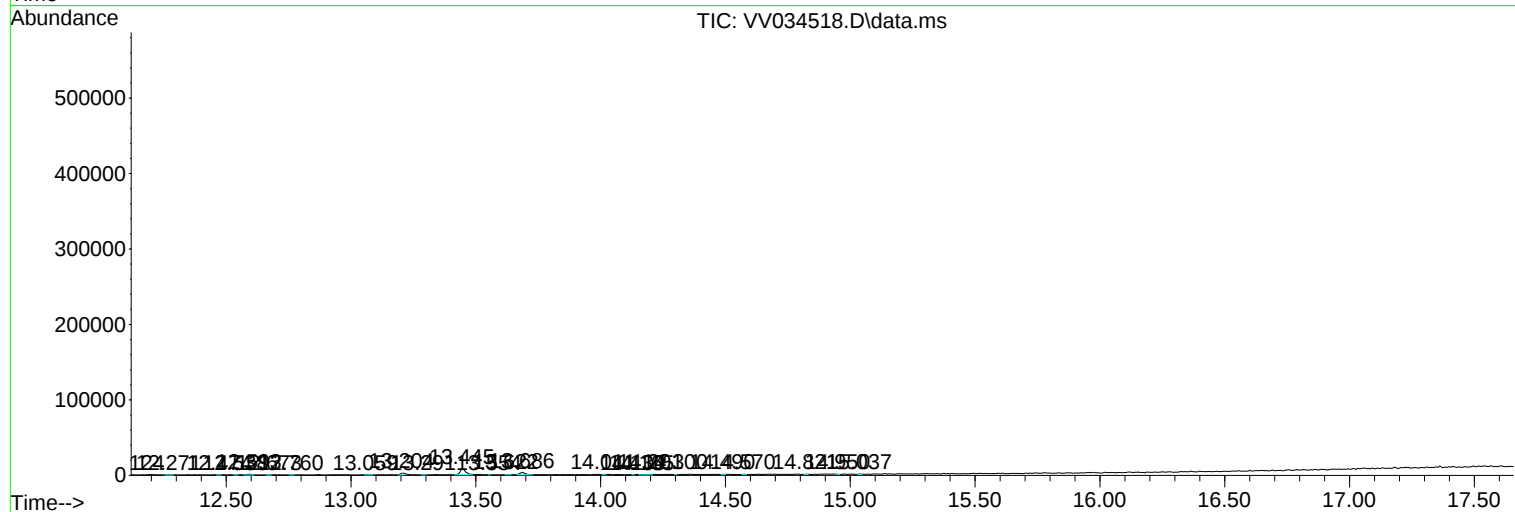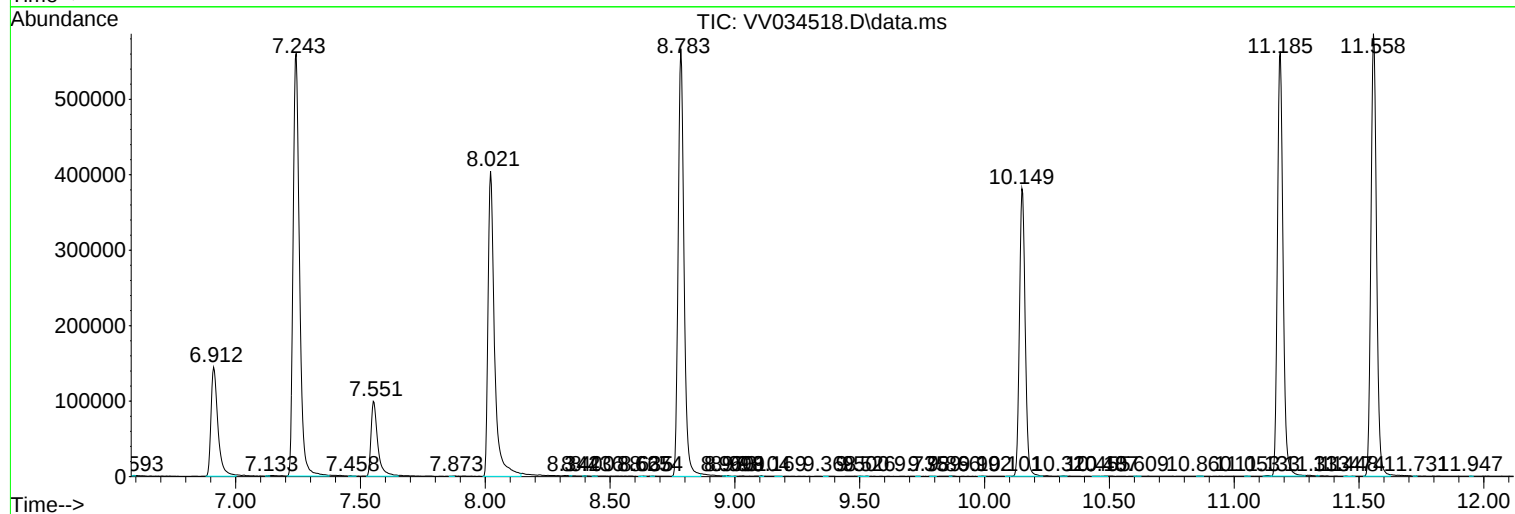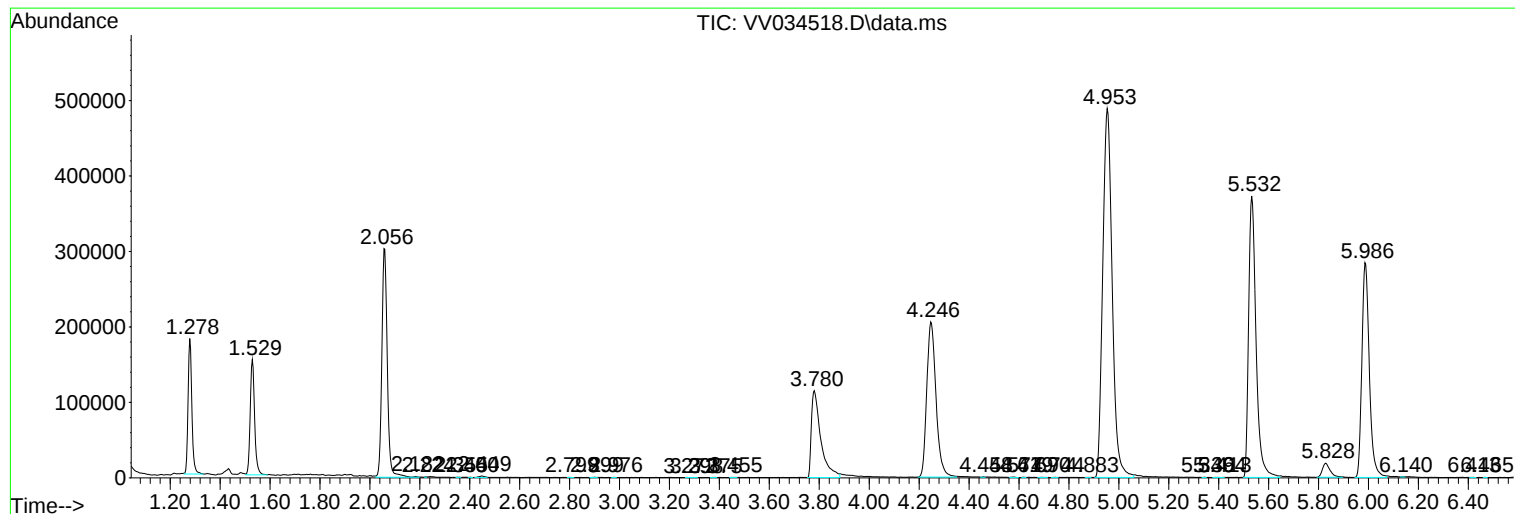

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034518.D
Acq On : 08 Mar 2024 09:38
Operator : SY/MD
Sample : VV0308MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034518.D
Acq On : 08 Mar 2024 09:38
Operator : SY/MD
Sample : VV0308MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
