

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034519.D
 Acq On : 08 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0308WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	174511	181270	14.08%	1.862%
2	1.529	145	152	169	rVB	152816	182512	14.17%	1.875%
3	2.057	306	316	332	rBV	299033	433568	33.67%	4.454%
4	2.237	367	372	377	rBV4	578	777	0.06%	0.008%
5	2.397	414	422	424	rBV3	480	543	0.04%	0.006%
6	2.446	430	437	444	rBV6	1613	2578	0.20%	0.026%
7	2.503	453	455	458	rBV	247	119	0.01%	0.001%
8	2.706	512	518	522	rBV3	331	369	0.03%	0.004%
9	3.082	632	635	638	rBV	236	128	0.01%	0.001%
10	3.169	657	662	667	rBV2	227	314	0.02%	0.003%
11	3.240	681	684	687	rVB2	154	110	0.01%	0.001%
12	3.259	688	690	693	rBV2	186	132	0.01%	0.001%
13	3.327	707	711	713	rVV2	163	124	0.01%	0.001%
14	3.407	734	736	740	rVB	148	86	0.01%	0.001%
15	3.429	740	743	749	rBV	319	316	0.02%	0.003%
16	3.474	755	757	761	rBV2	124	90	0.01%	0.001%
17	3.606	794	798	801	rBV2	150	125	0.01%	0.001%
18	3.629	801	805	810	rBV2	178	220	0.02%	0.002%
19	3.780	843	852	888	rBV	118153	313523	24.35%	3.221%
20	4.246	980	997	1040	rBV	206142	536850	41.69%	5.515%
21	4.638	1115	1119	1123	rBV2	276	310	0.02%	0.003%
22	4.838	1176	1181	1185	rBV3	357	455	0.04%	0.005%
23	4.899	1197	1200	1201	rBV	319	163	0.01%	0.002%
24	4.953	1201	1217	1256	rVV2	480172	1287687	100.00%	13.229%
25	5.314	1328	1329	1331	rBV2	153	85	0.01%	0.001%
26	5.346	1337	1339	1340	rBV	308	116	0.01%	0.001%
27	5.407	1351	1358	1361	rVB3	349	441	0.03%	0.005%
28	5.442	1361	1369	1374	rBV3	413	614	0.05%	0.006%
29	5.471	1374	1378	1380	rBV2	222	206	0.02%	0.002%
30	5.532	1386	1397	1428	rBV	368124	761015	59.10%	7.818%
31	5.828	1479	1489	1516	rVB3	17990	41538	3.23%	0.427%
32	5.986	1525	1538	1571	rBV	277049	581256	45.14%	5.971%
33	6.256	1619	1622	1623	rBV	320	147	0.01%	0.002%
34	6.320	1640	1642	1644	rBV	298	134	0.01%	0.001%
35	6.352	1649	1652	1656	rBV2	398	292	0.02%	0.003%
36	6.375	1657	1659	1664	rVB	248	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034519.D
 Acq On : 08 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0308WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.410	1666	1670	1671	rBV	212	148	0.01%	0.002%
38	6.458	1683	1685	1688	rVV2	200	91	0.01%	0.001%
39	6.478	1689	1691	1696	rVB2	307	132	0.01%	0.001%
40	6.503	1696	1699	1702	rBV2	130	91	0.01%	0.001%
41	6.661	1745	1748	1751	rBV2	267	266	0.02%	0.003%
42	6.754	1774	1777	1782	rVB	283	219	0.02%	0.002%
43	6.783	1782	1786	1790	rBV2	248	222	0.02%	0.002%
44	6.806	1790	1793	1794	rBV2	187	111	0.01%	0.001%
45	6.828	1798	1800	1805	rVB	232	167	0.01%	0.002%
46	6.912	1813	1826	1858	rBV	144510	278106	21.60%	2.857%
47	7.198	1912	1915	1917	rBV2	365	230	0.02%	0.002%
48	7.243	1918	1929	1970	rVV	550945	970419	75.36%	9.969%
49	7.551	2016	2025	2053	rBV	96312	180027	13.98%	1.849%
50	7.818	2106	2108	2110	rBV	217	101	0.01%	0.001%
51	7.873	2123	2125	2127	rBV2	302	158	0.01%	0.002%
52	7.912	2135	2137	2141	rVB	496	340	0.03%	0.003%
53	7.931	2141	2143	2146	rBV	264	146	0.01%	0.001%
54	8.021	2162	2171	2210	rBV	401216	720969	55.99%	7.407%
55	8.487	2312	2316	2317	rBV2	376	237	0.02%	0.002%
56	8.497	2317	2319	2320	rBV	343	125	0.01%	0.001%
57	8.558	2336	2338	2343	rBV3	223	252	0.02%	0.003%
58	8.580	2343	2345	2348	rVB2	300	119	0.01%	0.001%
59	8.600	2348	2351	2352	rBV	240	117	0.01%	0.001%
60	8.632	2359	2361	2363	rBV2	244	113	0.01%	0.001%
61	8.648	2363	2366	2368	rBV	287	202	0.02%	0.002%
62	8.690	2377	2379	2381	rVB	209	86	0.01%	0.001%
63	8.783	2393	2408	2435	rBV	548065	895756	69.56%	9.202%
64	9.069	2494	2497	2499	rBV	348	168	0.01%	0.002%
65	9.169	2522	2528	2533	rBV2	247	291	0.02%	0.003%
66	9.191	2533	2535	2537	rVV	270	135	0.01%	0.001%
67	9.326	2573	2577	2579	rBV	239	159	0.01%	0.002%
68	9.403	2599	2601	2604	rBV	148	94	0.01%	0.001%
69	9.423	2604	2607	2608	rVV	205	99	0.01%	0.001%
70	9.455	2613	2617	2621	rVB3	211	177	0.01%	0.002%
71	9.477	2621	2624	2627	rBV2	170	135	0.01%	0.001%
72	9.522	2636	2638	2639	rBV2	174	85	0.01%	0.001%
73	9.577	2652	2655	2659	rVB	260	157	0.01%	0.002%
74	9.603	2660	2663	2667	rBV3	225	207	0.02%	0.002%
75	9.767	2711	2714	2720	rBV2	186	241	0.02%	0.002%
76	9.918	2759	2761	2763	rBV	212	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034519.D
 Acq On : 08 Mar 2024 10:02
 Operator : SY/MD
 Sample : VV0308WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.149	2822	2833	2862	rBV	368631	596710	46.34%	6.130%
78	10.317	2881	2885	2887	rBV2	464	410	0.03%	0.004%
79	10.436	2918	2922	2928	rBV2	242	300	0.02%	0.003%
80	10.577	2960	2966	2969	rBV2	189	233	0.02%	0.002%
81	10.596	2969	2972	2975	rVB	334	220	0.02%	0.002%
82	10.625	2975	2981	2984	rBV2	190	239	0.02%	0.002%
83	10.866	3050	3056	3057	rBV2	362	317	0.02%	0.003%
84	10.934	3074	3077	3080	rBV	259	155	0.01%	0.002%
85	11.133	3135	3139	3144	rBV2	328	328	0.03%	0.003%
86	11.185	3144	3155	3176	rBV	545598	853658	66.29%	8.770%
87	11.329	3196	3200	3203	rBV4	429	389	0.03%	0.004%
88	11.474	3243	3245	3248	rVB	313	131	0.01%	0.001%
89	11.500	3249	3253	3259	rBV2	347	371	0.03%	0.004%
90	11.558	3259	3271	3299	rBV	568462	895171	69.52%	9.196%
91	11.805	3345	3348	3353	rBV	491	338	0.03%	0.003%
92	12.079	3430	3433	3434	rBV	186	110	0.01%	0.001%
93	12.593	3590	3593	3598	rBV2	555	441	0.03%	0.005%
94	12.786	3651	3653	3657	rBV	265	144	0.01%	0.001%
95	13.021	3722	3726	3727	rBV2	487	369	0.03%	0.004%
96	13.088	3740	3747	3750	rBV2	407	532	0.04%	0.005%
97	13.210	3777	3785	3789	rBV4	1119	1555	0.12%	0.016%
98	13.329	3817	3822	3825	rBV2	476	467	0.04%	0.005%
99	13.419	3846	3850	3852	rBV2	523	462	0.04%	0.005%
100	13.680	3925	3931	3934	rBV4	1258	1513	0.12%	0.016%




Sum of corrected areas: 9733933

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034519.D
Acq On : 08 Mar 2024 10:02
Operator : SY/MD
Sample : VV0308WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

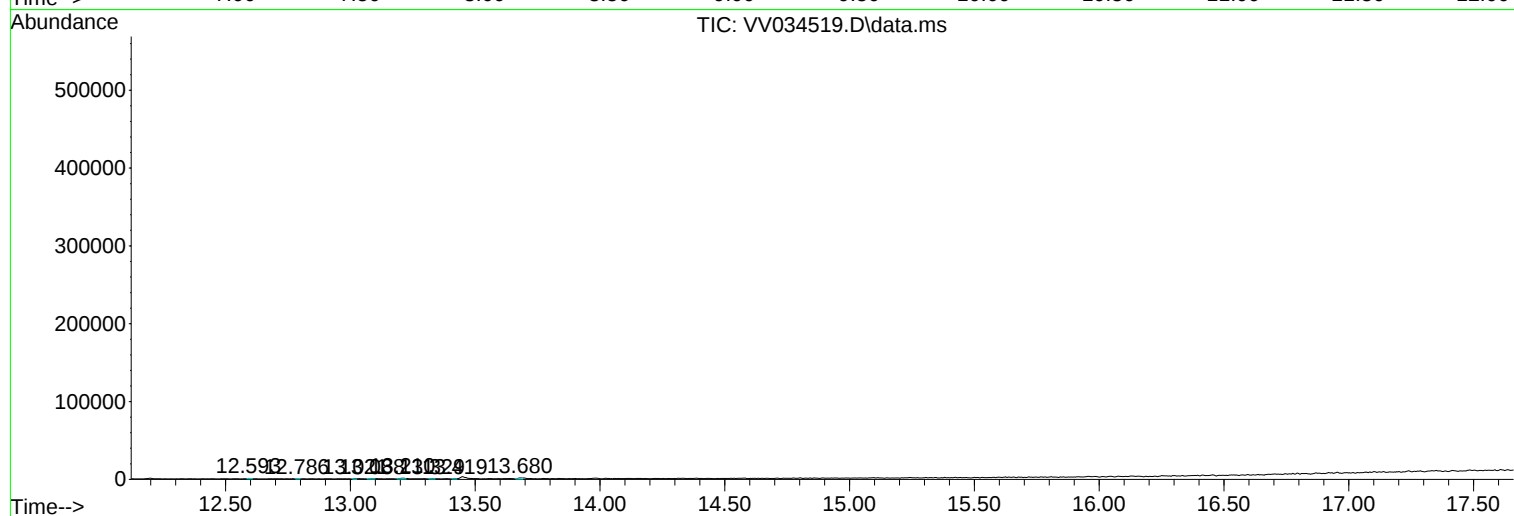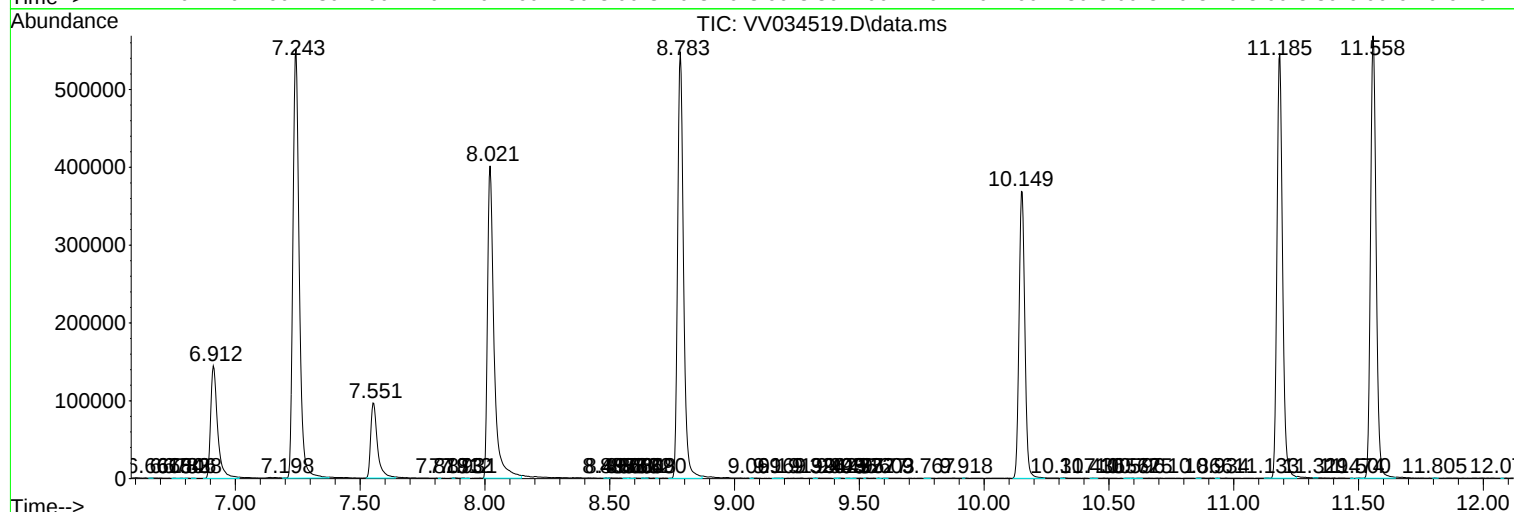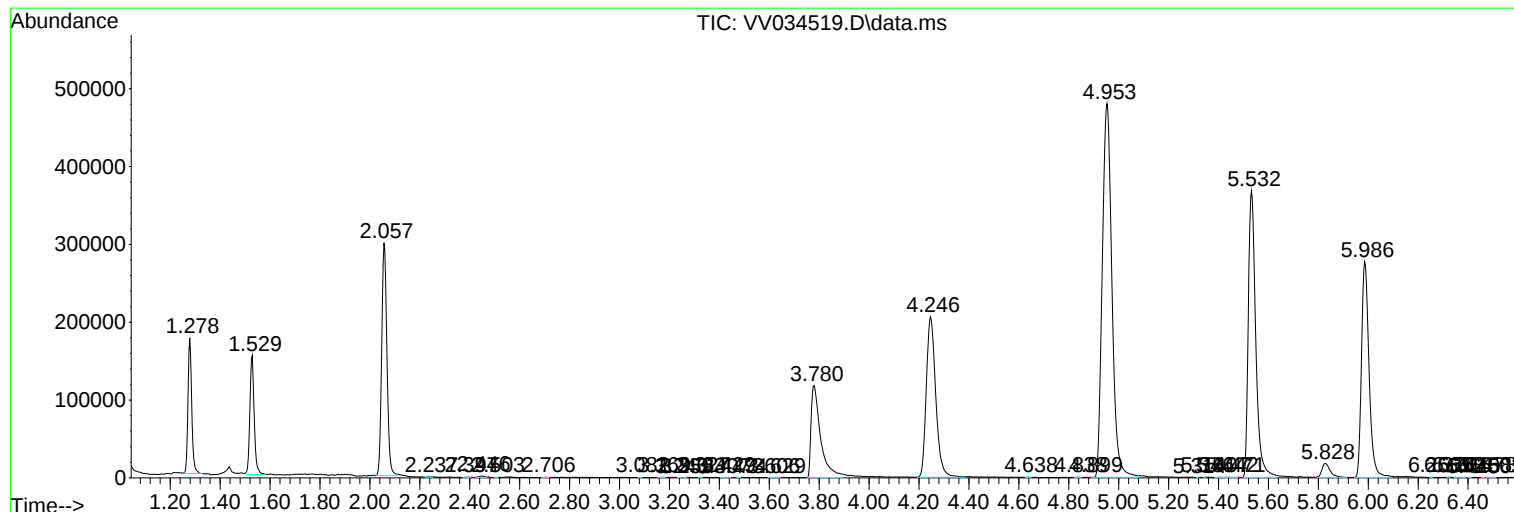

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034519.D
Acq On : 08 Mar 2024 10:02
Operator : SY/MD
Sample : VV0308WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034519.D
Acq On : 08 Mar 2024 10:02
Operator : SY/MD
Sample : VV0308WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc