

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034520.D
 Acq On : 08 Mar 2024 10:26
 Operator : SY/MD
 Sample : P1681-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	160722	172839	14.02%	1.849%
2	1.526	145	151	166	rVB	133633	162874	13.21%	1.743%
3	2.056	306	316	343	rVB	273928	409985	33.26%	4.386%
4	2.227	367	369	370	rBV	535	270	0.02%	0.003%
5	2.445	430	437	447	rVB3	1856	2933	0.24%	0.031%
6	2.622	489	492	493	rBV	248	142	0.01%	0.002%
7	2.757	532	534	536	rBV	160	87	0.01%	0.001%
8	2.838	555	559	562	rBV2	125	128	0.01%	0.001%
9	2.870	567	569	574	rVB2	256	171	0.01%	0.002%
10	2.905	576	580	581	rBV	128	99	0.01%	0.001%
11	2.934	587	589	593	rBV2	105	84	0.01%	0.001%
12	2.973	600	601	604	rBV	185	84	0.01%	0.001%
13	3.121	643	647	649	rBV2	97	93	0.01%	0.001%
14	3.249	682	687	690	rBV	309	252	0.02%	0.003%
15	3.294	699	701	704	rVB	243	71	0.01%	0.001%
16	3.336	710	714	717	rBV	196	156	0.01%	0.002%
17	3.368	721	724	727	rVV	184	122	0.01%	0.001%
18	3.490	759	762	764	rBV2	129	99	0.01%	0.001%
19	3.529	770	774	775	rBV2	168	110	0.01%	0.001%
20	3.587	789	792	795	rVB3	228	134	0.01%	0.001%
21	3.613	795	800	804	rBV2	177	198	0.02%	0.002%
22	3.703	826	828	831	rBV	163	102	0.01%	0.001%
23	3.728	832	836	838	rVV2	133	95	0.01%	0.001%
24	3.780	843	852	881	rBV	119823	310626	25.20%	3.323%
25	4.246	983	997	1026	rBV	195442	501543	40.69%	5.366%
26	4.741	1148	1151	1155	rBV3	315	225	0.02%	0.002%
27	4.815	1173	1174	1178	rBV	270	216	0.02%	0.002%
28	4.953	1200	1217	1254	rBV2	457669	1232654	100.00%	13.188%
29	5.339	1334	1337	1344	rVB	356	239	0.02%	0.003%
30	5.442	1367	1369	1371	rVB	263	131	0.01%	0.001%
31	5.455	1371	1373	1376	rBV	205	115	0.01%	0.001%
32	5.532	1386	1397	1428	rBV	342752	713314	57.87%	7.632%
33	5.828	1479	1489	1508	rBV4	17745	40026	3.25%	0.428%
34	5.931	1518	1521	1524	rVB4	351	220	0.02%	0.002%
35	5.986	1525	1538	1577	rBV	269063	565492	45.88%	6.050%
36	6.227	1610	1613	1617	rBV3	441	371	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034520.D
 Acq On : 08 Mar 2024 10:26
 Operator : SY/MD
 Sample : P1681-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.323	1639	1643	1645	rVB2	291	150	0.01%	0.002%
38	6.564	1714	1718	1721	rBV	139	120	0.01%	0.001%
39	6.596	1721	1728	1731	rBV3	885	1151	0.09%	0.012%
40	6.680	1752	1754	1756	rBV2	288	142	0.01%	0.002%
41	6.715	1763	1765	1768	rBV	294	199	0.02%	0.002%
42	6.828	1798	1800	1807	rVB2	280	182	0.01%	0.002%
43	6.912	1816	1826	1852	rBV	139365	268666	21.80%	2.874%
44	7.243	1918	1929	1962	rBV	519145	918395	74.51%	9.826%
45	7.551	2016	2025	2051	rBV	95606	176052	14.28%	1.884%
46	7.834	2111	2113	2116	rBV2	287	123	0.01%	0.001%
47	7.850	2116	2118	2121	rVV	198	110	0.01%	0.001%
48	7.876	2121	2126	2131	rVB3	547	660	0.05%	0.007%
49	7.895	2131	2132	2135	rVB2	307	115	0.01%	0.001%
50	7.918	2135	2139	2140	rBV2	223	148	0.01%	0.002%
51	7.957	2149	2151	2156	rBV	209	162	0.01%	0.002%
52	8.021	2162	2171	2216	rBV	413648	744157	60.37%	7.962%
53	8.616	2354	2356	2358	rBV	204	124	0.01%	0.001%
54	8.645	2363	2365	2367	rVV	232	78	0.01%	0.001%
55	8.696	2379	2381	2384	rBV	214	130	0.01%	0.001%
56	8.783	2397	2408	2433	rBV	522970	857877	69.60%	9.178%
57	8.995	2472	2474	2475	rBV	242	83	0.01%	0.001%
58	9.005	2475	2477	2479	rVV2	411	187	0.02%	0.002%
59	9.056	2490	2493	2497	rVB3	440	320	0.03%	0.003%
60	9.085	2501	2502	2506	rVB2	324	152	0.01%	0.002%
61	9.108	2506	2509	2512	rBV2	369	220	0.02%	0.002%
62	9.175	2528	2530	2531	rBV2	193	69	0.01%	0.001%
63	9.201	2535	2538	2541	rBV2	209	189	0.02%	0.002%
64	9.255	2552	2555	2557	rBV2	333	215	0.02%	0.002%
65	9.429	2606	2609	2611	rVV	149	92	0.01%	0.001%
66	9.493	2625	2629	2632	rBV	291	254	0.02%	0.003%
67	9.567	2650	2652	2656	rVB	248	122	0.01%	0.001%
68	9.664	2675	2682	2685	rBV2	250	299	0.02%	0.003%
69	9.712	2694	2697	2700	rBV2	191	147	0.01%	0.002%
70	9.792	2720	2722	2724	rBV2	146	93	0.01%	0.001%
71	9.857	2740	2742	2744	rBV	243	135	0.01%	0.001%
72	10.040	2793	2799	2801	rBV2	175	191	0.02%	0.002%
73	10.153	2822	2834	2856	rBV	374777	602229	48.86%	6.443%
74	10.381	2904	2905	2907	rBV	213	69	0.01%	0.001%
75	10.474	2926	2934	2937	rBV	362	429	0.03%	0.005%
76	10.526	2947	2950	2952	rBV2	154	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034520.D
 Acq On : 08 Mar 2024 10:26
 Operator : SY/MD
 Sample : P1681-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.538	2952	2954	2955	rBV	271	74	0.01%	0.001%
78	10.590	2966	2970	2973	rBV	334	255	0.02%	0.003%
79	10.651	2986	2989	2990	rBV	129	78	0.01%	0.001%
80	10.789	3030	3032	3036	rBV2	294	152	0.01%	0.002%
81	10.812	3036	3039	3043	rBV2	164	161	0.01%	0.002%
82	10.860	3051	3054	3056	rBV	304	166	0.01%	0.002%
83	10.963	3084	3086	3089	rBV2	182	125	0.01%	0.001%
84	11.130	3137	3138	3140	rBV	398	207	0.02%	0.002%
85	11.185	3144	3155	3182	rVV	510219	803911	65.22%	8.601%
86	11.455	3236	3239	3241	rBV	211	145	0.01%	0.002%
87	11.558	3259	3271	3292	rBV	527525	847619	68.76%	9.069%
88	11.767	3334	3336	3338	rBV	306	143	0.01%	0.002%
89	11.815	3346	3351	3352	rBV	245	185	0.02%	0.002%
90	11.931	3385	3387	3388	rBV	264	70	0.01%	0.001%
91	12.255	3485	3488	3490	rBV2	190	114	0.01%	0.001%
92	12.599	3591	3595	3599	rBV2	556	372	0.03%	0.004%
93	12.622	3599	3602	3603	rBV	217	119	0.01%	0.001%
94	12.747	3637	3641	3645	rBV2	602	540	0.04%	0.006%
95	12.818	3660	3663	3667	rBV2	325	238	0.02%	0.003%
96	12.947	3700	3703	3705	rBV2	307	189	0.02%	0.002%
97	13.117	3753	3756	3759	rBV	470	319	0.03%	0.003%
98	13.210	3783	3785	3787	rBV	453	220	0.02%	0.002%
99	13.423	3850	3851	3854	rBV	352	230	0.02%	0.002%
100	13.622	3911	3913	3918	rVB2	480	354	0.03%	0.004%




Sum of corrected areas: 9346636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034520.D
Acq On : 08 Mar 2024 10:26
Operator : SY/MD
Sample : P1681-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

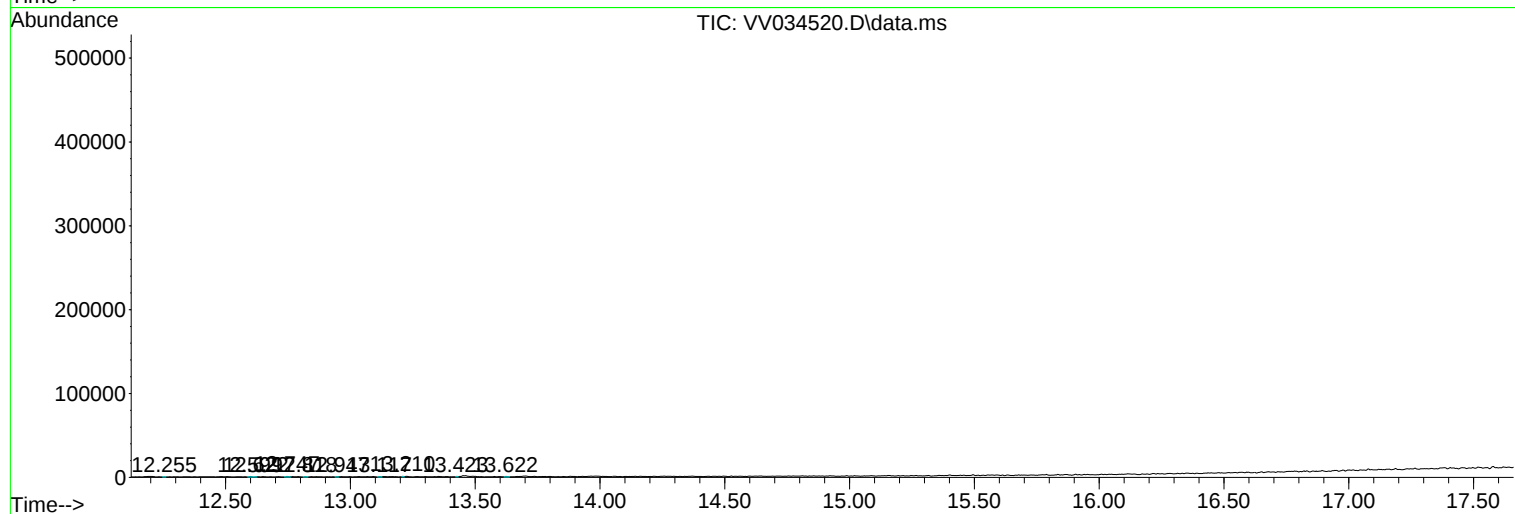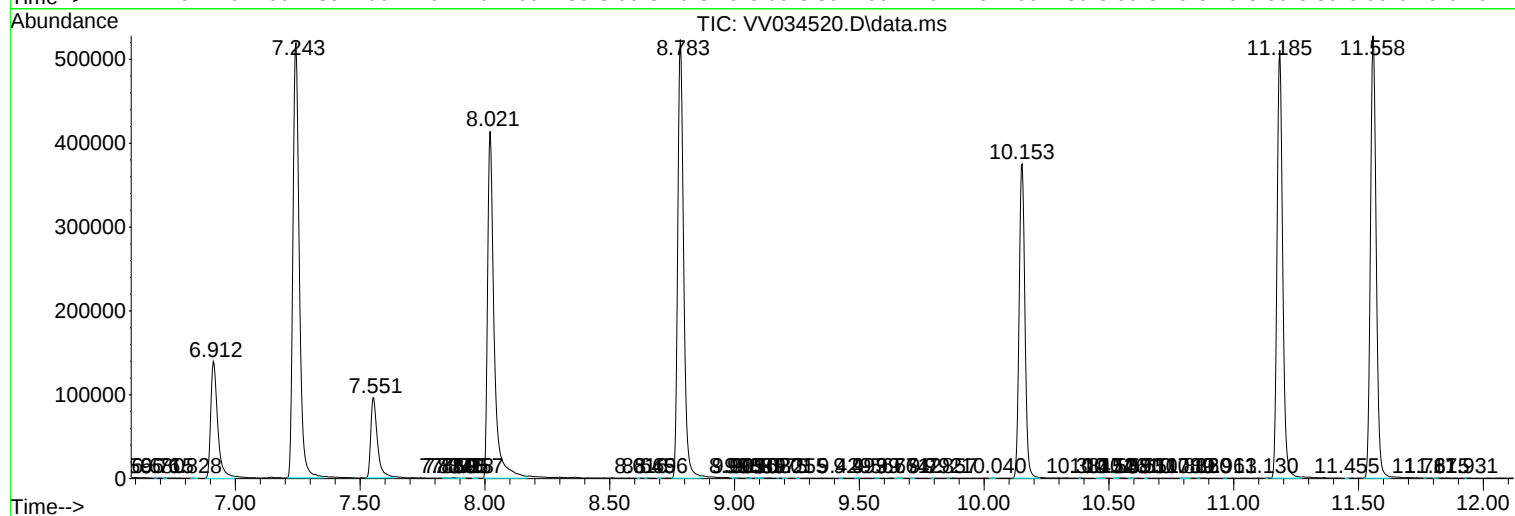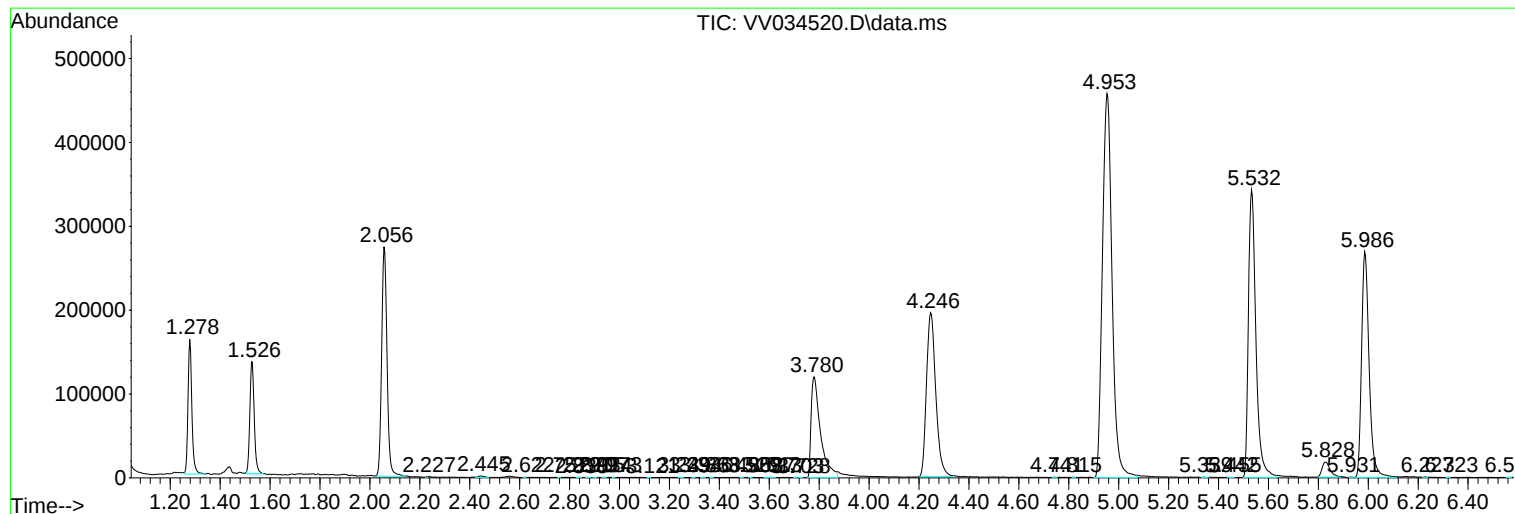

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034520.D
Acq On : 08 Mar 2024 10:26
Operator : SY/MD
Sample : P1681-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034520.D
Acq On : 08 Mar 2024 10:26
Operator : SY/MD
Sample : P1681-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc