

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034523.D
 Acq On : 08 Mar 2024 11:39
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	174615	192696	14.50%	1.886%
2	1.529	145	152	166	rVB	154268	183793	13.83%	1.799%
3	2.059	306	317	330	rBV	308966	451237	33.94%	4.416%
4	2.442	432	436	438	rBV3	1342	1151	0.09%	0.011%
5	2.545	466	468	469	rBV	346	130	0.01%	0.001%
6	2.709	517	519	521	rVB	355	111	0.01%	0.001%
7	2.767	534	537	538	rBV	124	71	0.01%	0.001%
8	2.793	544	545	546	rBV	169	56	0.00%	0.001%
9	2.854	557	564	567	rBV2	394	367	0.03%	0.004%
10	2.876	567	571	572	rBV	323	192	0.01%	0.002%
11	2.928	584	587	589	rBV2	125	74	0.01%	0.001%
12	3.005	609	611	616	rBV2	107	99	0.01%	0.001%
13	3.098	634	640	642	rBV2	175	192	0.01%	0.002%
14	3.159	655	659	662	rBV2	143	142	0.01%	0.001%
15	3.294	695	701	704	rBV2	214	274	0.02%	0.003%
16	3.333	710	713	716	rBV2	158	144	0.01%	0.001%
17	3.381	725	728	734	rBV2	147	144	0.01%	0.001%
18	3.445	745	748	752	rBV2	163	128	0.01%	0.001%
19	3.503	764	766	767	rBB2	21	16	0.00%	0.000%
20	3.580	786	790	791	rBV	281	172	0.01%	0.002%
21	3.596	792	795	798	rVV3	331	262	0.02%	0.003%
22	3.667	815	817	822	rVB2	91	55	0.00%	0.001%
23	3.690	822	824	825	rBV	25	11	0.00%	0.000%
24	3.703	825	828	831	rBV2	164	101	0.01%	0.001%
25	3.722	831	834	842	rVB	193	180	0.01%	0.002%
26	3.780	844	852	883	rBV	117934	311130	23.40%	3.045%
27	4.249	982	998	1031	rBV	219985	616723	46.39%	6.036%
28	4.458	1062	1063	1066	rBV	382	267	0.02%	0.003%
29	4.567	1093	1097	1103	rBV2	423	418	0.03%	0.004%
30	4.648	1116	1122	1124	rBV	246	275	0.02%	0.003%
31	4.709	1140	1141	1144	rBV2	162	71	0.01%	0.001%
32	4.802	1167	1170	1172	rVB	238	125	0.01%	0.001%
33	4.828	1172	1178	1179	rBV2	227	213	0.02%	0.002%
34	4.886	1194	1196	1200	rVB2	277	138	0.01%	0.001%
35	4.953	1201	1217	1252	rBV2	495890	1329363	100.00%	13.010%
36	5.384	1348	1351	1353	rBV2	339	180	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034523.D
 Acq On : 08 Mar 2024 11:39
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1432	rBV	376676	781160	58.76%	7.645%
38	5.828	1478	1489	1510	rBV2	26085	57840	4.35%	0.566%
39	5.921	1516	1518	1523	rVB	317	174	0.01%	0.002%
40	5.989	1526	1539	1569	rBV	287702	602701	45.34%	5.898%
41	6.304	1633	1637	1640	rBV4	351	385	0.03%	0.004%
42	6.352	1647	1652	1654	rBV	162	129	0.01%	0.001%
43	6.381	1658	1661	1663	rBV2	104	63	0.00%	0.001%
44	6.445	1670	1681	1692	rBV5	5573	11566	0.87%	0.113%
45	6.516	1700	1703	1705	rBV2	259	166	0.01%	0.002%
46	6.574	1719	1721	1722	rBV2	275	117	0.01%	0.001%
47	6.699	1758	1760	1761	rBV	189	69	0.01%	0.001%
48	6.783	1784	1786	1788	rBV	176	77	0.01%	0.001%
49	6.873	1812	1814	1816	rBV	182	83	0.01%	0.001%
50	6.911	1816	1826	1851	rBV	152203	290197	21.83%	2.840%
51	7.243	1918	1929	1950	rBV	568869	1005423	75.63%	9.840%
52	7.506	2007	2011	2014	rBV3	402	270	0.02%	0.003%
53	7.554	2015	2026	2063	rVV	103540	195929	14.74%	1.918%
54	7.812	2104	2106	2110	rVB2	549	201	0.02%	0.002%
55	7.831	2110	2112	2114	rBV	145	58	0.00%	0.001%
56	7.915	2130	2138	2145	rVB7	2977	4619	0.35%	0.045%
57	7.969	2153	2155	2157	rBV	142	75	0.01%	0.001%
58	8.021	2162	2171	2212	rBV	419138	757904	57.01%	7.417%
59	8.513	2320	2324	2333	rBV2	469	550	0.04%	0.005%
60	8.551	2333	2336	2338	rVV3	418	217	0.02%	0.002%
61	8.616	2354	2356	2358	rBV2	331	171	0.01%	0.002%
62	8.725	2388	2390	2393	rBV2	182	124	0.01%	0.001%
63	8.783	2397	2408	2444	rBV	571530	940618	70.76%	9.206%
64	9.159	2523	2525	2529	rBV2	151	61	0.00%	0.001%
65	9.194	2532	2536	2537	rBV	270	164	0.01%	0.002%
66	9.342	2580	2582	2587	rVB2	294	150	0.01%	0.001%
67	9.419	2604	2606	2609	rVB	212	71	0.01%	0.001%
68	9.490	2624	2628	2630	rBV3	346	259	0.02%	0.003%
69	9.535	2639	2642	2647	rBV2	566	428	0.03%	0.004%
70	9.664	2673	2682	2684	rBV2	198	243	0.02%	0.002%
71	9.709	2693	2696	2700	rBV	213	149	0.01%	0.001%
72	9.731	2700	2703	2705	rBV2	173	131	0.01%	0.001%
73	9.818	2727	2730	2732	rBV2	266	158	0.01%	0.002%
74	9.937	2764	2767	2770	rBV	249	148	0.01%	0.001%
75	9.998	2783	2786	2788	rBV	292	202	0.02%	0.002%
76	10.152	2821	2834	2860	rBV	375241	601203	45.22%	5.884%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034523.D
 Acq On : 08 Mar 2024 11:39
 Operator : SY/MD
 Sample : P1679-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0700

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.564	2960	2962	2964	rVB	218	65	0.00%	0.001%
78	10.638	2982	2985	2990	rVB2	198	176	0.01%	0.002%
79	10.664	2990	2993	2995	rBV	154	97	0.01%	0.001%
80	10.863	3053	3055	3061	rVB3	503	358	0.03%	0.004%
81	11.185	3143	3155	3179	rBV	576389	902533	67.89%	8.833%
82	11.403	3222	3223	3225	rVB	185	67	0.01%	0.001%
83	11.416	3225	3227	3229	rBV2	355	153	0.01%	0.001%
84	11.558	3258	3271	3296	rBV	604879	951322	71.56%	9.310%
85	11.763	3333	3335	3336	rBV	303	149	0.01%	0.001%
86	11.882	3370	3372	3374	rBV	286	130	0.01%	0.001%
87	12.072	3430	3431	3434	rBV	187	118	0.01%	0.001%
88	12.107	3439	3442	3443	rBV	300	182	0.01%	0.002%
89	12.734	3631	3637	3639	rBV	235	276	0.02%	0.003%
90	13.127	3756	3759	3765	rVB3	374	275	0.02%	0.003%
91	13.210	3777	3785	3798	rVB4	1489	2293	0.17%	0.022%
92	13.384	3834	3839	3845	rBV6	1334	1475	0.11%	0.014%
93	13.448	3851	3859	3877	rBV2	7557	13084	0.98%	0.128%
94	13.593	3902	3904	3906	rBV	320	182	0.01%	0.002%




Sum of corrected areas: 10217889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034523.D
Acq On : 08 Mar 2024 11:39
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

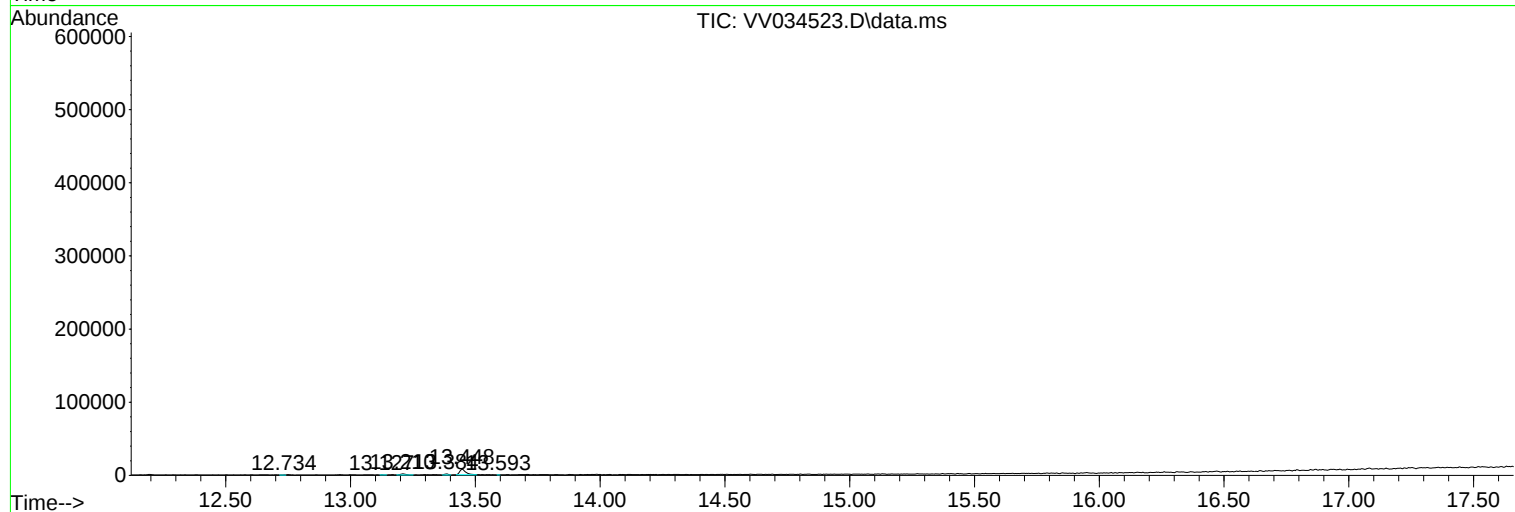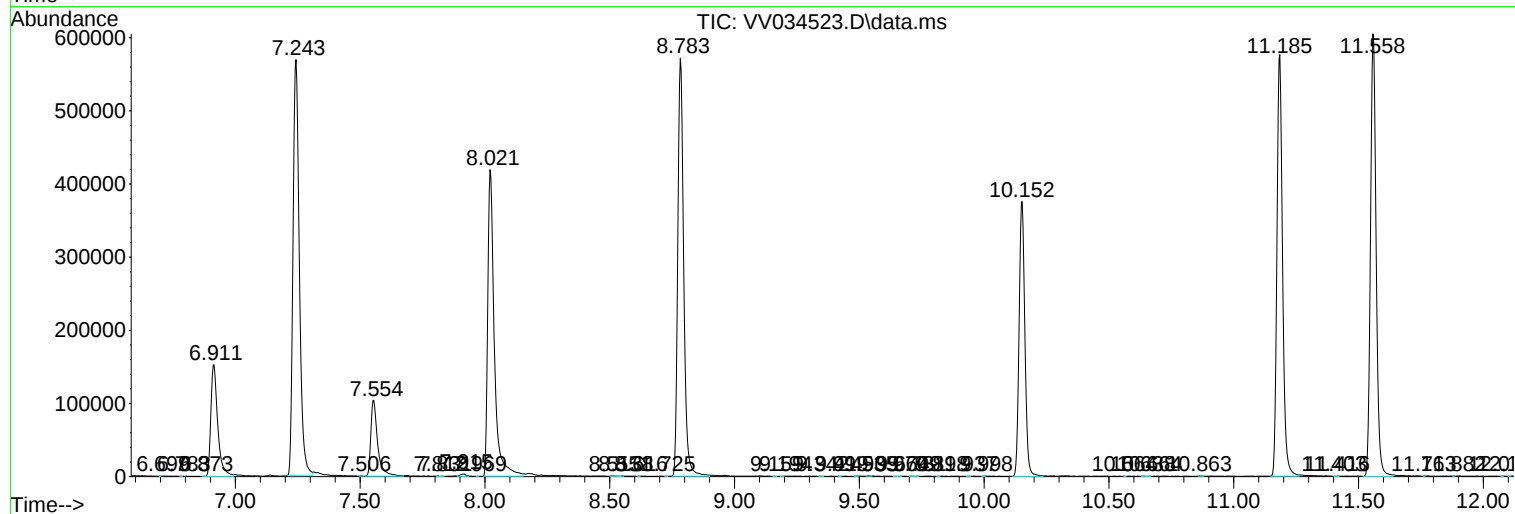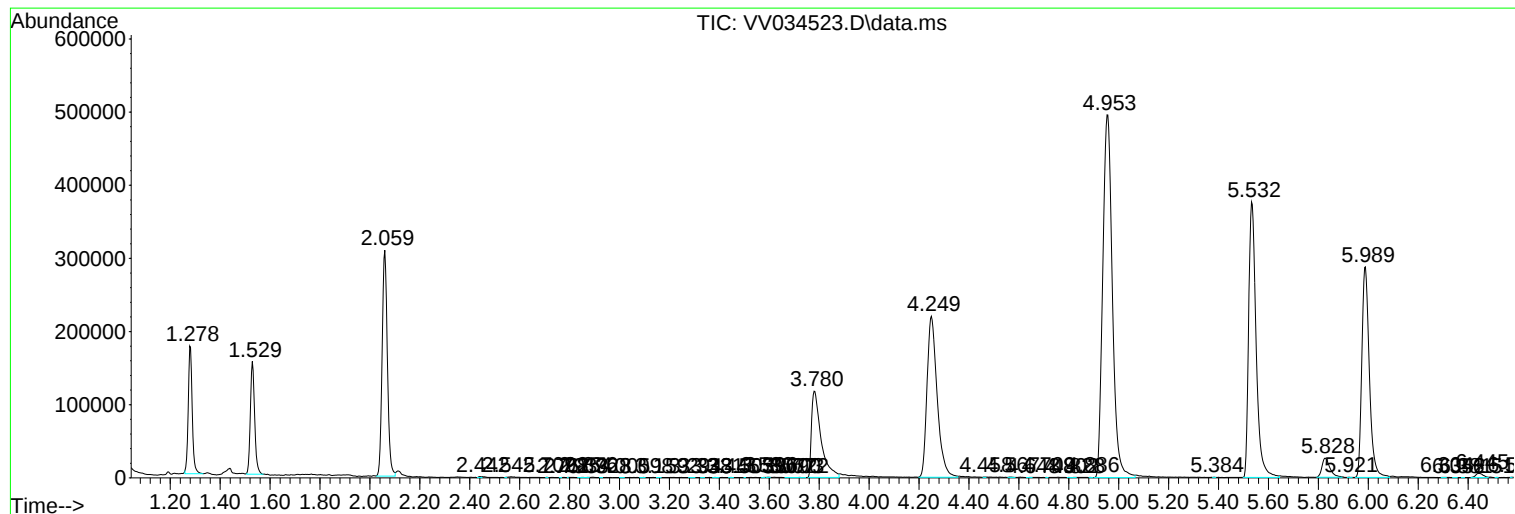

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034523.D
Acq On : 08 Mar 2024 11:39
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034523.D
Acq On : 08 Mar 2024 11:39
Operator : SY/MD
Sample : P1679-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc