

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034524.D
 Acq On : 08 Mar 2024 12:03
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	169334	177009	14.22%	1.841%
2	1.529	145	152	169	rVB	141477	176660	14.19%	1.837%
3	2.056	306	316	328	rBV	287361	419155	33.67%	4.360%
4	2.230	367	370	380	rBV4	748	917	0.07%	0.010%
5	2.825	552	555	557	rBV	193	136	0.01%	0.001%
6	2.834	557	558	559	rBV	213	53	0.00%	0.001%
7	2.879	568	572	574	rBV2	664	463	0.04%	0.005%
8	2.963	593	598	599	rBV2	203	177	0.01%	0.002%
9	3.031	616	619	620	rBV	201	111	0.01%	0.001%
10	3.121	644	647	651	rVB	227	119	0.01%	0.001%
11	3.191	667	669	672	rBV2	312	187	0.02%	0.002%
12	3.207	672	674	676	rVB2	255	65	0.01%	0.001%
13	3.262	686	691	693	rBV	189	181	0.01%	0.002%
14	3.294	697	701	702	rBV2	209	139	0.01%	0.001%
15	3.387	727	730	733	rVB2	127	88	0.01%	0.001%
16	3.416	733	739	744	rBV2	194	261	0.02%	0.003%
17	3.442	744	747	750	rBV	290	141	0.01%	0.001%
18	3.539	775	777	779	rBB	75	30	0.00%	0.000%
19	3.561	779	784	787	rVB2	134	102	0.01%	0.001%
20	3.587	787	792	795	rBV2	122	111	0.01%	0.001%
21	3.613	795	800	801	rBV2	219	163	0.01%	0.002%
22	3.658	806	814	819	rBV2	314	506	0.04%	0.005%
23	3.780	843	852	888	rBV	117781	310622	24.95%	3.231%
24	4.246	981	997	1026	rBV	204325	563604	45.27%	5.862%
25	4.455	1061	1062	1065	rBV2	405	183	0.01%	0.002%
26	4.587	1100	1103	1105	rBV3	392	246	0.02%	0.003%
27	4.686	1132	1134	1137	rBV2	253	129	0.01%	0.001%
28	4.706	1137	1140	1143	rBV	346	331	0.03%	0.003%
29	4.767	1157	1159	1160	rBV	112	26	0.00%	0.000%
30	4.796	1163	1168	1173	rBV3	312	377	0.03%	0.004%
31	4.953	1199	1217	1255	rBV2	471152	1244882	100.00%	12.948%
32	5.326	1331	1333	1335	rBV	231	107	0.01%	0.001%
33	5.355	1339	1342	1345	rVB3	418	282	0.02%	0.003%
34	5.381	1346	1350	1356	rBV3	381	383	0.03%	0.004%
35	5.452	1371	1372	1375	rVB2	299	83	0.01%	0.001%
36	5.532	1386	1397	1430	rBV	361865	746706	59.98%	7.766%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034524.D
 Acq On : 08 Mar 2024 12:03
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.828	1477	1489	1507	rBV2	24395	54116	4.35%	0.563%
38	5.985	1525	1538	1578	rBV	276036	564608	45.35%	5.872%
39	6.268	1625	1626	1629	rBV	261	168	0.01%	0.002%
40	6.323	1636	1643	1645	rBV2	227	221	0.02%	0.002%
41	6.336	1645	1647	1649	rVB	183	84	0.01%	0.001%
42	6.355	1649	1653	1655	rBV	267	175	0.01%	0.002%
43	6.439	1670	1679	1700	rVB5	6507	14102	1.13%	0.147%
44	6.587	1721	1725	1730	rBV4	713	774	0.06%	0.008%
45	6.754	1774	1777	1778	rBV2	271	180	0.01%	0.002%
46	6.789	1785	1788	1792	rVB	232	152	0.01%	0.002%
47	6.850	1804	1807	1811	rBV	184	127	0.01%	0.001%
48	6.876	1811	1815	1816	rBV2	329	151	0.01%	0.002%
49	6.911	1816	1826	1852	rBV	141586	267164	21.46%	2.779%
50	7.243	1918	1929	1954	rBV	528434	937228	75.29%	9.748%
51	7.554	2016	2026	2057	rBV	95907	177677	14.27%	1.848%
52	7.831	2110	2112	2113	rBV	184	93	0.01%	0.001%
53	7.837	2113	2114	2116	rVV2	416	172	0.01%	0.002%
54	7.866	2119	2123	2125	rBV2	374	306	0.02%	0.003%
55	7.915	2132	2138	2144	rBV4	913	1161	0.09%	0.012%
56	7.976	2154	2157	2159	rBV	345	154	0.01%	0.002%
57	8.021	2162	2171	2212	rBV	400487	731596	58.77%	7.609%
58	8.464	2305	2309	2311	rBV3	313	286	0.02%	0.003%
59	8.542	2330	2333	2337	rBV2	204	166	0.01%	0.002%
60	8.577	2341	2344	2348	rBV2	242	225	0.02%	0.002%
61	8.680	2374	2376	2377	rBV	276	128	0.01%	0.001%
62	8.715	2383	2387	2388	rBV	311	192	0.02%	0.002%
63	8.783	2397	2408	2440	rBV	542772	900545	72.34%	9.366%
64	9.082	2499	2501	2503	rVB2	420	190	0.02%	0.002%
65	9.098	2503	2506	2508	rBV	289	161	0.01%	0.002%
66	9.114	2509	2511	2514	rVB	616	335	0.03%	0.003%
67	9.226	2542	2546	2549	rBV2	246	191	0.02%	0.002%
68	9.242	2549	2551	2552	rBV2	231	79	0.01%	0.001%
69	9.323	2573	2576	2579	rBV	214	154	0.01%	0.002%
70	9.487	2624	2627	2631	rVB2	351	269	0.02%	0.003%
71	9.513	2631	2635	2638	rBV	195	193	0.02%	0.002%
72	9.529	2638	2640	2641	rBV	191	62	0.00%	0.001%
73	9.564	2647	2651	2653	rBV2	251	238	0.02%	0.002%
74	9.619	2662	2668	2669	rBV2	391	275	0.02%	0.003%
75	9.654	2676	2679	2681	rBV2	141	106	0.01%	0.001%
76	9.744	2704	2707	2709	rBV2	186	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034524.D
 Acq On : 08 Mar 2024 12:03
 Operator : SY/MD
 Sample : P1679-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.040	2797	2799	2802	rVB	189	65	0.01%	0.001%
78	10.152	2821	2834	2855	rBV	359134	570516	45.83%	5.934%
79	10.374	2901	2903	2906	rBV	222	127	0.01%	0.001%
80	10.824	3040	3043	3045	rBV	255	155	0.01%	0.002%
81	10.869	3053	3057	3060	rVB	396	316	0.03%	0.003%
82	11.185	3144	3155	3179	rBV	547590	858311	68.95%	8.927%
83	11.458	3237	3240	3245	rBV3	274	207	0.02%	0.002%
84	11.558	3260	3271	3298	rBV	550888	877933	70.52%	9.131%
85	11.786	3340	3342	3350	rVB3	372	334	0.03%	0.003%
86	11.818	3350	3352	3353	rBV	511	133	0.01%	0.001%
87	11.953	3392	3394	3395	rBV	200	78	0.01%	0.001%
88	12.037	3418	3420	3422	rVB	367	103	0.01%	0.001%
89	12.185	3462	3466	3470	rBV3	671	751	0.06%	0.008%
90	12.239	3481	3483	3489	rVB	297	239	0.02%	0.002%
91	12.268	3490	3492	3494	rBV	247	88	0.01%	0.001%
92	12.442	3544	3546	3552	rBV	233	116	0.01%	0.001%
93	12.821	3661	3664	3670	rBV3	396	331	0.03%	0.003%
94	13.210	3780	3785	3787	rBV5	1000	923	0.07%	0.010%
95	13.451	3852	3860	3870	rBV5	3237	4863	0.39%	0.051%




Sum of corrected areas: 9614642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034524.D
Acq On : 08 Mar 2024 12:03
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

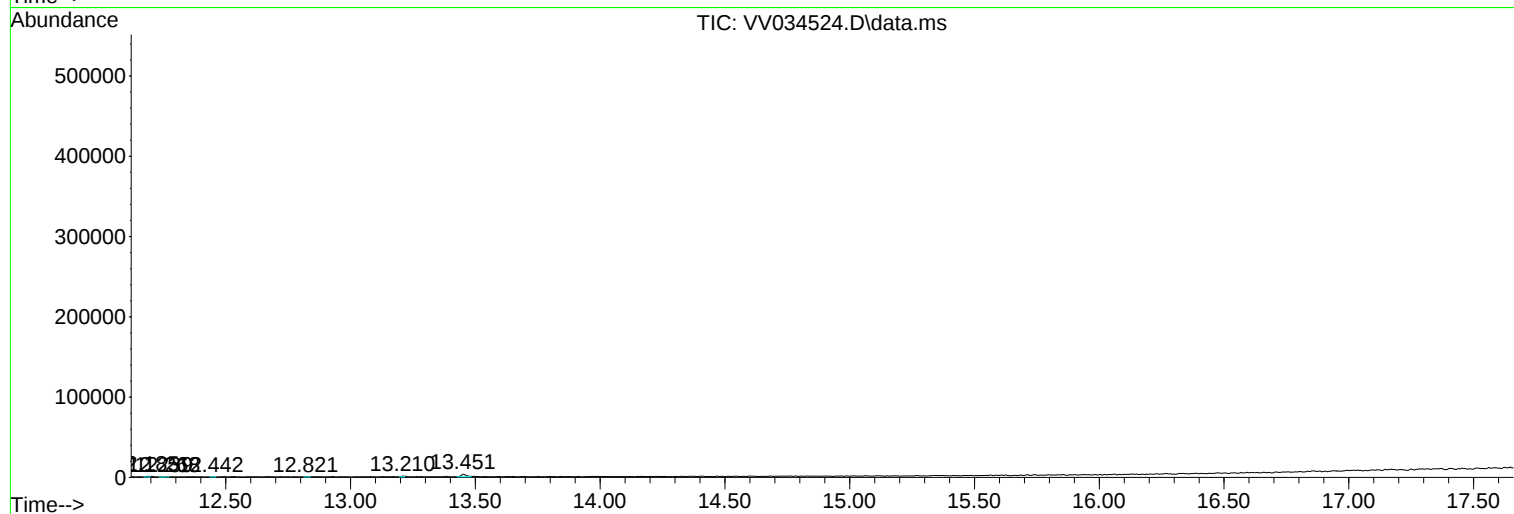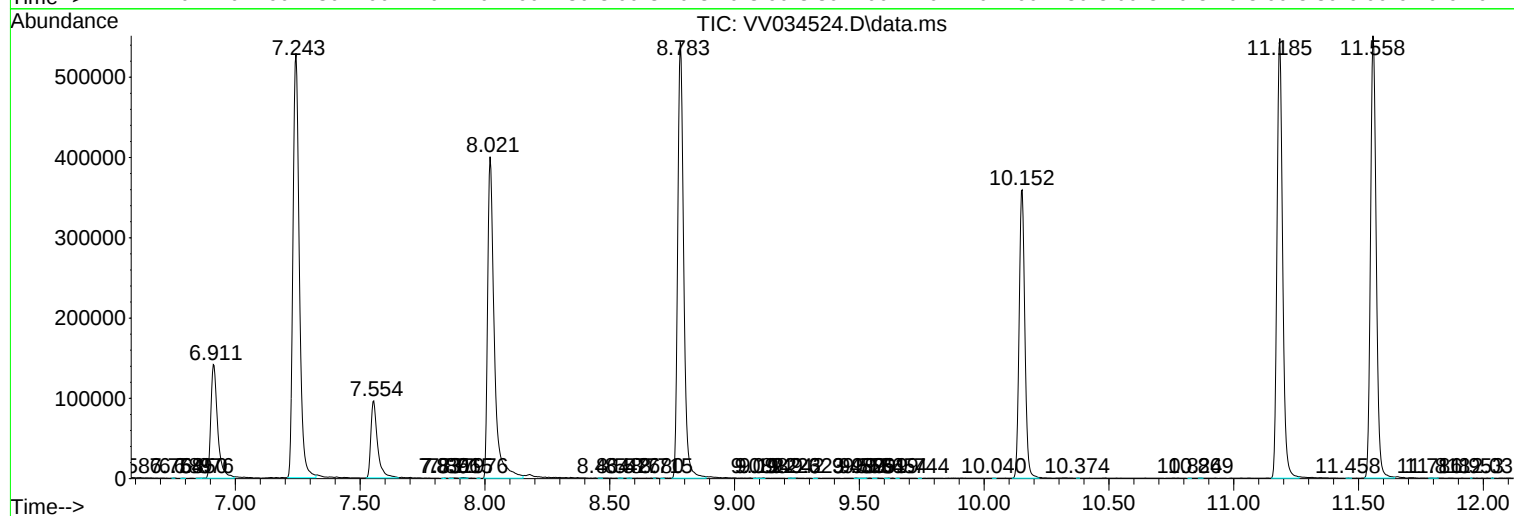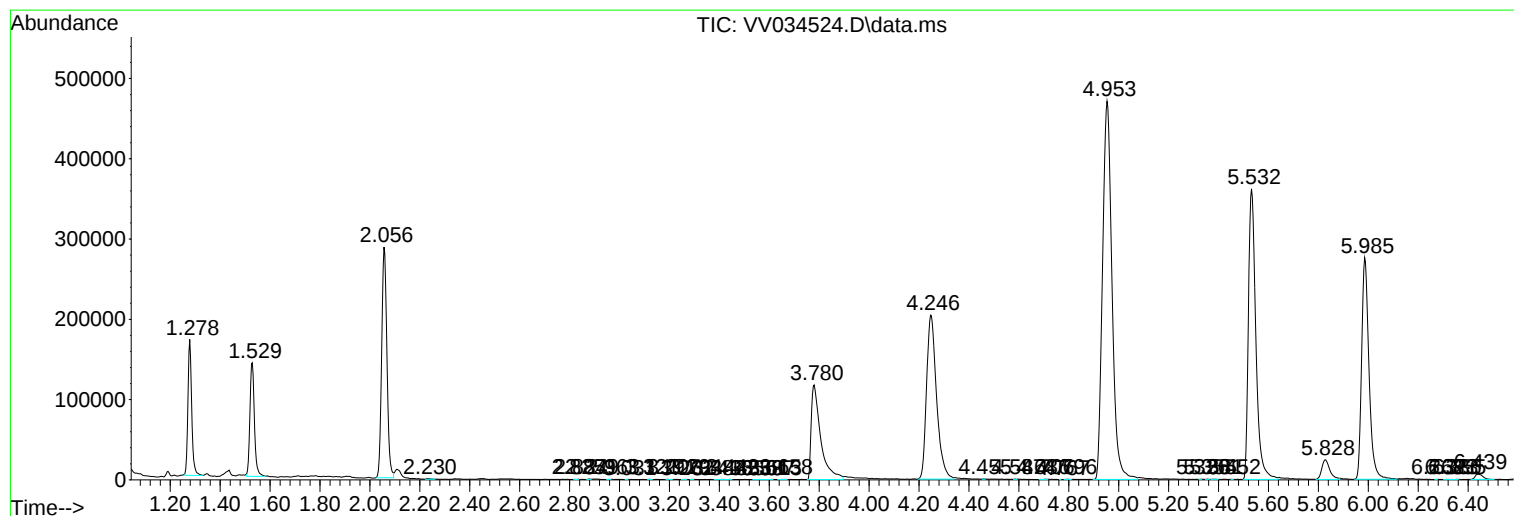

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034524.D
Acq On : 08 Mar 2024 12:03
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034524.D
Acq On : 08 Mar 2024 12:03
Operator : SY/MD
Sample : P1679-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc