

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034525.D
 Acq On : 08 Mar 2024 12:27
 Operator : SY/MD
 Sample : P1637-02 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	163832	171829	13.99%	1.816%
2	1.526	145	151	166	rVB	141140	169015	13.76%	1.786%
3	2.057	306	316	340	rBV	284273	414350	33.74%	4.380%
4	2.446	431	437	439	rBV3	1599	1591	0.13%	0.017%
5	2.558	467	472	477	rBV2	822	1030	0.08%	0.011%
6	2.825	550	555	558	rBV2	426	340	0.03%	0.004%
7	2.841	558	560	562	rBV	149	93	0.01%	0.001%
8	2.954	591	595	603	rVB2	230	305	0.02%	0.003%
9	2.995	603	608	611	rBV3	534	428	0.03%	0.005%
10	3.195	665	670	674	rVB2	246	187	0.02%	0.002%
11	3.217	674	677	682	rBV2	169	156	0.01%	0.002%
12	3.278	689	696	699	rBV2	300	295	0.02%	0.003%
13	3.298	700	702	703	rBV	174	55	0.00%	0.001%
14	3.413	735	738	741	rVB2	153	98	0.01%	0.001%
15	3.429	741	743	745	rBV	87	48	0.00%	0.001%
16	3.446	745	748	749	rBV	198	119	0.01%	0.001%
17	3.484	758	760	763	rBV	233	138	0.01%	0.001%
18	3.510	766	768	770	rBV	120	48	0.00%	0.001%
19	3.574	786	788	790	rBV	112	62	0.01%	0.001%
20	3.600	794	796	799	rBV2	119	67	0.01%	0.001%
21	3.667	810	817	818	rBV	152	145	0.01%	0.002%
22	3.696	821	826	828	rBV	206	174	0.01%	0.002%
23	3.780	843	852	892	rBV	114233	306209	24.93%	3.237%
24	4.246	980	997	1037	rBV	195238	512472	41.73%	5.417%
25	4.571	1096	1098	1099	rBV2	305	136	0.01%	0.001%
26	4.757	1151	1156	1160	rBV2	354	342	0.03%	0.004%
27	4.809	1169	1172	1176	rVB2	249	191	0.02%	0.002%
28	4.880	1191	1194	1196	rBV	212	111	0.01%	0.001%
29	4.953	1196	1217	1248	rBV3	463568	1228045	100.00%	12.980%
30	5.211	1295	1297	1300	rBV2	370	217	0.02%	0.002%
31	5.333	1334	1335	1339	rVB2	220	131	0.01%	0.001%
32	5.378	1346	1349	1356	rVB4	439	516	0.04%	0.005%
33	5.423	1356	1363	1366	rBV2	375	512	0.04%	0.005%
34	5.532	1384	1397	1424	rBV	363245	753388	61.35%	7.963%
35	5.828	1480	1489	1510	rVB3	16074	35745	2.91%	0.378%
36	5.986	1525	1538	1568	rBV	267254	561659	45.74%	5.937%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034525.D
 Acq On : 08 Mar 2024 12:27
 Operator : SY/MD
 Sample : P1637-02 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.198	1602	1604	1607	rBV3	437	298	0.02%	0.003%
38	6.265	1621	1625	1631	rVB4	425	455	0.04%	0.005%
39	6.291	1631	1633	1634	rBV	182	55	0.00%	0.001%
40	6.310	1637	1639	1644	rVB2	168	85	0.01%	0.001%
41	6.336	1644	1647	1651	rBV2	337	221	0.02%	0.002%
42	6.355	1651	1653	1656	rBV2	184	99	0.01%	0.001%
43	6.391	1660	1664	1666	rVV	374	219	0.02%	0.002%
44	6.404	1666	1668	1676	rVB2	321	268	0.02%	0.003%
45	6.442	1677	1680	1681	rBV	136	66	0.01%	0.001%
46	6.516	1699	1703	1707	rBV2	194	173	0.01%	0.002%
47	6.812	1793	1795	1797	rVB	280	117	0.01%	0.001%
48	6.834	1797	1802	1804	rBV2	128	137	0.01%	0.001%
49	6.851	1805	1807	1811	rVV2	163	97	0.01%	0.001%
50	6.912	1816	1826	1855	rBV	140797	266204	21.68%	2.814%
51	7.243	1918	1929	1955	rBV	534988	933517	76.02%	9.867%
52	7.551	2016	2025	2054	rBV	94833	176645	14.38%	1.867%
53	7.770	2090	2093	2096	rBV2	364	270	0.02%	0.003%
54	7.812	2101	2106	2108	rBV	305	248	0.02%	0.003%
55	7.825	2108	2110	2115	rVB	272	181	0.01%	0.002%
56	7.857	2116	2120	2122	rBV2	371	305	0.02%	0.003%
57	7.912	2131	2137	2151	rVB5	1945	2757	0.22%	0.029%
58	7.963	2151	2153	2156	rVB2	183	81	0.01%	0.001%
59	8.021	2162	2171	2204	rBV	407239	718575	58.51%	7.595%
60	8.545	2332	2334	2336	rBV	255	116	0.01%	0.001%
61	8.783	2397	2408	2443	rBV	551928	907665	73.91%	9.594%
62	9.008	2476	2478	2479	rBV	215	81	0.01%	0.001%
63	9.108	2505	2509	2511	rVB3	321	216	0.02%	0.002%
64	9.252	2552	2554	2557	rVB2	265	95	0.01%	0.001%
65	9.313	2570	2573	2574	rBV	136	70	0.01%	0.001%
66	9.342	2579	2582	2584	rBV	191	115	0.01%	0.001%
67	9.500	2627	2631	2633	rBV2	245	176	0.01%	0.002%
68	9.545	2642	2645	2648	rBV	216	129	0.01%	0.001%
69	9.564	2648	2651	2654	rBV2	310	148	0.01%	0.002%
70	9.593	2657	2660	2662	rBV2	140	86	0.01%	0.001%
71	9.641	2673	2675	2678	rBV2	194	85	0.01%	0.001%
72	9.793	2718	2722	2725	rVB	230	176	0.01%	0.002%
73	9.847	2732	2739	2740	rBV	249	285	0.02%	0.003%
74	9.886	2747	2751	2754	rBV2	364	190	0.02%	0.002%
75	10.095	2813	2816	2820	rVB2	224	161	0.01%	0.002%
76	10.153	2821	2834	2857	rBV	371728	588912	47.96%	6.225%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034525.D
 Acq On : 08 Mar 2024 12:27
 Operator : SY/MD
 Sample : P1637-02 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.400	2908	2911	2913	rBV	424	236	0.02%	0.002%
78	10.519	2945	2948	2953	rBV2	202	163	0.01%	0.002%
79	10.564	2960	2962	2964	rVB2	349	138	0.01%	0.001%
80	10.587	2964	2969	2973	rBV2	261	242	0.02%	0.003%
81	10.674	2993	2996	2998	rBV	223	172	0.01%	0.002%
82	10.712	3005	3008	3013	rBV	302	298	0.02%	0.003%
83	10.747	3017	3019	3021	rBV	251	115	0.01%	0.001%
84	10.796	3031	3034	3036	rBV2	243	119	0.01%	0.001%
85	11.059	3111	3116	3118	rBV	243	233	0.02%	0.002%
86	11.130	3136	3138	3143	rBV2	342	261	0.02%	0.003%
87	11.185	3143	3155	3177	rBV	534102	845944	68.89%	8.941%
88	11.416	3222	3227	3229	rBV2	477	377	0.03%	0.004%
89	11.558	3259	3271	3297	rBV	530512	850740	69.28%	8.992%
90	11.786	3338	3342	3347	rBV2	439	358	0.03%	0.004%
91	11.809	3347	3349	3352	rVB2	323	114	0.01%	0.001%
92	11.825	3352	3354	3358	rBV	253	190	0.02%	0.002%
93	11.992	3404	3406	3409	rBV	156	90	0.01%	0.001%
94	12.288	3496	3498	3499	rBV	264	74	0.01%	0.001%
95	12.802	3656	3658	3660	rBV2	254	86	0.01%	0.001%
96	12.982	3712	3714	3716	rBV	240	131	0.01%	0.001%
97	13.320	3817	3819	3824	rVB3	378	199	0.02%	0.002%
98	13.384	3838	3839	3843	rBV2	424	181	0.01%	0.002%
99	13.439	3853	3856	3857	rBV2	439	234	0.02%	0.002%
100	13.783	3961	3963	3965	rBV2	420	211	0.02%	0.002%




Sum of corrected areas: 9460932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034525.D
Acq On : 08 Mar 2024 12:27
Operator : SY/MD
Sample : P1637-02 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

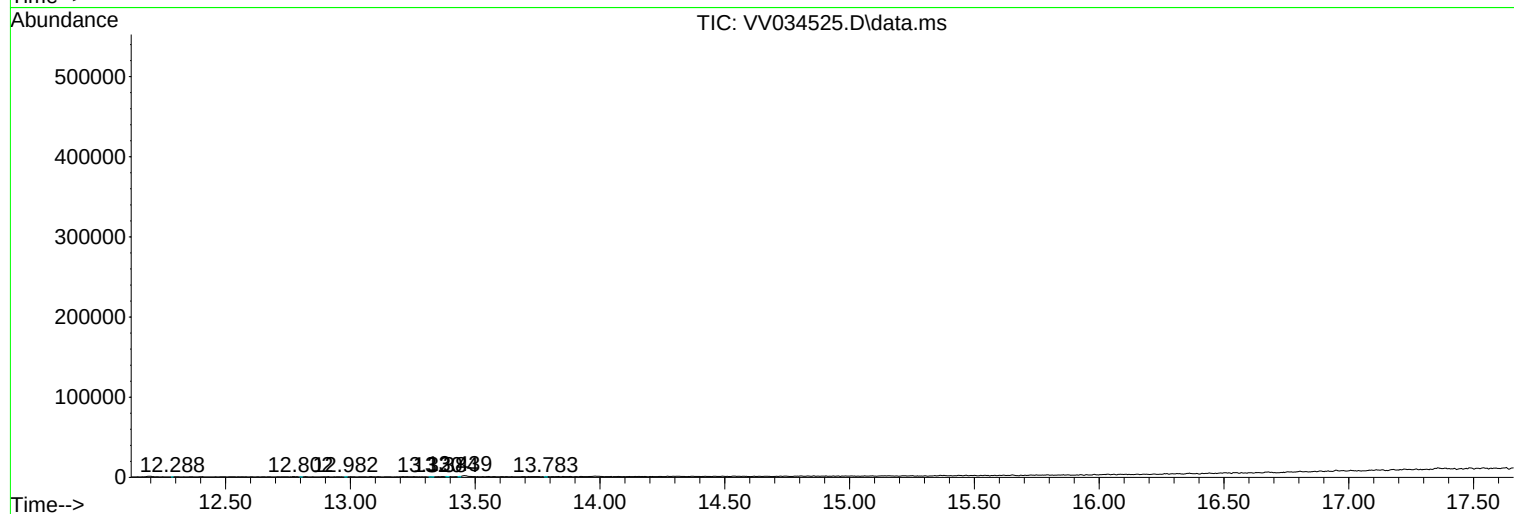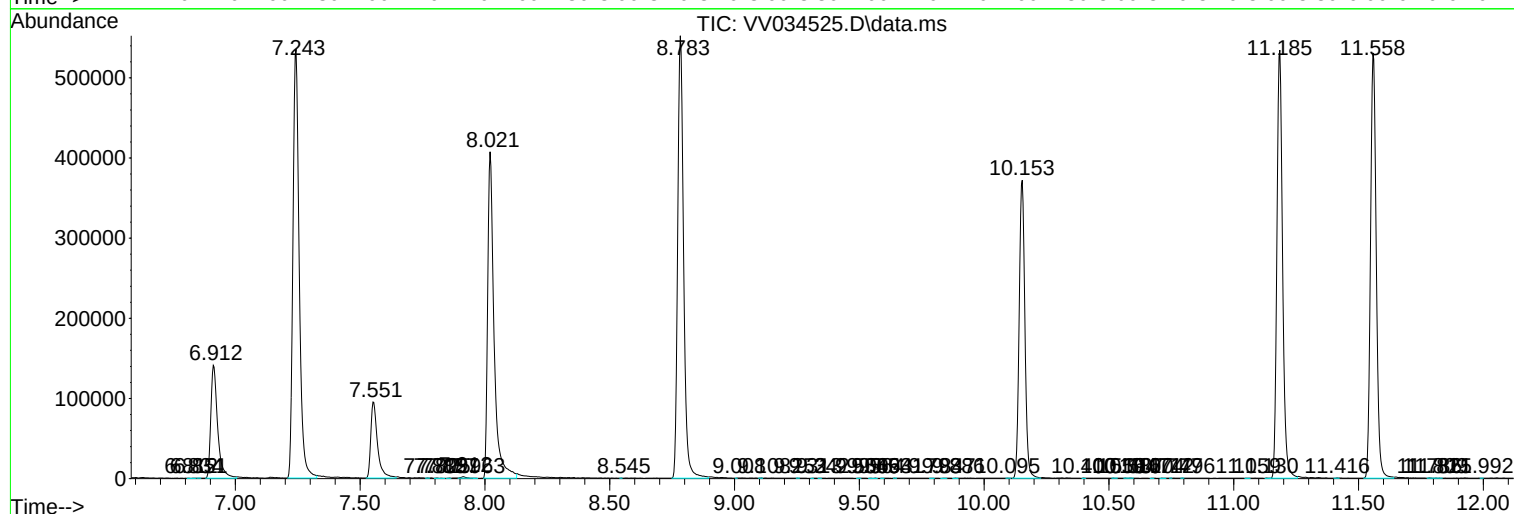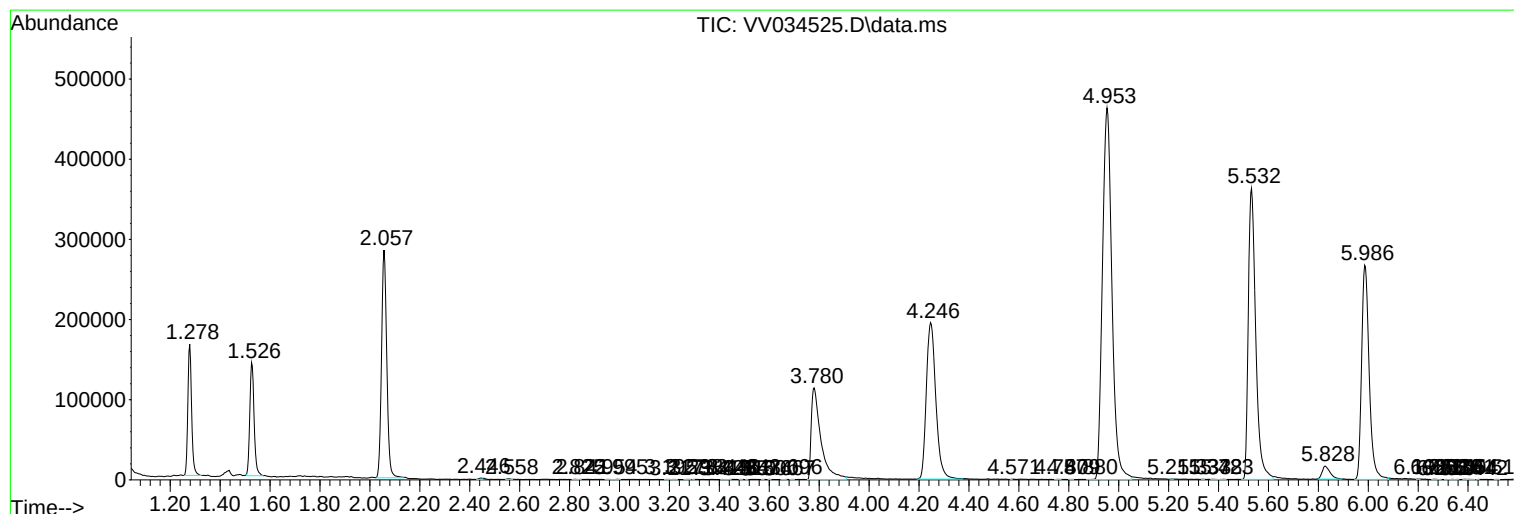

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034525.D
Acq On : 08 Mar 2024 12:27
Operator : SY/MD
Sample : P1637-02 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034525.D
Acq On : 08 Mar 2024 12:27
Operator : SY/MD
Sample : P1637-02 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc