

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034526.D
 Acq On : 08 Mar 2024 13:03
 Operator : SY/MD
 Sample : P1637-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	174427	179269	14.13%	1.669%
2	1.526	143	151	168	rVB	146312	180533	14.23%	1.681%
3	1.966	286	288	290	rBV3	1048	646	0.05%	0.006%
4	2.056	305	316	330	rBV	293853	426954	33.66%	3.975%
5	2.224	364	368	379	rVB6	1654	2385	0.19%	0.022%
6	2.320	396	398	403	rBV2	363	219	0.02%	0.002%
7	2.346	403	406	410	rVV2	291	196	0.02%	0.002%
8	2.413	424	427	430	rBV	433	378	0.03%	0.004%
9	2.445	430	437	446	rVV4	2947	4721	0.37%	0.044%
10	2.558	458	472	483	rBV5	1425	3363	0.27%	0.031%
11	2.674	500	508	510	rBV2	260	344	0.03%	0.003%
12	3.092	635	638	643	rBV	328	208	0.02%	0.002%
13	3.185	665	667	672	rVB	256	186	0.01%	0.002%
14	3.230	677	681	683	rBV2	379	201	0.02%	0.002%
15	3.439	743	746	755	rVB2	241	274	0.02%	0.003%
16	3.519	765	771	773	rBV2	313	367	0.03%	0.003%
17	3.722	831	834	838	rVB	266	210	0.02%	0.002%
18	3.777	843	851	889	rBV	107784	291938	23.02%	2.718%
19	4.127	956	960	964	rVB4	406	351	0.03%	0.003%
20	4.156	966	969	970	rBV2	465	214	0.02%	0.002%
21	4.243	979	996	1029	rBV2	204920	529772	41.77%	4.933%
22	4.764	1155	1158	1161	rVB	310	196	0.02%	0.002%
23	4.873	1188	1192	1193	rBV2	323	222	0.02%	0.002%
24	4.950	1199	1216	1242	rBV2	478501	1268360	100.00%	11.810%
25	5.333	1333	1335	1337	rBV2	543	289	0.02%	0.003%
26	5.394	1352	1354	1361	rVB3	336	373	0.03%	0.003%
27	5.423	1361	1363	1367	rBV	424	294	0.02%	0.003%
28	5.445	1367	1370	1377	rVB3	281	291	0.02%	0.003%
29	5.481	1377	1381	1385	rBV3	383	444	0.04%	0.004%
30	5.529	1385	1396	1429	rBV	393167	813199	64.11%	7.572%
31	5.828	1478	1489	1504	rBV2	16621	37589	2.96%	0.350%
32	5.986	1525	1538	1574	rBV	280477	581808	45.87%	5.417%
33	6.211	1606	1608	1615	rVB5	609	457	0.04%	0.004%
34	6.236	1615	1616	1621	rVB3	342	248	0.02%	0.002%
35	6.262	1621	1624	1631	rBV2	355	310	0.02%	0.003%
36	6.326	1640	1644	1646	rVB2	280	192	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034526.D
 Acq On : 08 Mar 2024 13:03
 Operator : SY/MD
 Sample : P1637-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.413	1668	1671	1675	rVV2	221	216	0.02%	0.002%
38	6.600	1719	1729	1736	rBV3	1126	2128	0.17%	0.020%
39	6.670	1748	1751	1757	rVB4	414	296	0.02%	0.003%
40	6.912	1815	1826	1856	rBV	147370	280999	22.15%	2.616%
41	7.143	1890	1898	1907	rBV5	1304	2397	0.19%	0.022%
42	7.191	1910	1913	1916	rBV3	345	223	0.02%	0.002%
43	7.239	1916	1928	1957	rBV	546928	967038	76.24%	9.004%
44	7.551	2014	2025	2045	rBV	100202	184469	14.54%	1.718%
45	7.770	2091	2093	2097	rVB2	707	400	0.03%	0.004%
46	7.838	2110	2114	2116	rBV2	408	263	0.02%	0.002%
47	7.902	2119	2134	2157	rBV	522945	881681	69.51%	8.209%
48	8.021	2162	2171	2211	rVV	381240	677854	53.44%	6.311%
49	8.606	2351	2353	2357	rVB2	388	217	0.02%	0.002%
50	8.635	2357	2362	2367	rBV2	372	394	0.03%	0.004%
51	8.664	2368	2371	2377	rBV2	329	282	0.02%	0.003%
52	8.783	2396	2408	2443	rBV	594050	974497	76.83%	9.073%
53	9.008	2474	2478	2480	rBV2	360	271	0.02%	0.003%
54	9.082	2498	2501	2504	rVB2	499	330	0.03%	0.003%
55	9.101	2504	2507	2509	rBV	249	185	0.01%	0.002%
56	9.378	2589	2593	2596	rBV	264	177	0.01%	0.002%
57	9.407	2599	2602	2606	rBV2	308	253	0.02%	0.002%
58	9.500	2628	2631	2634	rVB2	378	225	0.02%	0.002%
59	9.641	2673	2675	2679	rVB2	338	184	0.01%	0.002%
60	9.799	2719	2724	2727	rBV	272	283	0.02%	0.003%
61	9.886	2749	2751	2756	rVB3	387	280	0.02%	0.003%
62	10.149	2822	2833	2854	rBV	372954	591786	46.66%	5.510%
63	10.284	2873	2875	2880	rVB3	380	245	0.02%	0.002%
64	10.323	2880	2887	2895	rBV5	1531	2204	0.17%	0.021%
65	10.776	3023	3028	3032	rBV2	188	240	0.02%	0.002%
66	10.825	3040	3043	3046	rVB	298	192	0.02%	0.002%
67	10.876	3054	3059	3063	rBV2	257	291	0.02%	0.003%
68	10.911	3066	3070	3073	rBV2	210	199	0.02%	0.002%
69	11.185	3143	3155	3178	rBV	595842	928710	73.22%	8.647%
70	11.513	3253	3257	3259	rBV2	261	196	0.02%	0.002%
71	11.558	3259	3271	3294	rBV	572396	903412	71.23%	8.412%
72	11.715	3317	3320	3325	rVB4	664	488	0.04%	0.005%
73	12.001	3406	3409	3413	rVB3	349	256	0.02%	0.002%
74	12.146	3451	3454	3458	rVB2	335	179	0.01%	0.002%
75	12.381	3523	3527	3532	rVB3	326	287	0.02%	0.003%
76	12.452	3545	3549	3554	rBV2	319	301	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034526.D
 Acq On : 08 Mar 2024 13:03
 Operator : SY/MD
 Sample : P1637-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCNR2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.644	3607	3609	3613	rVB2	280	175	0.01%	0.002%
78	12.805	3657	3659	3663	rVB2	363	183	0.01%	0.002%
79	13.107	3750	3753	3757	rBV2	338	236	0.02%	0.002%
80	13.220	3786	3788	3790	rBV2	477	212	0.02%	0.002%
81	13.281	3804	3807	3813	rBV	270	218	0.02%	0.002%
82	13.368	3832	3834	3839	rBV2	312	254	0.02%	0.002%
83	13.648	3919	3921	3924	rBV2	461	203	0.02%	0.002%
84	13.776	3959	3961	3965	rBV2	275	188	0.01%	0.002%
85	13.860	3985	3987	3992	rBV2	384	277	0.02%	0.003%
86	13.898	3997	3999	4002	rVV2	577	377	0.03%	0.004%
87	13.921	4004	4006	4010	rVB2	419	265	0.02%	0.002%
88	14.149	4074	4077	4078	rBV2	416	283	0.02%	0.003%
89	14.413	4156	4159	4162	rBV2	381	288	0.02%	0.003%
90	14.432	4163	4165	4168	rVB	459	253	0.02%	0.002%
91	14.503	4185	4187	4189	rBV2	408	191	0.02%	0.002%
92	14.577	4208	4210	4211	rBV	446	179	0.01%	0.002%
93	14.603	4215	4218	4225	rVV4	576	742	0.06%	0.007%
94	14.676	4238	4241	4245	rBV2	680	541	0.04%	0.005%
95	14.750	4261	4264	4265	rBV	400	254	0.02%	0.002%
96	14.882	4301	4305	4308	rBV4	712	713	0.06%	0.007%
97	15.027	4347	4350	4352	rBV2	566	480	0.04%	0.004%
98	15.226	4409	4412	4414	rBV3	1022	668	0.05%	0.006%
99	15.522	4502	4504	4513	rVB4	773	927	0.07%	0.009%
100	15.654	4542	4545	4547	rBV3	841	461	0.04%	0.004%

Sum of corrected areas: 10740097




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034526.D
Acq On : 08 Mar 2024 13:03
Operator : SY/MD
Sample : P1637-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

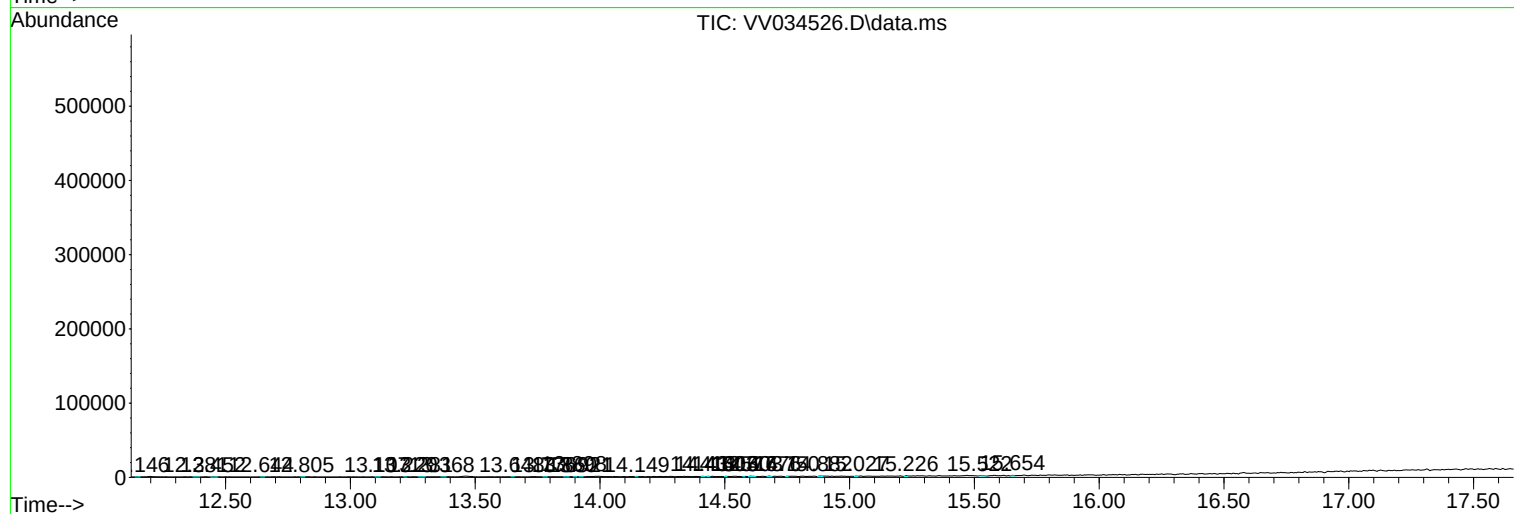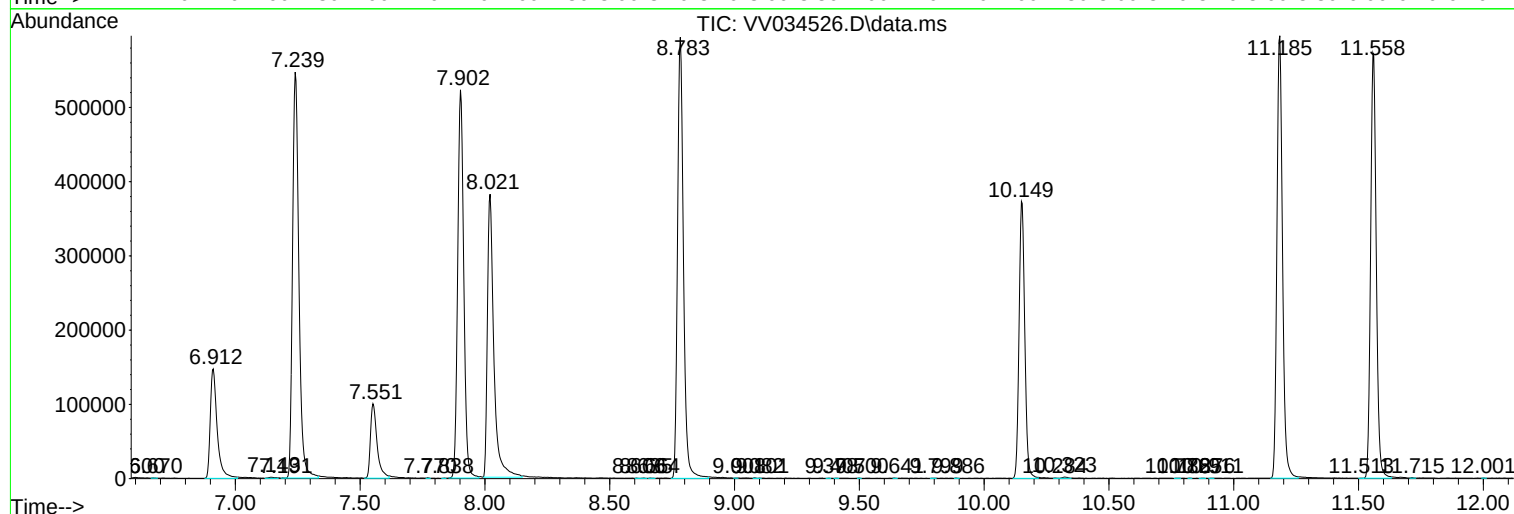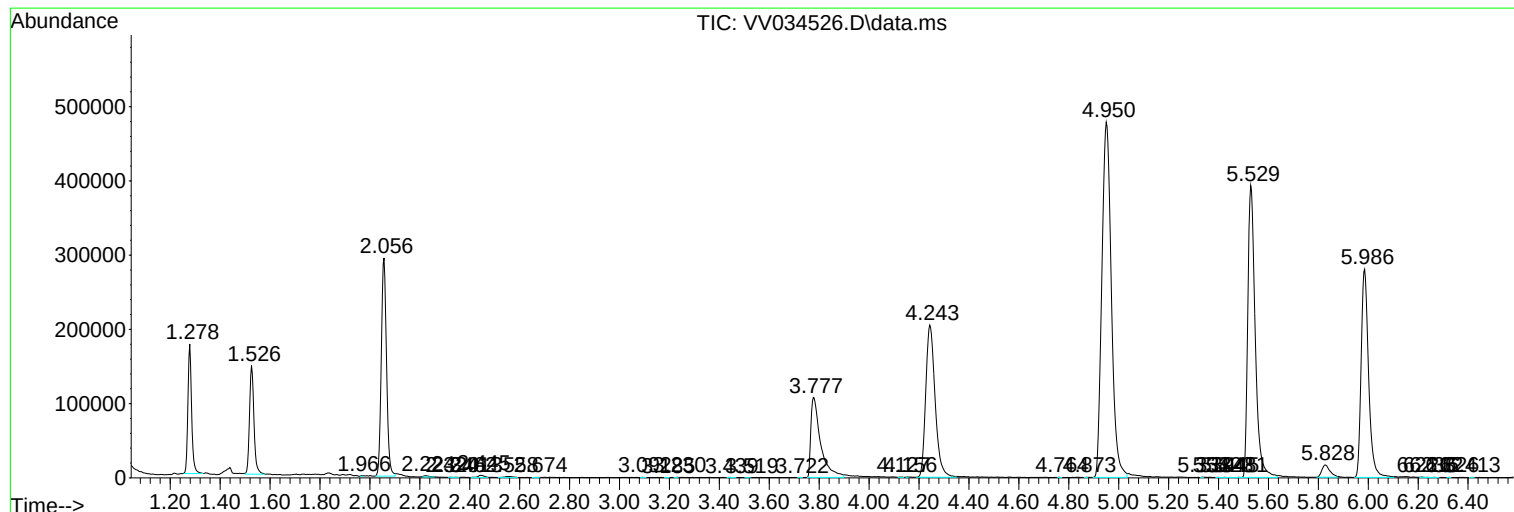

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034526.D
Acq On : 08 Mar 2024 13:03
Operator : SY/MD
Sample : P1637-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034526.D
Acq On : 08 Mar 2024 13:03
Operator : SY/MD
Sample : P1637-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCNR2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc