

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034527.D
 Acq On : 08 Mar 2024 13:27
 Operator : SY/MD
 Sample : P1679-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	164630	169481	13.75%	1.801%
2	1.526	144	151	170	rVB	137229	170362	13.82%	1.810%
3	2.056	306	316	331	rBV	278027	401764	32.60%	4.269%
4	2.400	419	423	424	rBV	290	185	0.02%	0.002%
5	2.449	430	438	450	rVB4	2556	4212	0.34%	0.045%
6	2.542	462	467	469	rBV2	365	236	0.02%	0.003%
7	2.555	469	471	472	rBV	403	190	0.02%	0.002%
8	2.603	484	486	487	rBV	237	102	0.01%	0.001%
9	2.683	508	511	513	rBV2	167	92	0.01%	0.001%
10	2.693	513	514	516	rBV2	217	86	0.01%	0.001%
11	2.802	546	548	550	rBV	124	55	0.00%	0.001%
12	2.825	551	555	561	rVB2	197	157	0.01%	0.002%
13	2.937	586	590	593	rBV2	142	128	0.01%	0.001%
14	2.973	598	601	603	rBV	217	117	0.01%	0.001%
15	3.092	636	638	639	rBV	143	63	0.01%	0.001%
16	3.201	670	672	675	rBV	106	56	0.00%	0.001%
17	3.217	675	677	679	rVB	188	57	0.00%	0.001%
18	3.240	679	684	687	rBV2	191	165	0.01%	0.002%
19	3.394	728	732	733	rBV	201	137	0.01%	0.001%
20	3.510	765	768	771	rBV2	139	99	0.01%	0.001%
21	3.542	775	778	780	rVV2	156	99	0.01%	0.001%
22	3.558	780	783	788	rVB2	213	161	0.01%	0.002%
23	3.687	819	823	825	rBV2	118	86	0.01%	0.001%
24	3.703	825	828	831	rVB2	191	119	0.01%	0.001%
25	3.722	831	834	836	rBV	139	86	0.01%	0.001%
26	3.780	843	852	897	rBV2	118294	316718	25.70%	3.366%
27	4.246	980	997	1025	rBV	197593	511609	41.51%	5.436%
28	4.799	1167	1169	1172	rBV	312	200	0.02%	0.002%
29	4.857	1184	1187	1190	rBV2	335	286	0.02%	0.003%
30	4.953	1200	1217	1252	rBV2	461147	1232426	100.00%	13.096%
31	5.262	1308	1313	1315	rBV2	303	246	0.02%	0.003%
32	5.371	1345	1347	1350	rBV	150	77	0.01%	0.001%
33	5.394	1350	1354	1356	rVV3	409	342	0.03%	0.004%
34	5.423	1360	1363	1366	rBV2	244	204	0.02%	0.002%
35	5.532	1386	1397	1431	rBV	368017	757196	61.44%	8.046%
36	5.828	1479	1489	1510	rBV4	16307	35421	2.87%	0.376%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034527.D
 Acq On : 08 Mar 2024 13:27
 Operator : SY/MD
 Sample : P1679-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.937	1521	1523	1525	rBV	224	116	0.01%	0.001%
38	5.986	1525	1538	1568	rBV2	273578	565639	45.90%	6.011%
39	6.204	1604	1606	1607	rBV3	452	185	0.02%	0.002%
40	6.323	1640	1643	1644	rBV	174	72	0.01%	0.001%
41	6.336	1644	1647	1649	rVV	286	132	0.01%	0.001%
42	6.368	1652	1657	1658	rBV2	261	227	0.02%	0.002%
43	6.410	1667	1670	1672	rBV	101	57	0.00%	0.001%
44	6.458	1682	1685	1687	rBV2	152	93	0.01%	0.001%
45	6.587	1719	1725	1727	rBV2	768	775	0.06%	0.008%
46	6.748	1773	1775	1777	rBV2	264	162	0.01%	0.002%
47	6.789	1787	1788	1790	rBV	194	78	0.01%	0.001%
48	6.805	1790	1793	1799	rVB2	212	191	0.02%	0.002%
49	6.912	1816	1826	1852	rBV	137101	258567	20.98%	2.748%
50	7.243	1918	1929	1954	rBV	501945	903724	73.33%	9.603%
51	7.555	2016	2026	2050	rBV	90734	169508	13.75%	1.801%
52	7.822	2108	2109	2112	rBV2	146	76	0.01%	0.001%
53	7.857	2118	2120	2121	rBV2	171	91	0.01%	0.001%
54	7.899	2131	2133	2134	rBV	474	177	0.01%	0.002%
55	8.021	2162	2171	2216	rBV	402509	727745	59.05%	7.733%
56	8.648	2364	2366	2367	rBV	190	87	0.01%	0.001%
57	8.738	2392	2394	2396	rBV	156	95	0.01%	0.001%
58	8.783	2397	2408	2440	rBV	545113	888578	72.10%	9.442%
59	9.098	2505	2506	2509	rVB	333	164	0.01%	0.002%
60	9.114	2509	2511	2514	rVB	195	75	0.01%	0.001%
61	9.143	2517	2520	2523	rVV	209	110	0.01%	0.001%
62	9.178	2529	2531	2535	rBV2	179	96	0.01%	0.001%
63	9.214	2539	2542	2544	rBV3	185	107	0.01%	0.001%
64	9.249	2549	2553	2558	rVB3	273	200	0.02%	0.002%
65	9.329	2574	2578	2587	rVB	339	424	0.03%	0.005%
66	9.365	2587	2589	2592	rBV	180	71	0.01%	0.001%
67	9.387	2593	2596	2597	rBV2	162	95	0.01%	0.001%
68	9.510	2631	2634	2636	rBV2	397	176	0.01%	0.002%
69	9.526	2637	2639	2643	rVB2	386	229	0.02%	0.002%
70	9.564	2646	2651	2654	rBV2	318	271	0.02%	0.003%
71	9.596	2658	2661	2664	rBV2	283	164	0.01%	0.002%
72	9.670	2681	2684	2686	rBV	191	105	0.01%	0.001%
73	9.767	2711	2714	2716	rBV	150	91	0.01%	0.001%
74	9.876	2745	2748	2755	rVB3	264	257	0.02%	0.003%
75	9.931	2763	2765	2766	rBV	267	75	0.01%	0.001%
76	9.973	2775	2778	2781	rBV2	174	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
 Data File : VV034527.D
 Acq On : 08 Mar 2024 13:27
 Operator : SY/MD
 Sample : P1679-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.072	2806	2809	2810	rBV	145	75	0.01%	0.001%
78	10.153	2821	2834	2859	rBV	367837	588487	47.75%	6.253%
79	10.317	2882	2885	2886	rBV	599	343	0.03%	0.004%
80	10.616	2973	2978	2983	rBV2	283	389	0.03%	0.004%
81	10.747	3016	3019	3022	rBV	228	180	0.01%	0.002%
82	10.844	3046	3049	3051	rBV	267	150	0.01%	0.002%
83	10.876	3056	3059	3066	rBV	356	430	0.03%	0.005%
84	11.008	3097	3100	3103	rBV	245	173	0.01%	0.002%
85	11.050	3110	3113	3117	rBV	381	331	0.03%	0.004%
86	11.095	3122	3127	3132	rBV2	396	426	0.03%	0.005%
87	11.185	3144	3155	3182	rBV	542914	843002	68.40%	8.958%
88	11.558	3259	3271	3297	rBV	529639	851491	69.09%	9.048%
89	11.789	3339	3343	3346	rBV2	376	331	0.03%	0.004%
90	12.226	3478	3479	3480	rBV	181	53	0.00%	0.001%
91	12.355	3515	3519	3522	rBV2	410	376	0.03%	0.004%
92	12.751	3638	3642	3644	rBV	277	200	0.02%	0.002%
93	12.963	3704	3708	3710	rBV	255	214	0.02%	0.002%
94	13.104	3750	3752	3756	rBV2	349	216	0.02%	0.002%
95	13.265	3799	3802	3805	rBV2	326	229	0.02%	0.002%
96	13.384	3835	3839	3842	rBV2	364	297	0.02%	0.003%
97	13.445	3855	3858	3859	rBV	423	221	0.02%	0.002%
98	13.638	3915	3918	3921	rBV2	419	285	0.02%	0.003%
99	13.882	3992	3994	3997	rBV2	472	285	0.02%	0.003%
100	13.953	4014	4016	4019	rBV3	409	283	0.02%	0.003%




Sum of corrected areas: 9410711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034527.D
Acq On : 08 Mar 2024 13:27
Operator : SY/MD
Sample : P1679-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

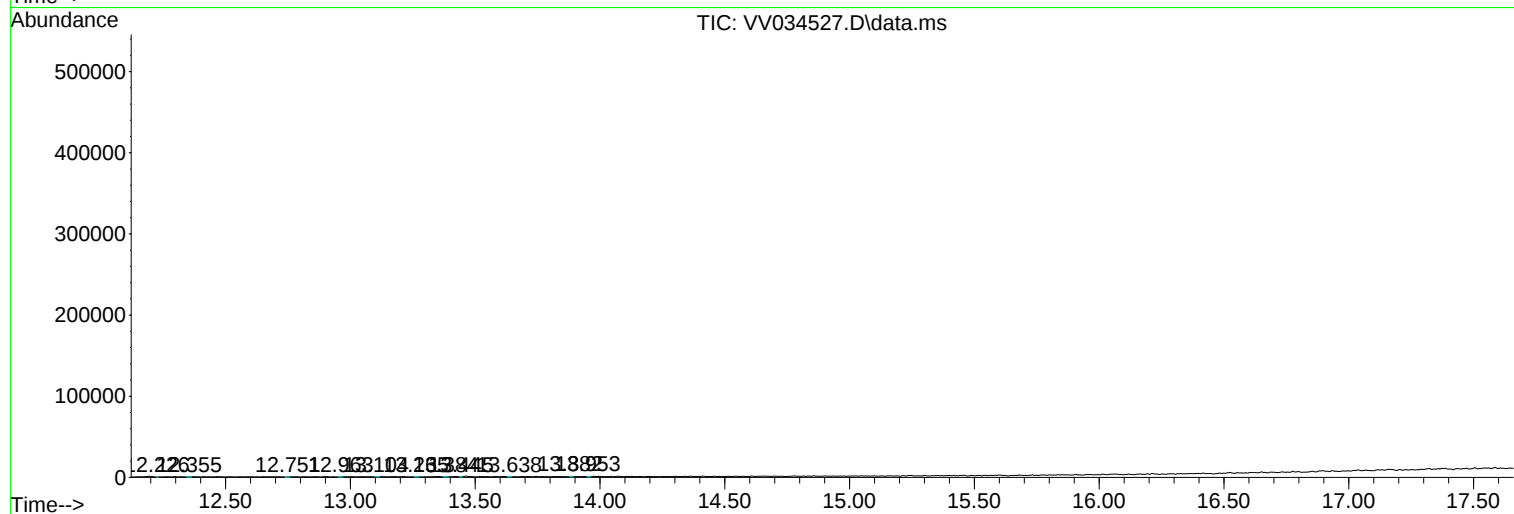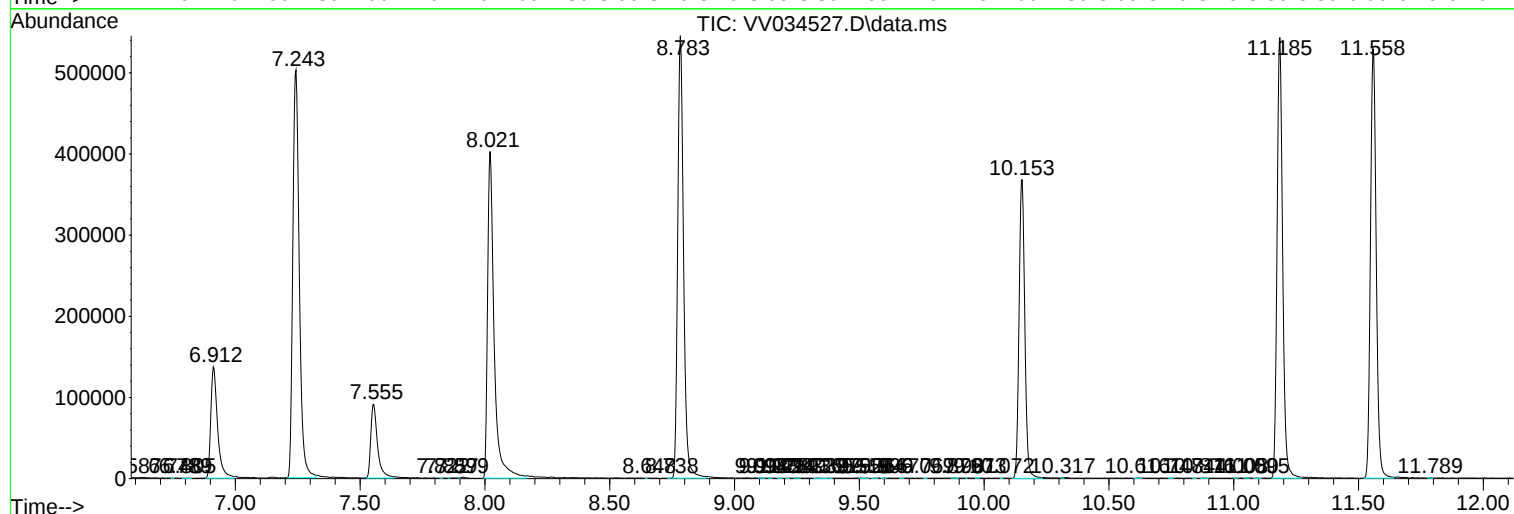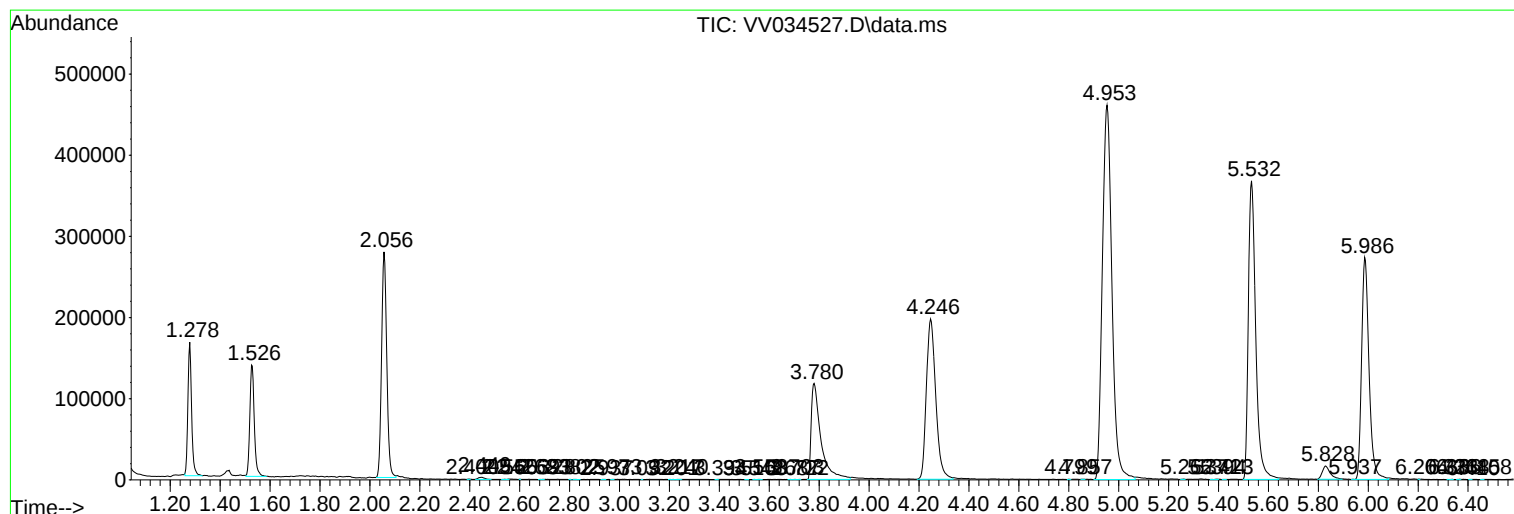

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034527.D
Acq On : 08 Mar 2024 13:27
Operator : SY/MD
Sample : P1679-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034527.D
Acq On : 08 Mar 2024 13:27
Operator : SY/MD
Sample : P1679-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
