
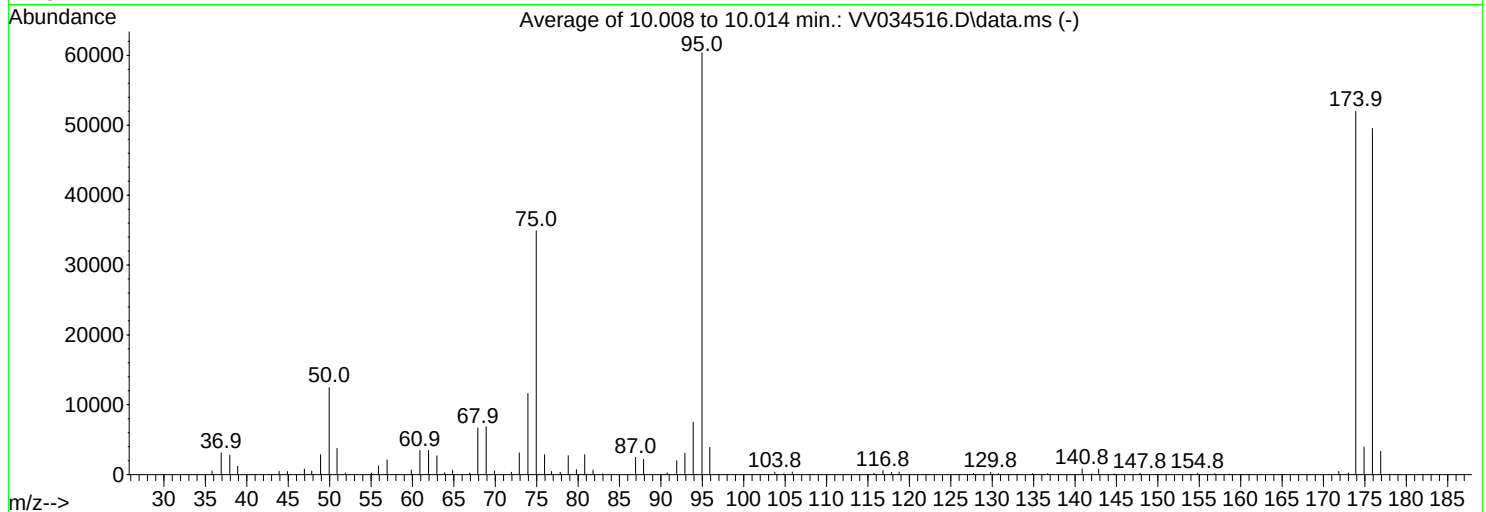


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030824\
Data File : VV034516.D
Acq On : 08 Mar 2024 08:25
Operator : SY/MD
Sample : BFB265
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB265

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Fri Mar 08 23:17:44 2024

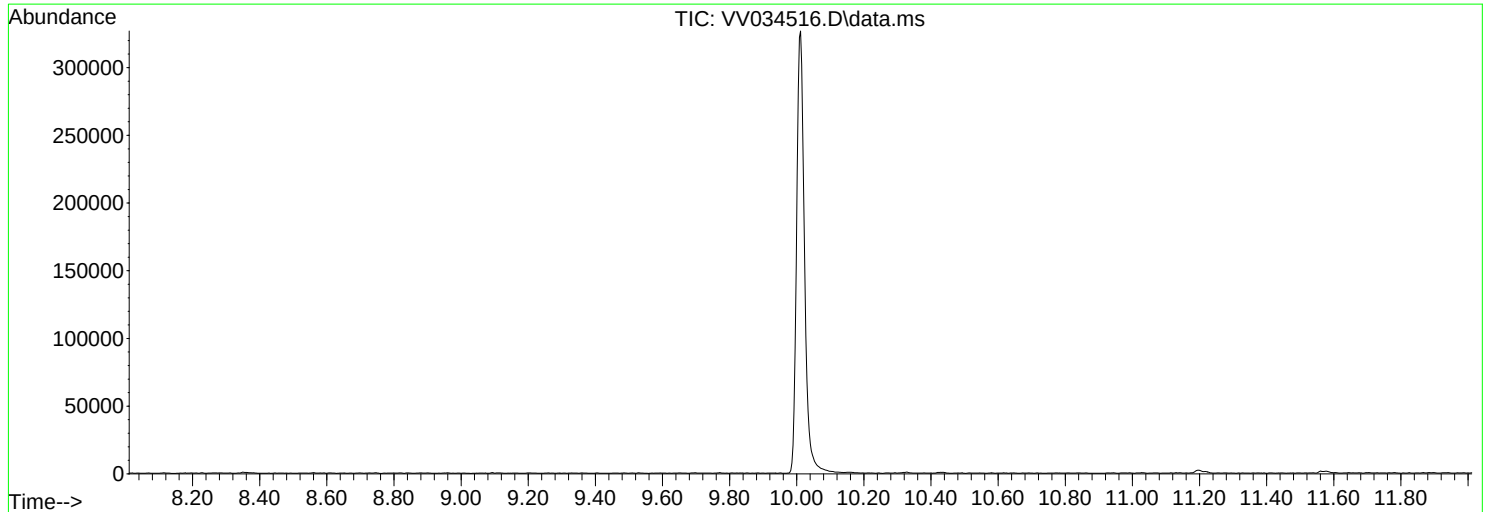

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	12489	PASS
75	95	30	80	57.8	34888	PASS
95	95	100	100	100.0	60365	PASS
96	95	5	9	6.5	3920	PASS
173	174	0.00	2	0.5	262	PASS
174	95	50	120	86.1	51984	PASS
175	174	5	9	7.6	3964	PASS
176	174	95	105	95.3	49544	PASS
177	176	5	10	6.7	3336	PASS

m/z	Abundance
39.80	303.0
43.80	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
35.80	534.0
36.90	2992.0
37.90	2889.0
38.90	1293.0
39.80	371.0
42.80	122.0
44.00	824.0
44.90	446.0
47.00	683.0
47.80	514.0
48.90	2915.0
49.90	13095.0
50.90	4023.0
51.90	188.0
55.00	324.0
55.90	1327.0
57.00	2115.0
59.90	697.0
60.90	3682.0
61.90	3620.0
62.90	2907.0
63.90	290.0
64.80	714.0
66.90	272.0
67.90	6996.0
68.90	6781.0
69.90	533.0
71.90	352.0
72.90	3351.0
74.00	12124.0
75.00	35296.0
75.90	3067.0
76.80	493.0
77.80	290.0
78.80	2824.0
79.80	747.0
80.80	2888.0
81.80	686.0
83.00	109.0
87.00	2446.0
87.90	2011.0
90.70	276.0
91.90	2037.0
92.90	3158.0
93.90	7800.0
94.90	61176.0
95.90	4046.0
103.70	328.0
104.80	151.0
105.80	386.0
115.70	185.0
116.80	587.0
117.90	346.0
118.70	315.0
127.70	234.0
129.80	396.0
130.70	194.0
134.90	184.0
136.70	122.0
140.80	878.0
142.00	104.0
142.90	670.0
144.70	183.0
147.80	178.0
154.80	208.0
156.80	132.0
158.70	108.0
171.80	534.0
173.00	787.0
173.90	52280.0
174.90	3988.0
175.90	49320.0
176.90	3186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
35.80	529.0
36.90	3207.0
37.90	2937.0
38.90	1226.0
39.80	340.0
44.00	768.0
44.90	448.0
47.00	840.0
47.80	484.0
48.90	2949.0
49.90	12865.0
50.90	3859.0
51.90	253.0
53.00	108.0
55.10	241.0
55.90	1268.0
56.90	2140.0
59.80	675.0
60.90	3546.0
61.90	3572.0
63.00	2768.0
63.90	307.0
64.90	664.0
66.90	269.0
67.90	6877.0
68.90	7043.0
69.90	526.0
71.90	365.0
72.90	3226.0
73.90	11890.0
74.90	36128.0
76.00	2945.0
76.80	471.0
77.90	352.0
78.80	2847.0
79.80	755.0
80.80	2998.0
81.80	661.0
82.90	114.0
87.00	2534.0
87.90	2220.0
90.70	278.0
91.90	2031.0
92.90	3211.0
93.90	7784.0
94.90	62184.0
95.90	4070.0
103.80	393.0
104.80	151.0
105.80	381.0
115.70	226.0
116.80	586.0
117.90	331.0
118.80	404.0
127.70	210.0
129.80	333.0
130.80	176.0
134.80	165.0
136.70	171.0
140.80	835.0
142.00	128.0
142.80	823.0
144.70	152.0
147.80	193.0
154.80	227.0
156.80	141.0
158.60	126.0
170.60	103.0
171.80	480.0
173.90	53720.0
174.90	4086.0
175.90	51144.0
176.90	3463.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
35.80	526.0
36.90	3222.0
38.00	2591.0
38.90	1062.0
39.80	332.0
43.90	632.0
44.90	463.0
46.90	857.0
47.90	485.0
48.90	2701.0
50.00	11506.0
50.90	3409.0
51.90	265.0
52.90	102.0
55.00	131.0
55.90	1094.0
56.90	2091.0
57.80	106.0
59.80	659.0
60.90	3153.0
62.00	3179.0
63.00	2401.0
63.90	304.0
64.90	558.0
66.90	238.0
67.90	6181.0
68.90	6801.0
69.90	517.0
72.00	336.0
72.90	2788.0
73.90	10812.0
74.90	33240.0
76.00	2592.0
76.80	423.0
77.90	414.0
78.80	2533.0
79.80	665.0
80.80	2740.0
81.80	572.0
82.90	131.0
86.90	2430.0
87.90	2301.0
90.80	265.0
91.90	1879.0
92.90	2831.0
93.90	6957.0
95.00	57736.0
95.90	3644.0
103.80	417.0
104.90	129.0
105.90	325.0
115.70	246.0
116.80	550.0
117.80	315.0
118.80	444.0
127.80	165.0
129.80	277.0
130.80	122.0
134.80	124.0
136.70	213.0
140.90	755.0
142.00	106.0
142.80	887.0
143.90	109.0
147.90	197.0
154.80	210.0
156.90	120.0
171.90	396.0
173.90	49952.0
174.90	3819.0
175.90	48168.0
176.90	3358.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265