


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014781.D
Acq On : 09 Mar 2020 17:00
Operator : SY/MD
Sample : L1834-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL3

Manual Integrations
APPROVED

MMDadoda
3/11/2020 9:41:31 AM

Quant Time: Mar 10 16:45:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 10 14:44:37 2020
Response via : Initial Calibration

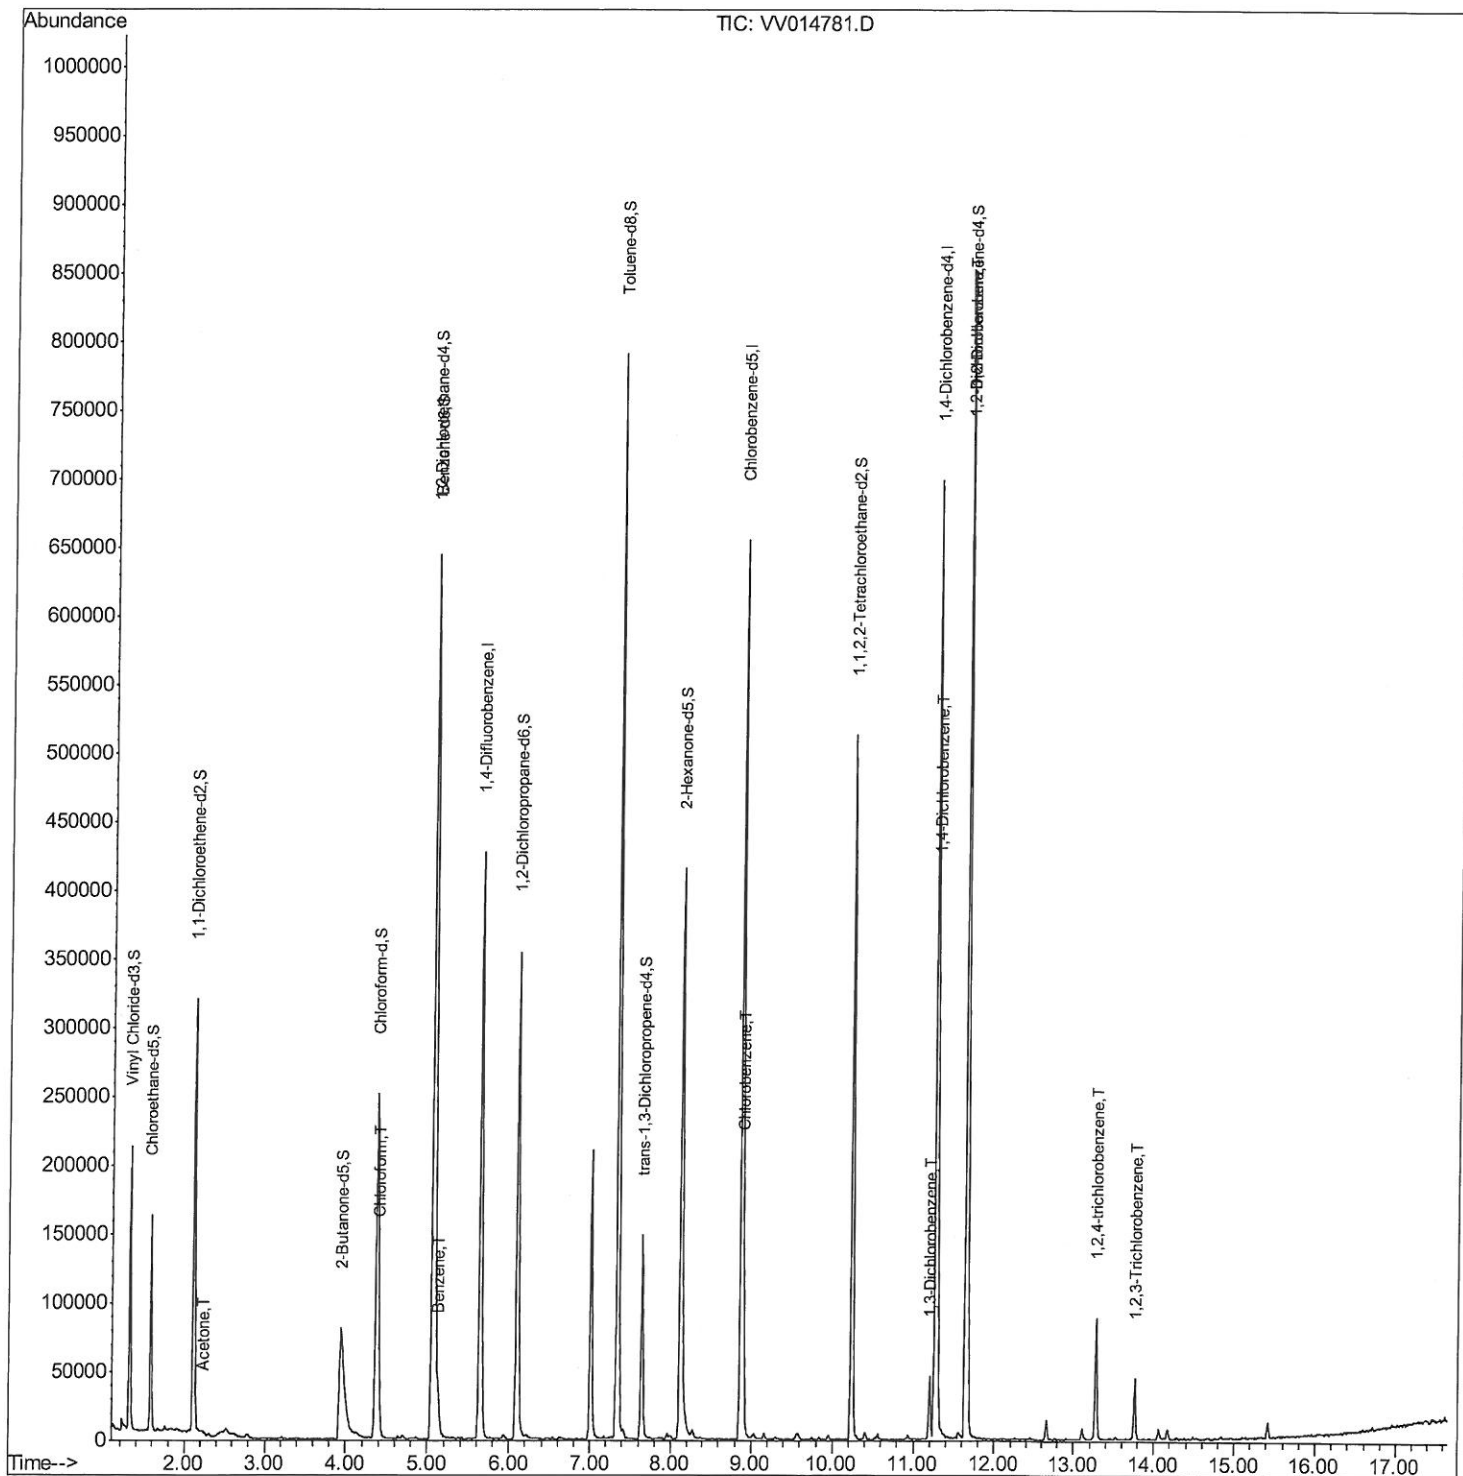

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014781.D
 Acq On : 09 Mar 2020 17:00
 Operator : SY/MD
 Sample : L1834-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL3

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:31 AM

Quant Time: Mar 10 14:49:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

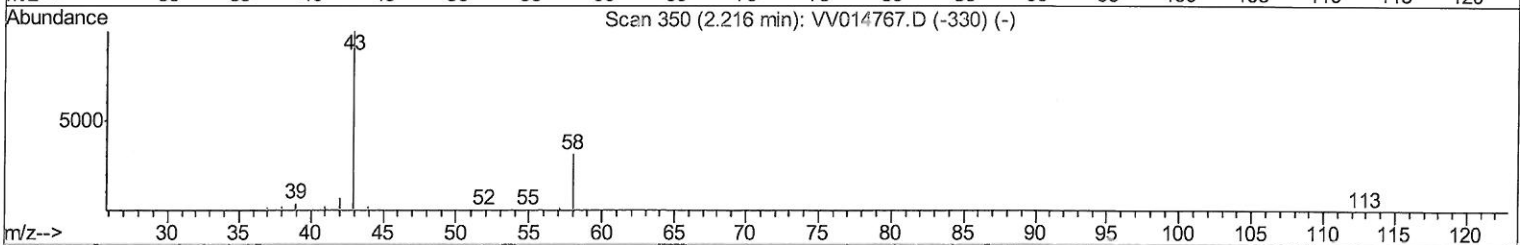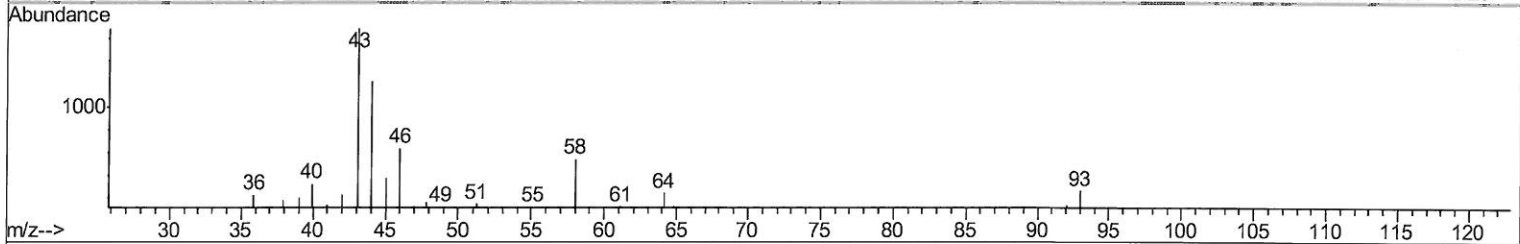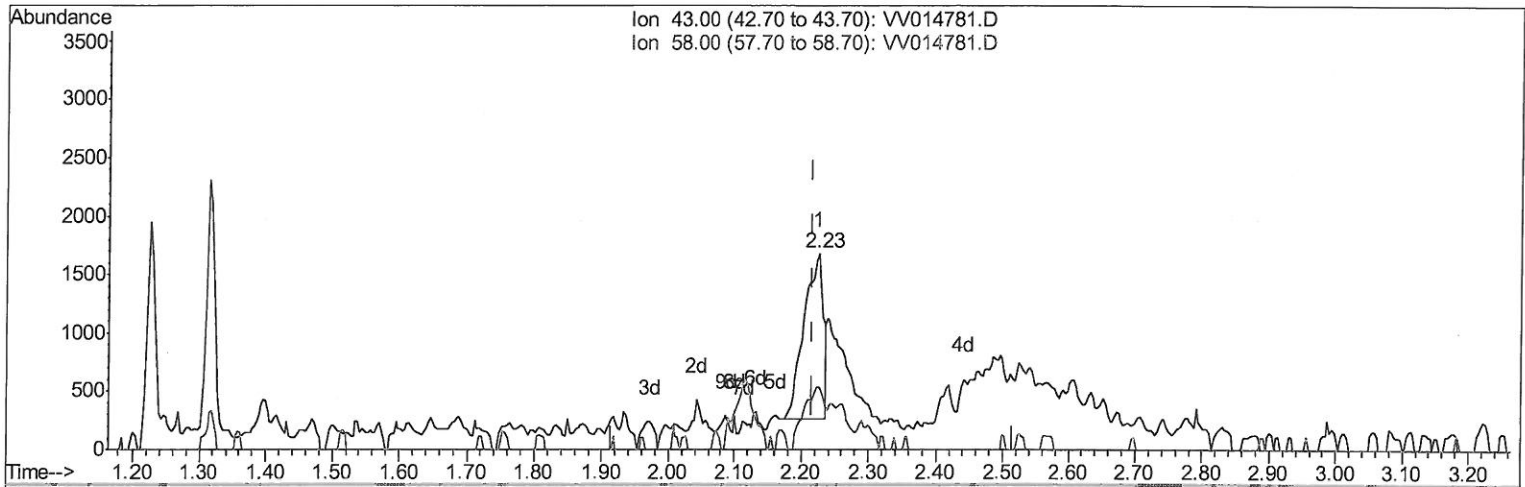

TIC: VV014781.D

(13) Acetone (T)

2.225min (+0.010) 1.82ug/L

response 2826

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	7.22
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014781.D
 Acq On : 09 Mar 2020 17:00
 Operator : SY/MD
 Sample : L1834-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0DL3

Manual Integrations
APPROVED

MMDadoda
 3/11/2020 9:41:31 AM

Quant Time: Mar 10 14:49:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

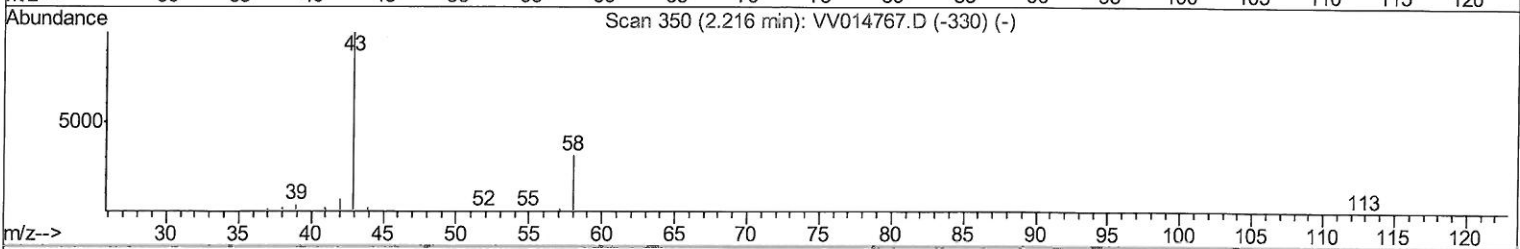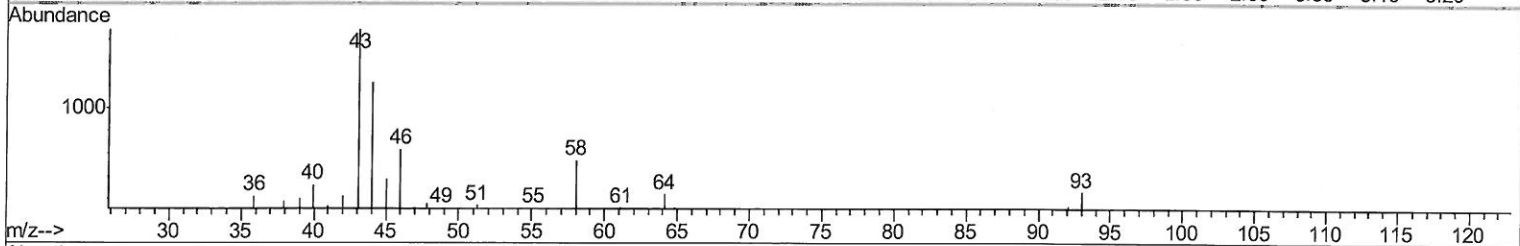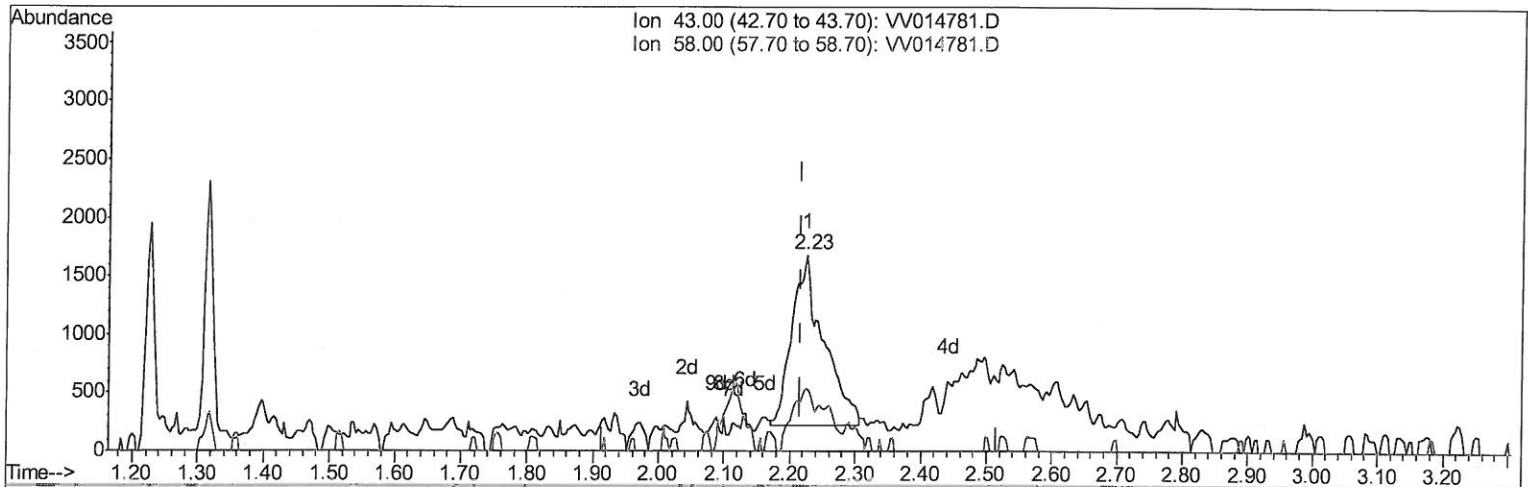

TIC: VV014781.D

(13) Acetone (T)

2.225min (+0.010) 3.17ug/L m

response 4912

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	4.15
0.00	0.00	0.00
0.00	0.00	0.00

7 MLD
3/11/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014781.D
 Acq On : 09 Mar 2020 17:00
 Operator : SY/MD
 Sample : L1834-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 C0DL3

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:31 AM

Quant Time: Mar 10 16:45:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	368255	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	358637	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	178909	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	132733	53.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.52%
7) Chloroethane-d5	1.58	69	105959	53.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.56%
11) 1,1-Dichloroethene-d2	2.12	63	163811	39.56	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.12%
21) 2-Butanone-d5	3.94	46	211191	113.62	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.62%
24) Chloroform-d	4.38	84	261824	55.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.96%
26) 1,2-Dichloroethane-d4	5.06	65	176457	55.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.10%
32) Benzene-d6	5.08	84	552237	58.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.64%
36) 1,2-Dichloropropane-d6	6.10	67	172338	54.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	109.82%
41) Toluene-d8	7.34	98	522749	56.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.72%
43) trans-1,3-Dichloropropene-	7.64	79	83943	54.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	109.56%
47) 2-Hexanone-d5	8.12	63	164257	117.87	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	117.87%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	238131	55.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	110.32%
64) 1,2-Dichlorobenzene-d4	11.65	152	209841	59.18	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.36%

Target Compounds

13) Acetone	2.23	43	4912m	3.17	ug/L	Qvalue, MO
25) Chloroform	4.41	83	6974	1.39	ug/L	91
33) Benzene	5.13	78	34468	3.32	ug/L	100
51) Chlorobenzene	8.90	112	56228	7.62	ug/L	100
62) 1,3-Dichlorobenzene	11.20	146	19563	3.38	ug/L	97
63) 1,4-Dichlorobenzene	11.29	146	82741	14.20	ug/L	99
65) 1,2-Dichlorobenzene	11.66	146	76314	13.25	ug/L	99
68) 1,2,4-trichlorobenzene	13.28	180	27250	6.63	ug/L	97
70) 1,2,3-Trichlorobenzene	13.77	180	14275	3.48	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed