


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014783.D
Acq On : 09 Mar 2020 17:49
Operator : SY/MD
Sample : L1835-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DJ6

Manual Integrations
APPROVED

MMDadoda
3/11/2020 9:41:35 AM

Quant Time: Mar 10 16:54:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 10 14:44:37 2020
Response via : Initial Calibration

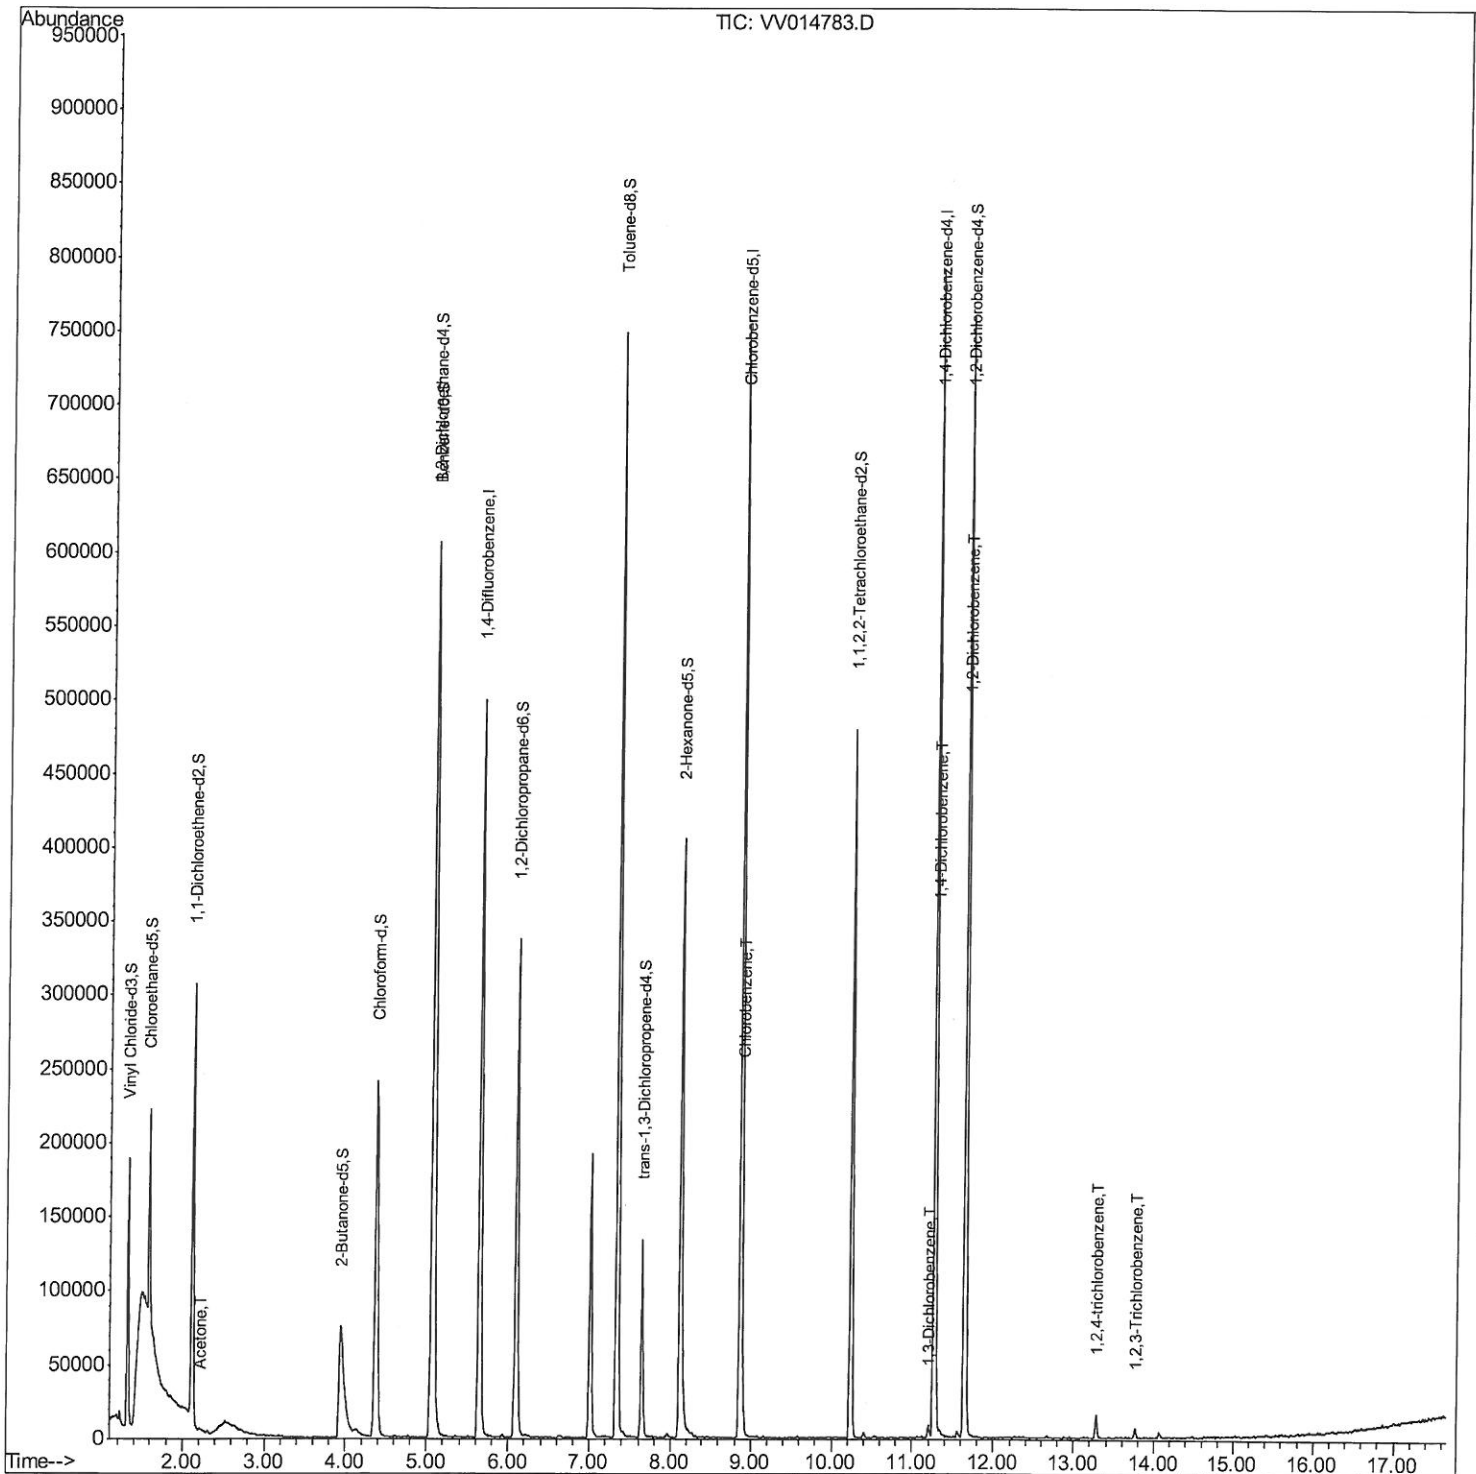

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
Data File : VV014783.D
Acq On : 09 Mar 2020 17:49
Operator : SY/MD
Sample : L1835-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DJ6

Manual Integrations
APPROVED

MMDadoda
3/11/2020 9:41:35 AM

Quant Time: Mar 10 14:49:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 10 14:44:37 2020
Response via : Initial Calibration

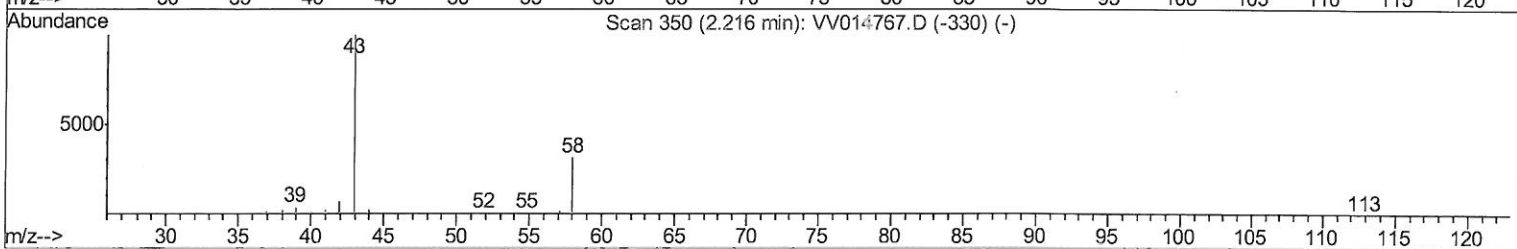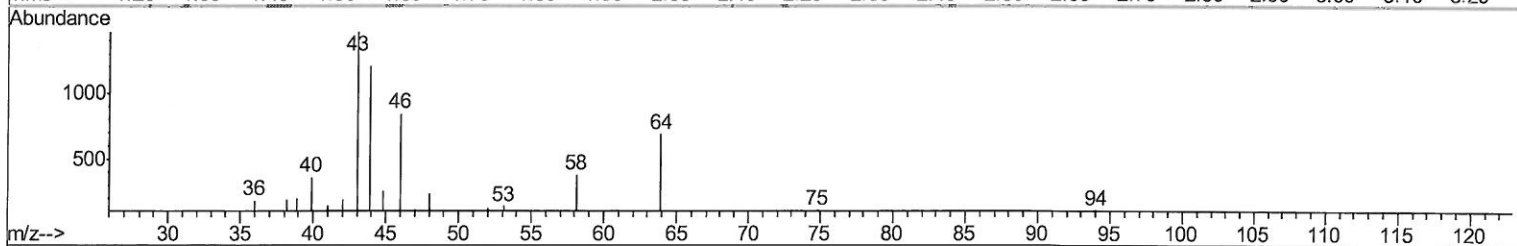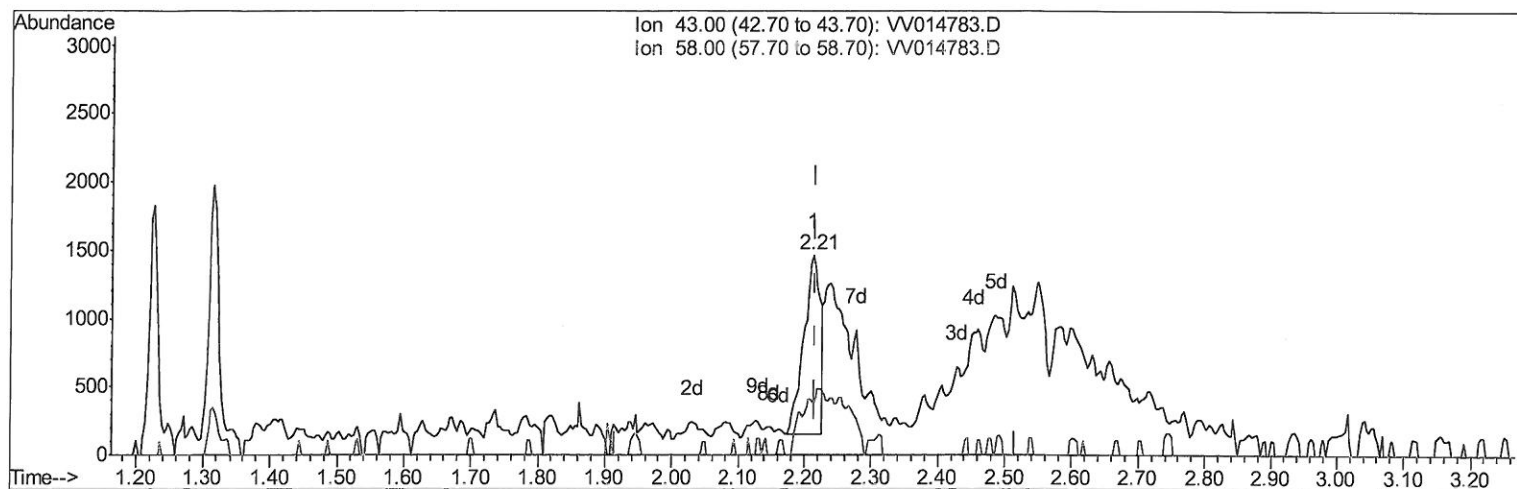

TIC: VV014783.D

(13) Acetone (T)

2.212min (-0.003) 1.23ug/L

response 2235

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	5.82
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014783.D
 Acq On : 09 Mar 2020 17:49
 Operator : SY/MD
 Sample : L1835-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ6

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:35 AM

Quant Time: Mar 10 14:49:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

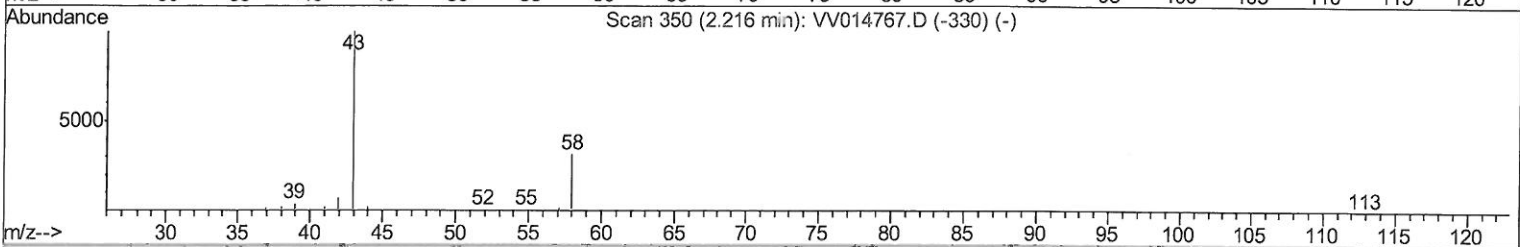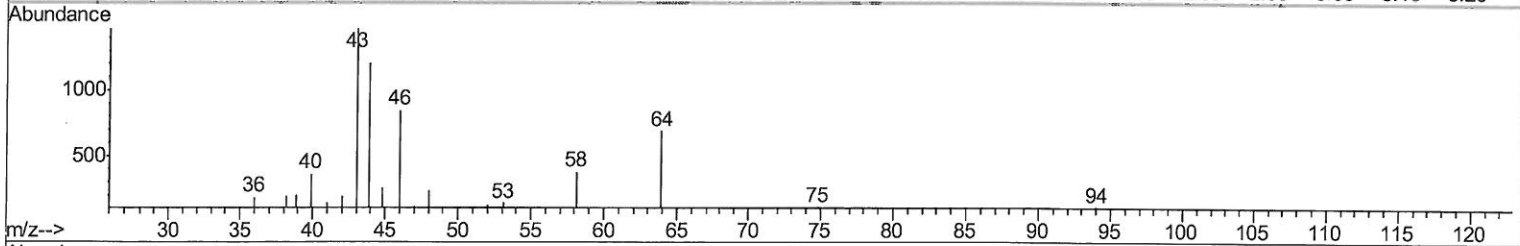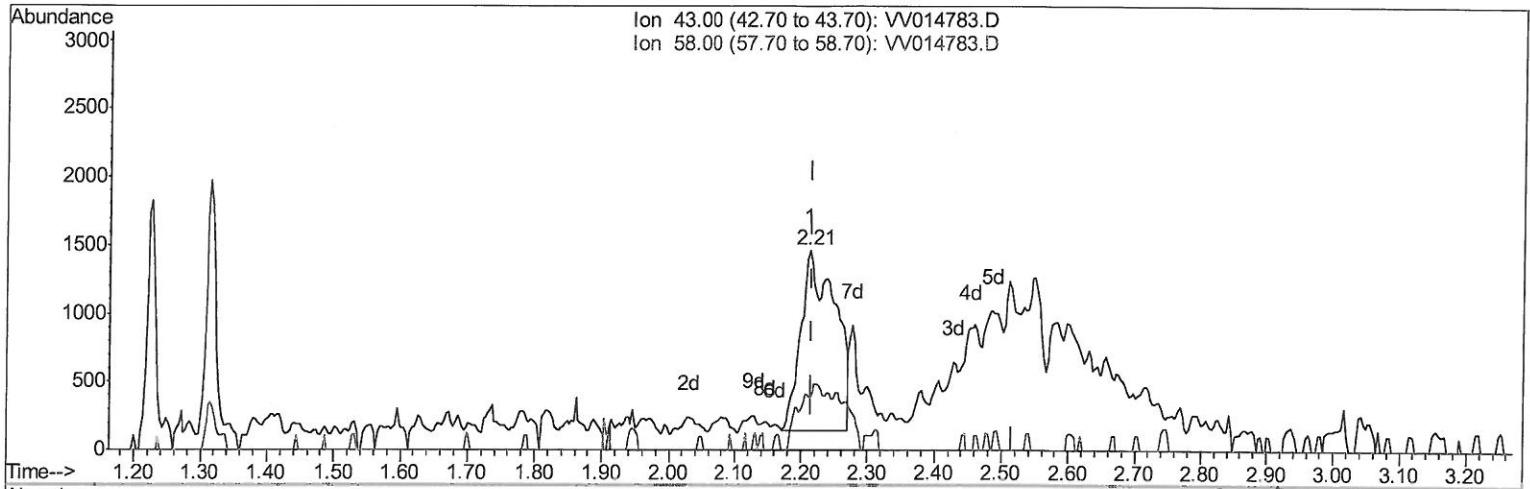

TIC: VV014783.D

(13) Acetone (T)

2.212min (-0.003) 2.56ug/L m

response 4673

Ion	Exp%	Act%
43.00	100	100
58.00	31.10	2.78
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 3/11/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030920\
 Data File : VV014783.D
 Acq On : 09 Mar 2020 17:49
 Operator : SY/MD
 Sample : L1835-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DJ6

Manual Integrations
 APPROVED

MMDadoda
 3/11/2020 9:41:35 AM

Quant Time: Mar 10 16:54:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM030620WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 10 14:44:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	432401	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	415688	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	203867	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	119203	40.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.48%
7) Chloroethane-d5	1.58	69	98349	42.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.02%
11) 1,1-Dichloroethene-d2	2.12	63	151583	31.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.34%
21) 2-Butanone-d5	3.94	46	200107	91.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.69%
24) Chloroform-d	4.38	84	254728	45.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.94%
26) 1,2-Dichloroethane-d4	5.06	65	171256	45.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.00%
32) Benzene-d6	5.08	84	519311	47.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.62%
36) 1,2-Dichloropropane-d6	6.10	67	165411	45.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.94%
41) Toluene-d8	7.34	98	493846	45.94	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.88%
43) trans-1,3-Dichloropropene-	7.64	79	77292	43.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.04%
47) 2-Hexanone-d5	8.12	63	159942	99.02	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.02%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	223409	44.65	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.30%
64) 1,2-Dichlorobenzene-d4	11.65	152	199598	49.40	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.80%

Target Compounds

					Qvalue
13) Acetone	2.21	43	4673m	2.56	ug/L
51) Chlorobenzene	8.90	112	11227	1.31	ug/L
62) 1,3-Dichlorobenzene	11.20	146	3706	0.56	ug/L
63) 1,4-Dichlorobenzene	11.29	146	16024	2.41	ug/L
65) 1,2-Dichlorobenzene	11.67	146	12396	1.89	ug/L
68) 1,2,4-trichlorobenzene	13.28	180	4856	1.04	ug/L #
70) 1,2,3-Trichlorobenzene	13.77	180	1937	0.41	ug/L #

7 m2
 3/11/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed